

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF031119\
 Data File : BF112984.D
 Acq On : 12 Mar 2019 5:16
 Operator : JU/SJ
 Sample : K1817-15
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PST-027-B111-030619

Quant Time: Mar 12 07:45:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 01 15:40:43 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	21935	20.00	ng	-0.01
21) Naphthalene-d8	8.01	136	76643	20.00	ng	-0.01
39) Acenaphthene-d10	9.76	164	50903	20.00	ng	0.00
64) Phenanthrene-d10	11.24	188	127351	20.00	ng	0.00
76) Chrysene-d12	13.86	240	106122	20.00	ng	-0.01
87) Perylene-d12	15.27	264	79284	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	106247	75.35	ng	-0.02
7) Phenol-d6	6.36	99	139468	78.74	ng	-0.01
23) Nitrobenzene-d5	7.29	82	71936	56.16	ng	-0.02
42) 2,4,6-Tribromophenol	10.55	330	61372	113.57	ng	-0.01
45) 2-Fluorobiphenyl	9.09	172	191592	57.20	ng	-0.01
79) Terphenyl-d14	12.82	244	301750	55.12	ng	-0.01
Target Compounds						
50) Dimethylphthalate	9.48	163	15741	4.194	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF031119\
Data File : BF112984.D
Acq On : 12 Mar 2019 5:16
Operator : JU/SJ
Sample : K1817-15
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PST-027-B111-030619

Quant Time: Mar 12 07:45:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 01 15:40:43 2019
Response via : Initial Calibration

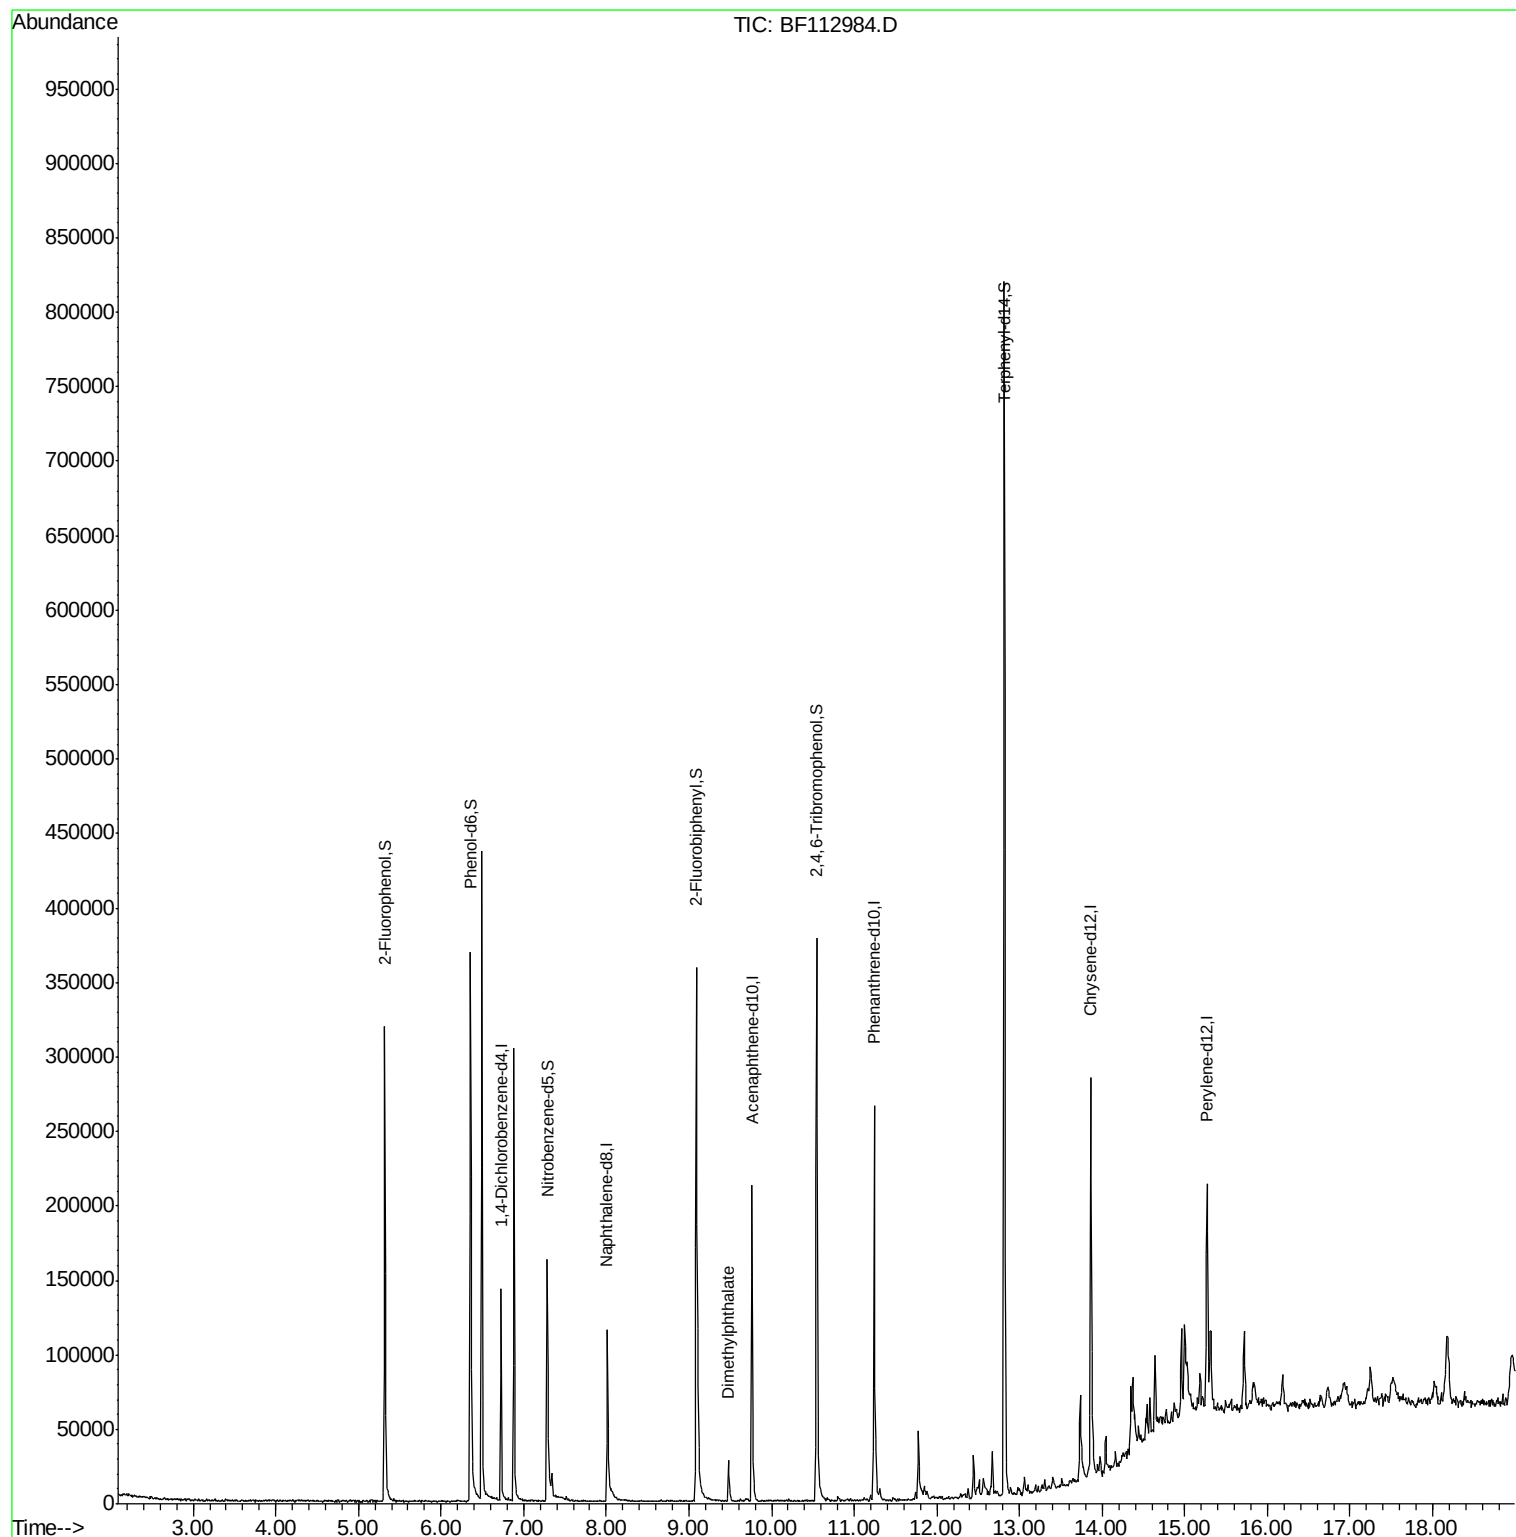


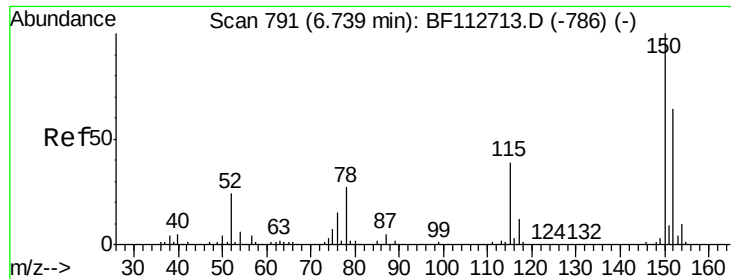




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.73 min Scan# 789
 Delta R.T. -0.01 min
 Lab File: BF112984.D
 Acq: 12 Mar 2019 5:16

Instrument :
 BNA_F
 ClientSampleId :
 PST-027-B111-030619

Tot Ion:152 Resp: 21935
 Ion Ratio Lower Upper
 152 100
 150 156.9 124.2 186.2
 115 59.6 48.2 72.4

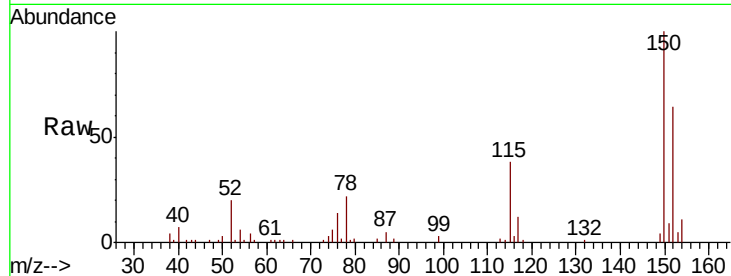


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

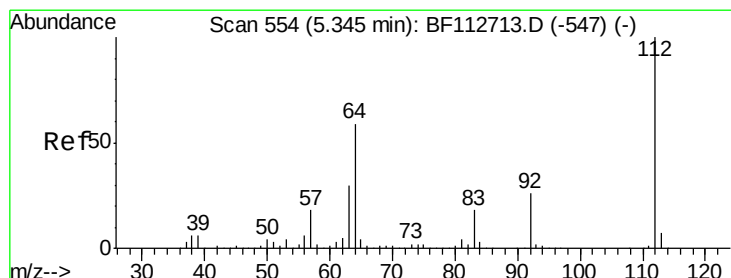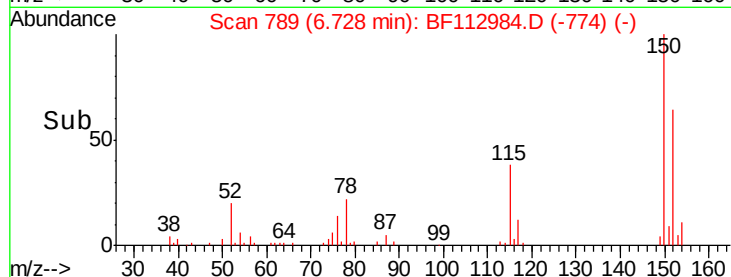
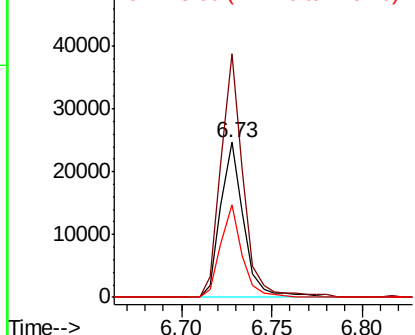



#5
 2-Fluorophenol
 Concen: 75.346 ng
 RT: 5.32 min Scan# 550
 Delta R.T. -0.02 min
 Lab File: BF112984.D
 Acq: 12 Mar 2019 5:16

Tgt Ion:112 Resp: 106247
 Ion Ratio Lower Upper
 112 100
 64 57.0 47.6 71.4
 63 27.5 24.4 36.6

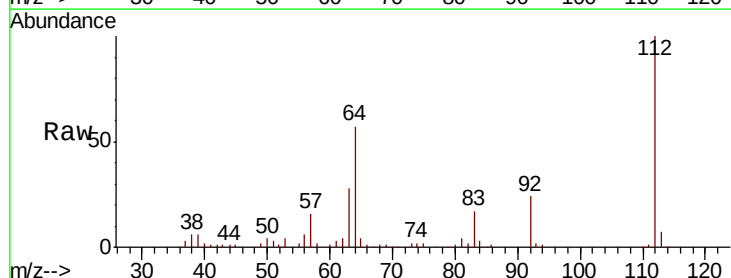

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

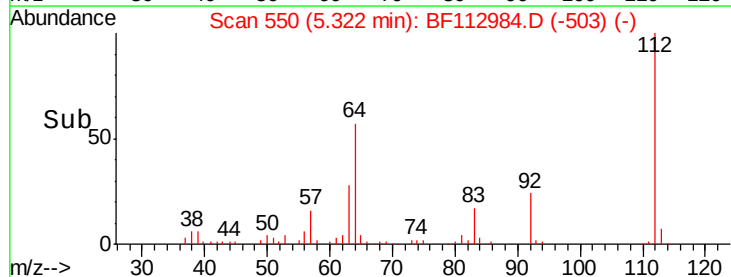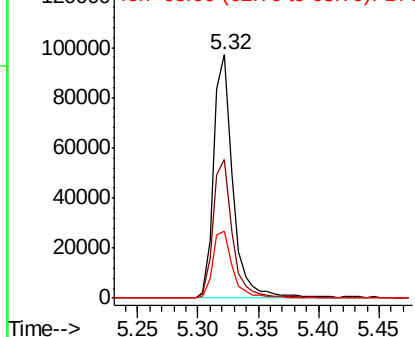

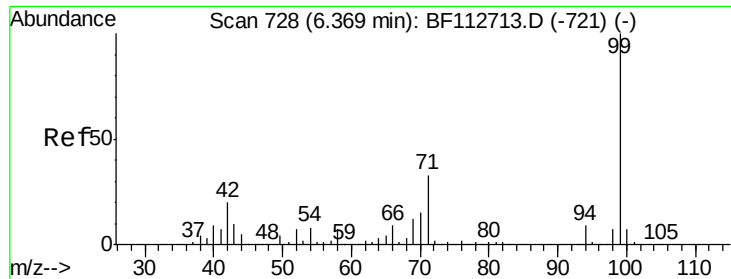

#7

Phenol-d6

Concen: 78.736 ng

RT: 6.36 min Scan# 726

Delta R.T. -0.01 min

Lab File: BF112984.D

Acq: 12 Mar 2019 5:16

Instrument :

BNA_F

ClientSampleId :

PST-027-B111-030619


Tot Ion: 99 Resp: 139468

Ion Ratio Lower Upper




99 100

42 16.9 16.3 24.5

71 29.8 26.2 39.4

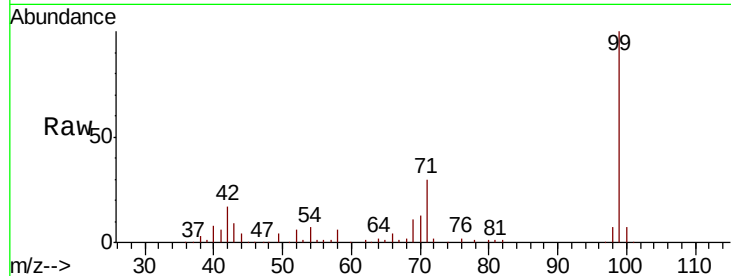

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

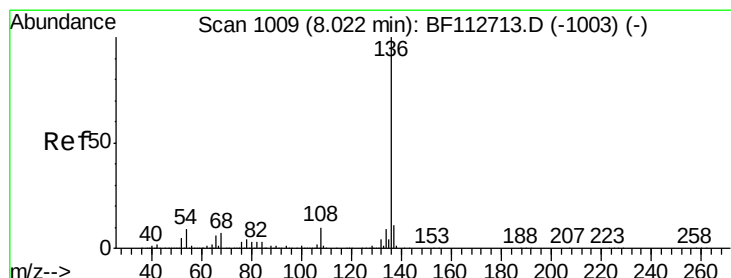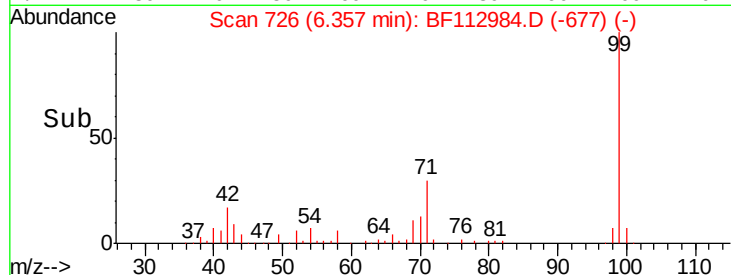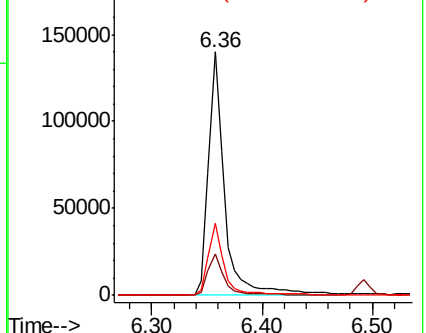

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.01 min Scan# 1007

Delta R.T. -0.01 min

Lab File: BF112984.D

Acq: 12 Mar 2019 5:16

Tgt Ion: 136 Resp: 76643


Ion Ratio Lower Upper

136 100



137 10.6 8.9 13.3


54 7.6 7.3 10.9

68 6.1 5.4 8.2

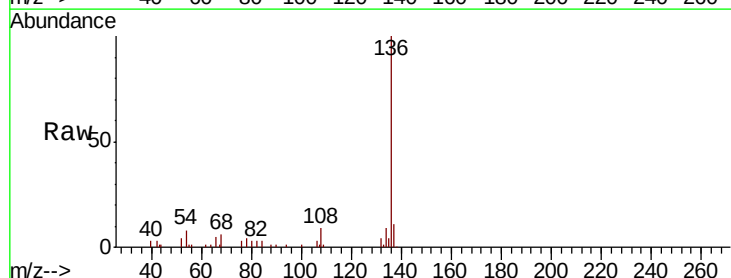

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

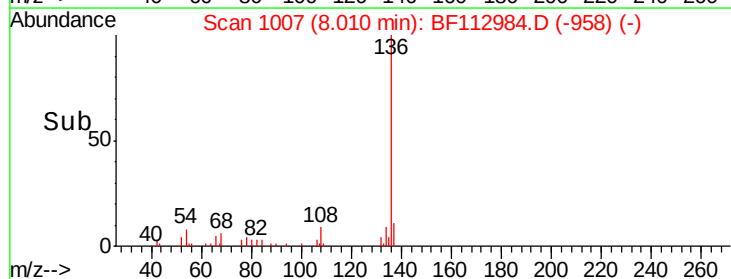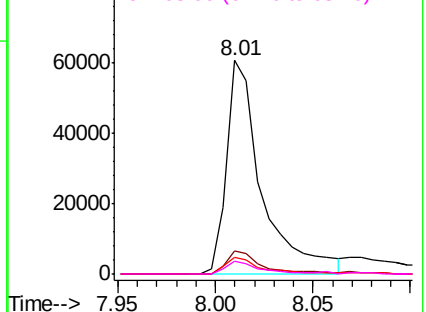


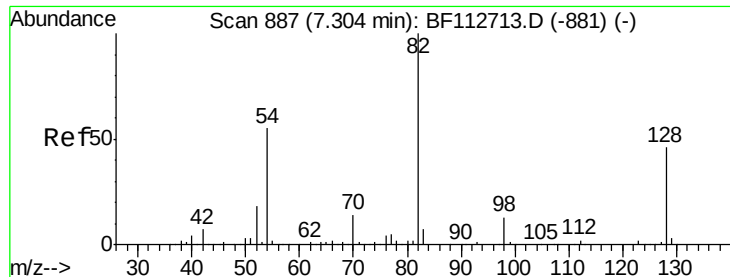




#23
 Nitrobenzene-d5
 Concen: 56.163 ng
 RT: 7.29 min Scan# 884
 Delta R.T. -0.02 min
 Lab File: BF112984.D
 Acq: 12 Mar 2019 5:16

Instrument :
 BNA_F
 ClientSampleId :
 PST-027-B111-030619

Tot Ion: 82 Resp: 71936
 Ion Ratio Lower Upper
 82 100
 128 46.2 36.3 54.5
 54 49.6 43.7 65.5

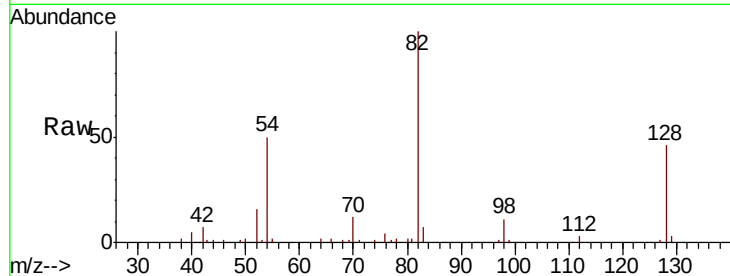


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

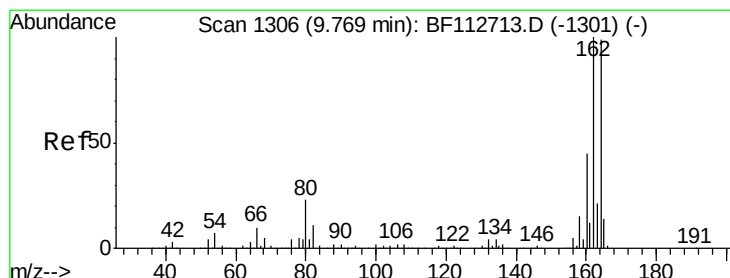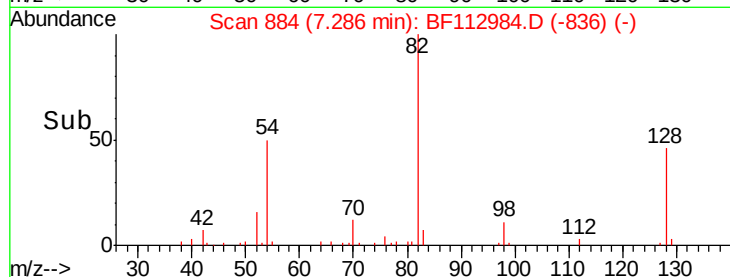
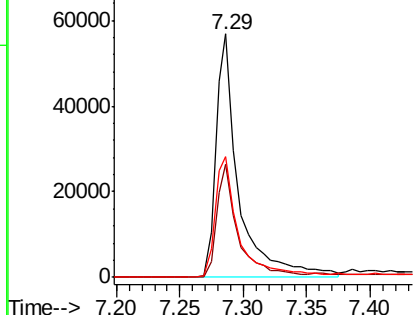



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.76 min Scan# 1305
 Delta R.T. -0.01 min
 Lab File: BF112984.D
 Acq: 12 Mar 2019 5:16

Tgt Ion: 164 Resp: 50903
 Ion Ratio Lower Upper
 164 100
 162 98.4 80.6 120.8
 160 44.3 36.0 54.0

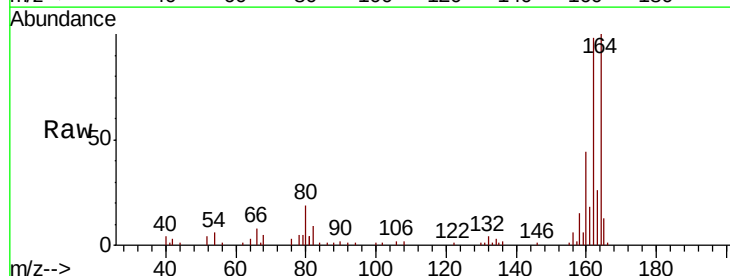

Abundance Ion 164.00 (163.70 to 164.70): BF1
 Ion 162.00 (161.70 to 162.70): BF1
 Ion 160.00 (159.70 to 160.70): BF1

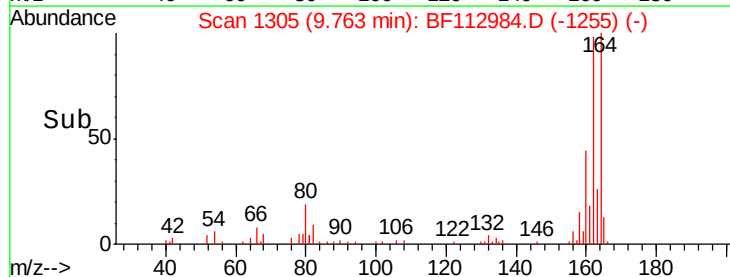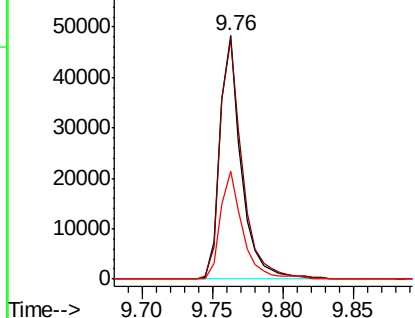


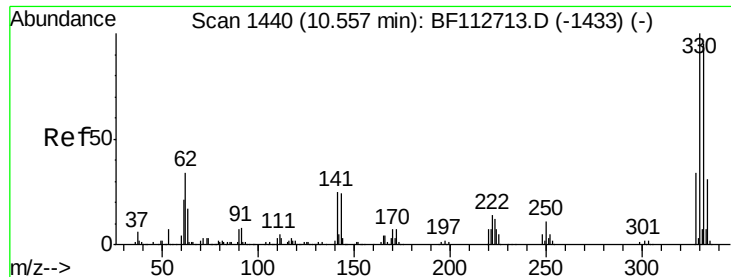




#42
 2,4,6-Tribromophenol
 Concen: 113.568 ng
 RT: 10.55 min Scan# 1438
 Delta R.T. -0.01 min
 Lab File: BF112984.D
 Acq: 12 Mar 2019 5:16

Instrument :
 BNA_F
 ClientSampleId :
 PST-027-B111-030619

Tot Ion:330 Resp: 61372
 Ion Ratio Lower Upper
 330 100
 332 97.1 76.2 114.4
 141 27.7 27.0 40.6

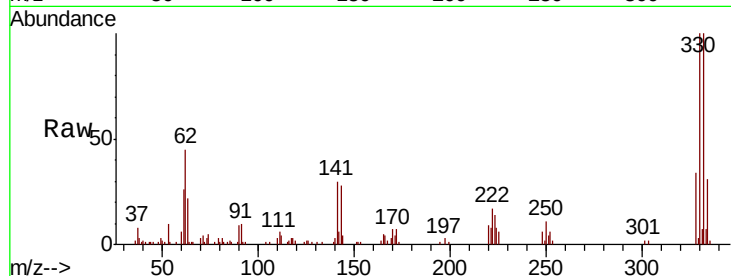


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

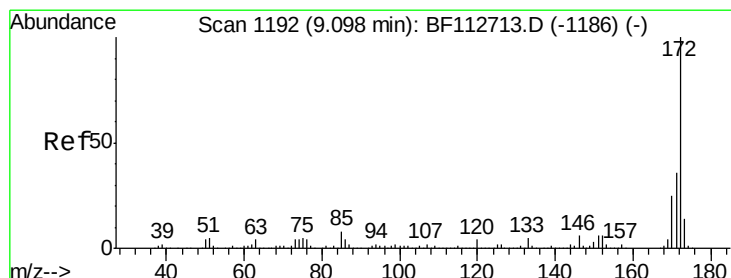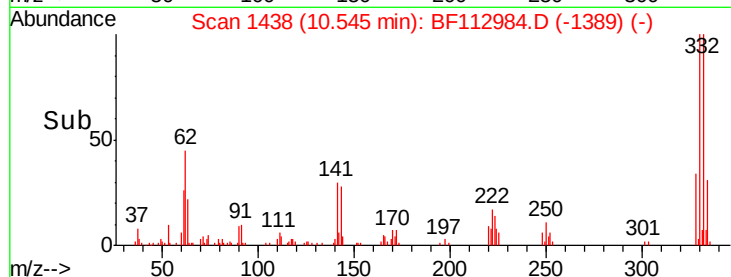
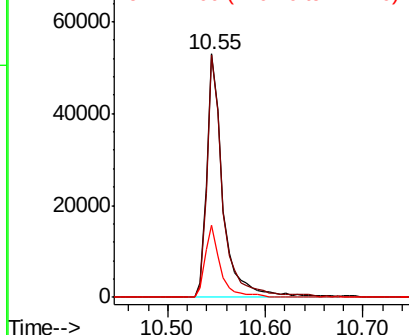



#45
 2-Fluorobiphenyl
 Concen: 57.199 ng
 RT: 9.09 min Scan# 1190
 Delta R.T. -0.01 min
 Lab File: BF112984.D
 Acq: 12 Mar 2019 5:16

Tgt Ion:172 Resp: 191592
 Ion Ratio Lower Upper
 172 100
 171 33.4 29.0 43.4
 170 23.2 20.0 30.0

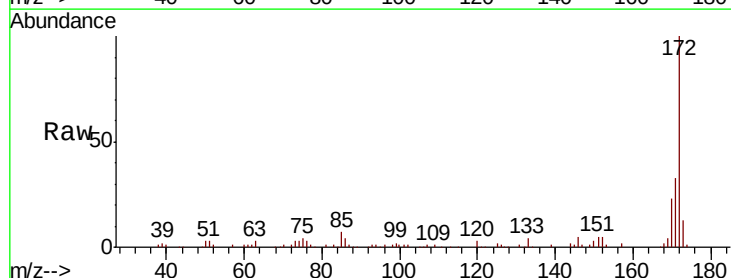

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

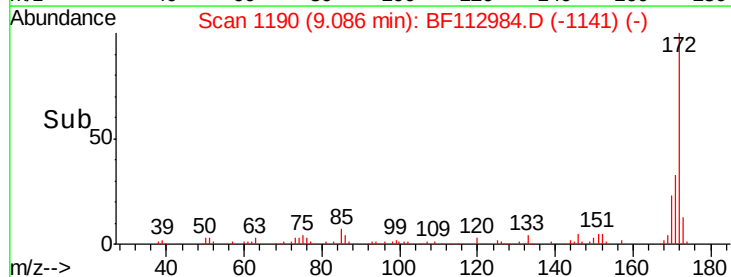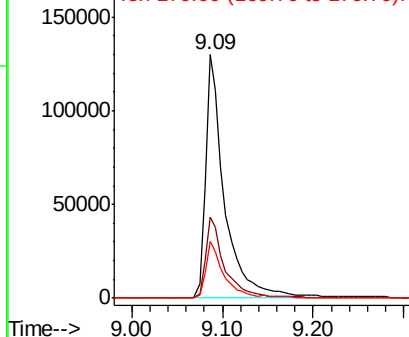


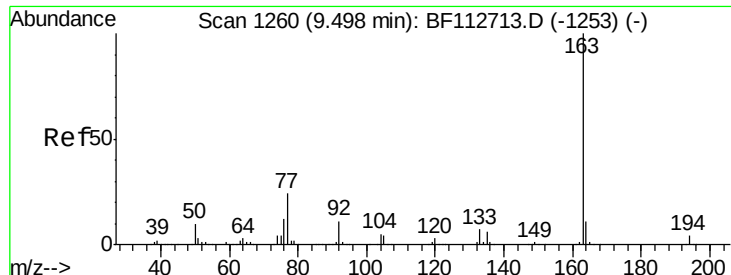




#50
Dimethylphthalate
Concen: 4.194 ng
RT: 9.48 min Scan# 1257
Delta R.T. -0.02 min
Lab File: BF112984.D
Acq: 12 Mar 2019 5:16

Instrument :
BNA_F
ClientSampleId :
PST-027-B111-030619

Tot Ion:163 Resp: 15741
Ion Ratio Lower Upper
163 100
194 3.4 3.0 4.4
164 10.3 8.4 12.6

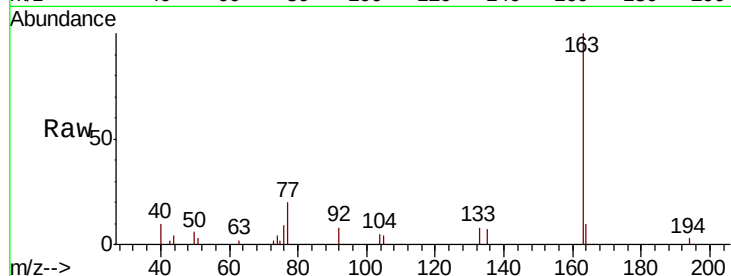


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

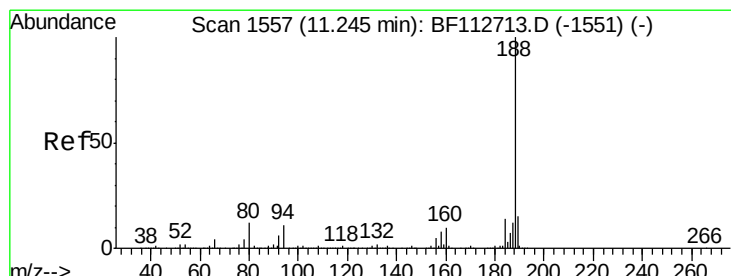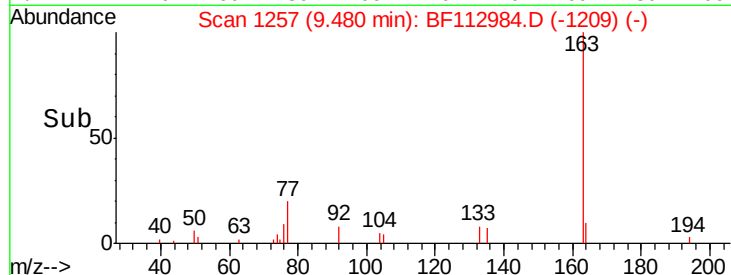
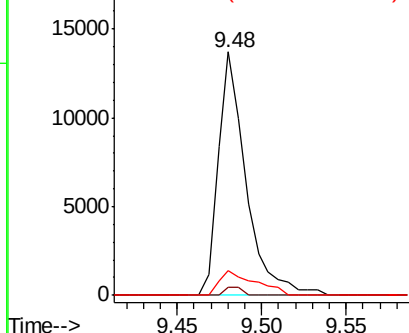



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.24 min Scan# 1556
Delta R.T. -0.01 min
Lab File: BF112984.D
Acq: 12 Mar 2019 5:16

Tgt Ion:188 Resp: 127351
Ion Ratio Lower Upper
188 100
94 9.3 9.0 13.4
80 9.5 9.2 13.8

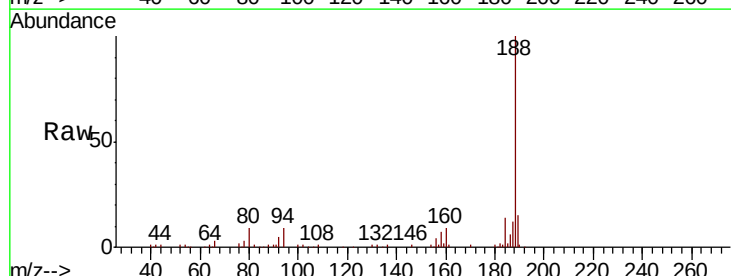

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

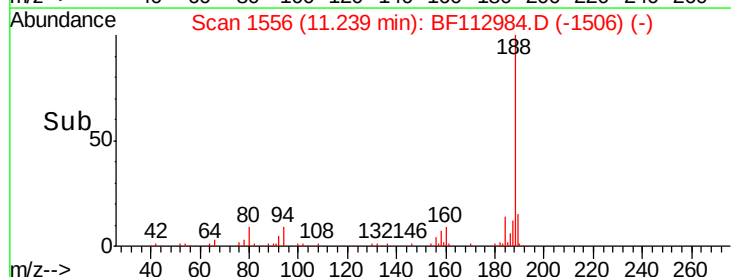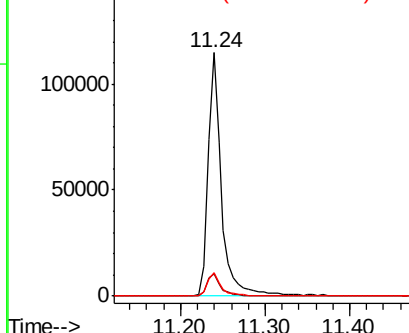

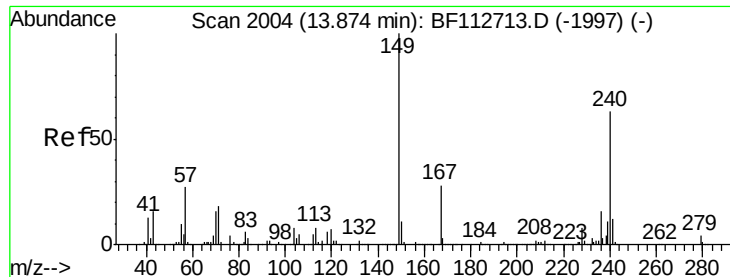

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.86 min Scan# 2002

Delta R.T. -0.01 min

Lab File: BF112984.D

Acq: 12 Mar 2019 5:16

Instrument :

BNA_F

ClientSampleId :

PST-027-B111-030619


Tot Ion:240 Resp: 106122

Ion Ratio Lower Upper

240 100

120 12.6 8.9 13.3




236 25.9 20.7 31.1

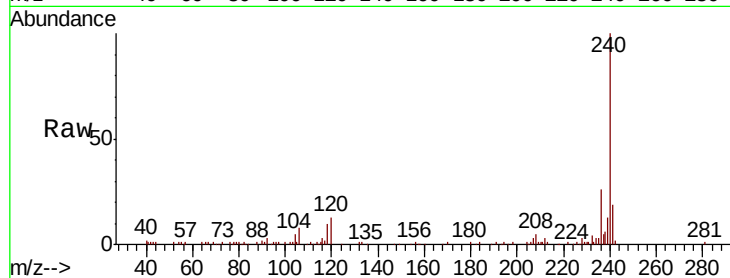

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

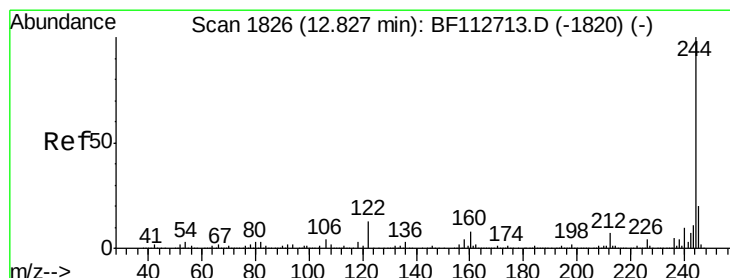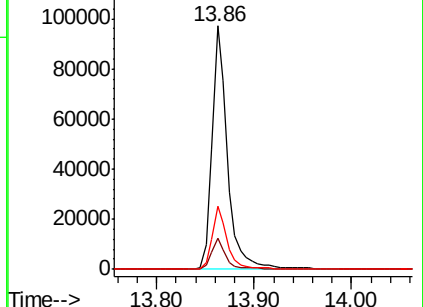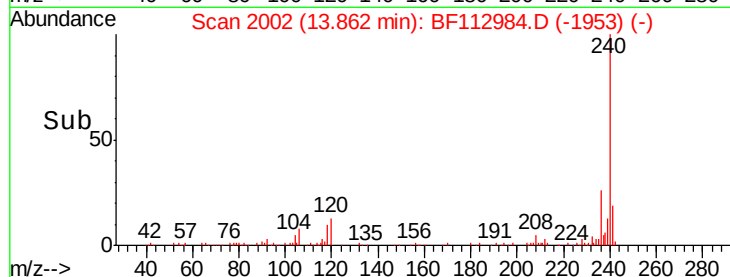

#79

Terphenyl-d14

Concen: 55.120 ng

RT: 12.82 min Scan# 1824

Delta R.T. -0.01 min

Lab File: BF112984.D

Acq: 12 Mar 2019 5:16


Tgt Ion:244 Resp: 301750

Ion Ratio Lower Upper

244 100

212 6.2 5.6 8.4



122 10.6 10.5 15.7

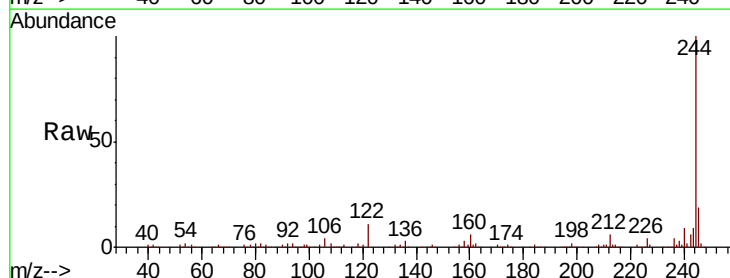


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

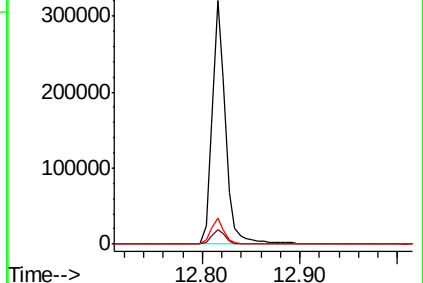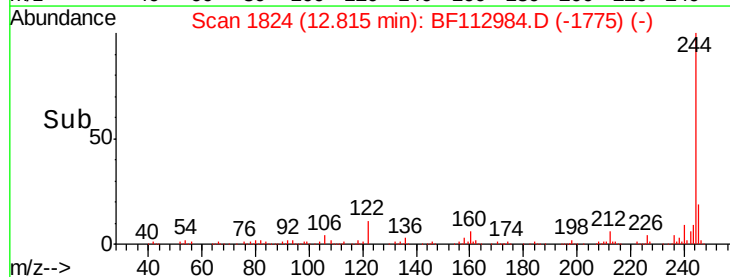


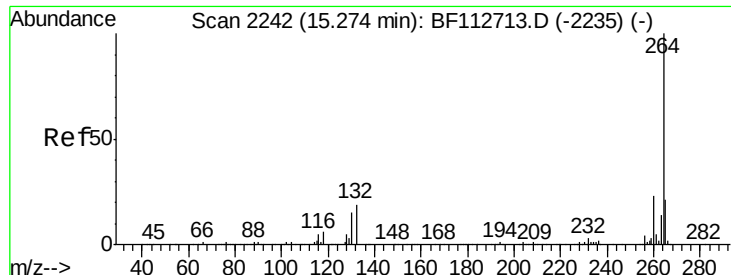

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.27 min Scan# 2241
 Delta R.T. -0.01 min
 Lab File: BF112984.D
 Acq: 12 Mar 2019 5:16

Instrument :
 BNA_F
 ClientSampleId :
 PST-027-B111-030619

Tot Ion:	264	Resp:	79284
Ion	Ratio	Lower	Upper
264	100		
260	24.7	18.7	28.1
265	22.0	17.2	25.8

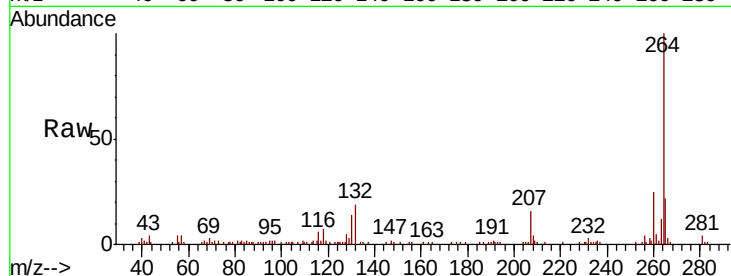

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

