


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031119\
 Data File : BF112953.D
 Acq On : 11 Mar 2019 14:30
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 01 15:40:43 2019

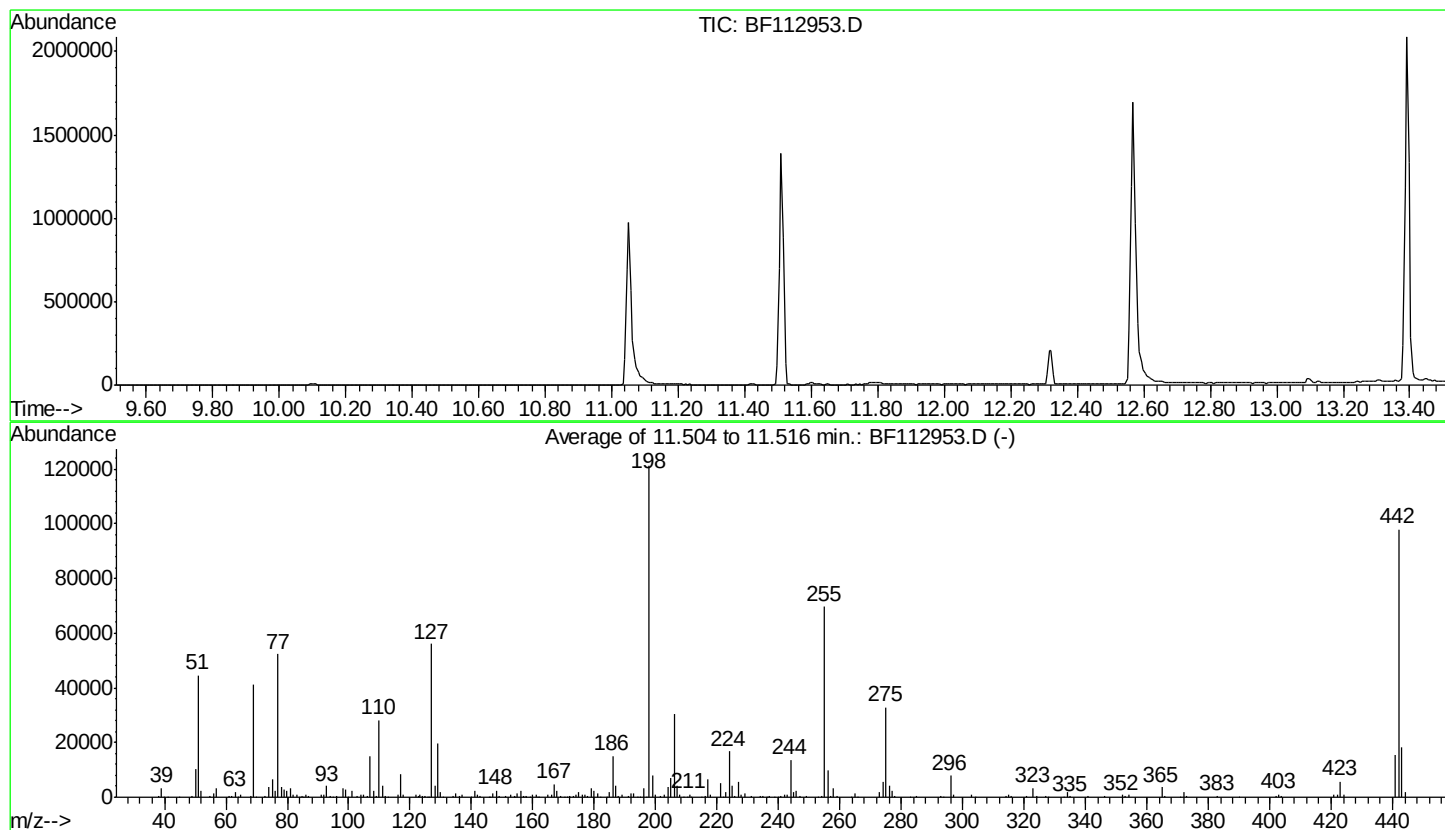

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	44701	PASS
68	69	0.00	2	1.7	701	PASS
69	198	0.00	100	33.9	41152	PASS
70	69	0.00	2	0.4	181	PASS
127	198	10	80	46.2	56040	PASS
197	198	0.00	2	0.2	205	PASS
198	198	100	100	100.0	121237	PASS
199	198	5	9	6.5	7861	PASS
275	198	10	60	27.1	32818	PASS
365	198	1	100	3.0	3671	PASS
441	198	0.01	100	12.6	15230	PASS
442	198	50	100	80.7	97818	PASS
443	442	15	24	18.6	18233	PASS