


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031119\
Data File : BF112978.D
Acq On : 12 Mar 2019 2:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 01 15:40:43 2019

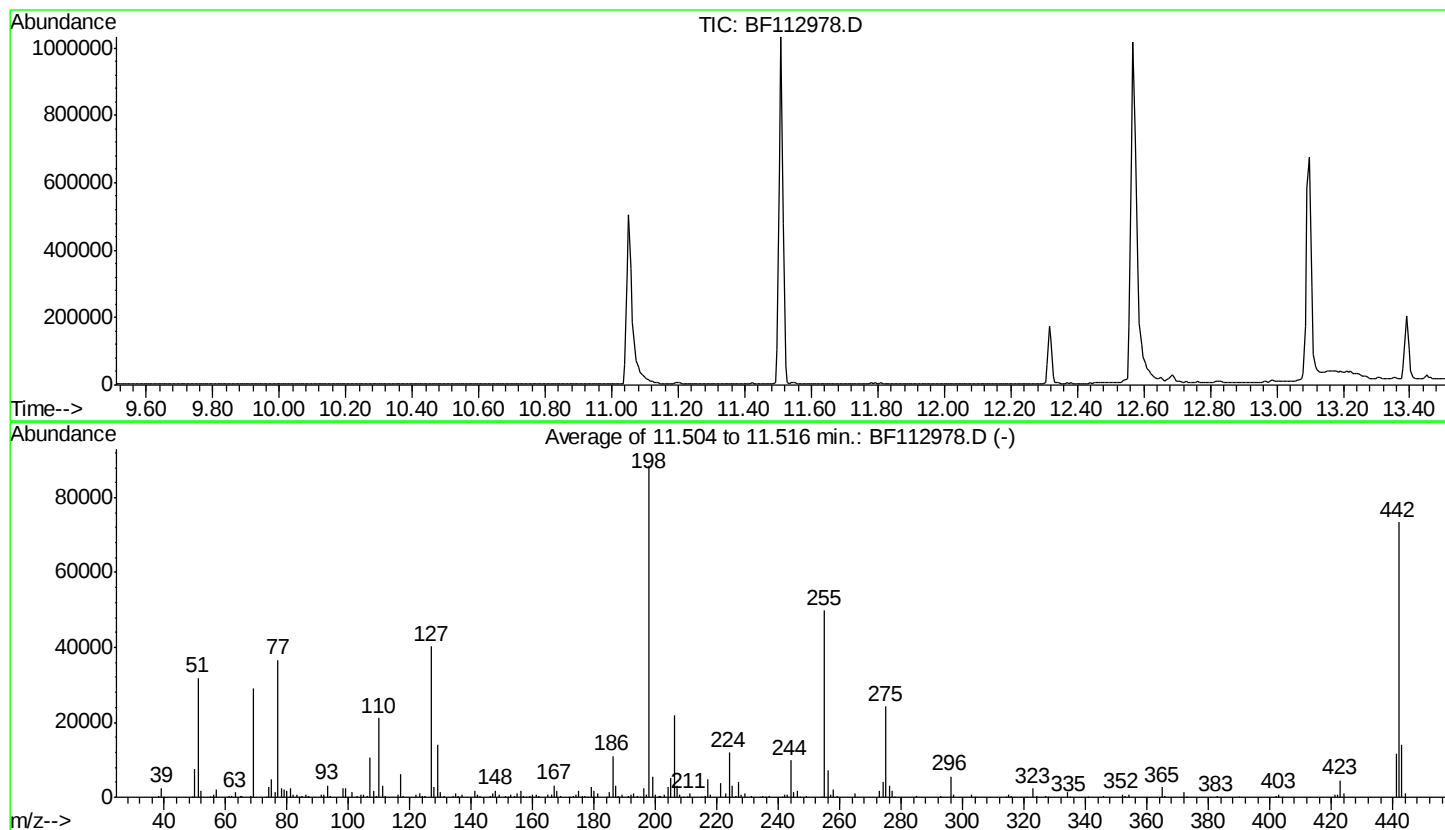

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	31924	PASS
68	69	0.00	2	1.7	501	PASS
69	198	0.00	100	32.8	29025	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.6	40330	PASS
197	198	0.00	2	0.7	613	PASS
198	198	100	100	100.0	88538	PASS
199	198	5	9	6.2	5513	PASS
275	198	10	60	27.4	24248	PASS
365	198	1	100	3.0	2613	PASS
441	198	0.01	100	13.2	11683	PASS
442	198	50	100	82.9	73368	PASS
443	442	15	24	19.0	13966	PASS