
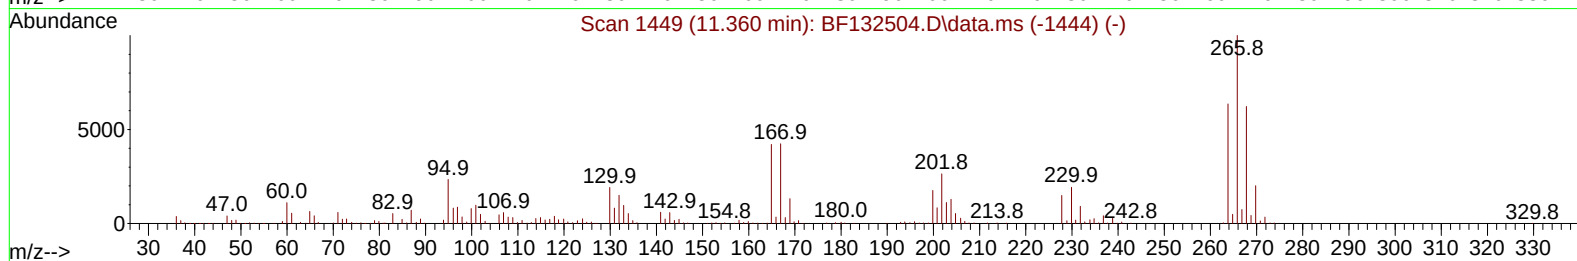
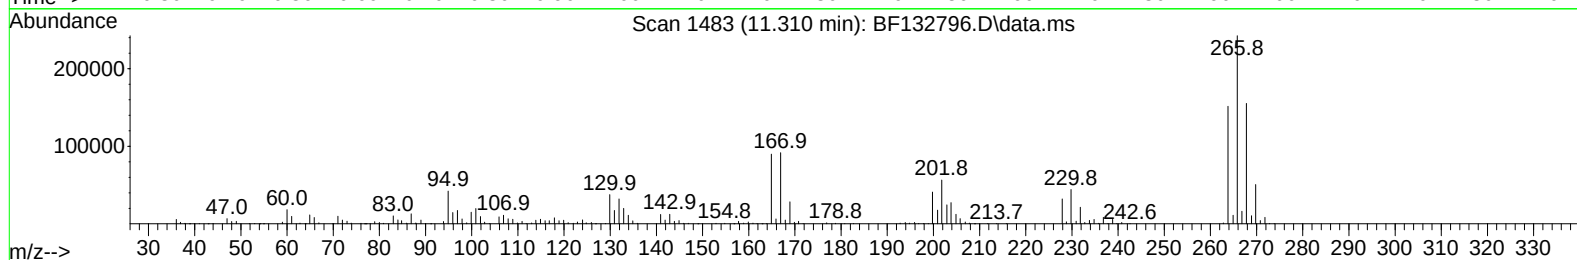


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031523\
Data File : BF132796.D
Acq On : 15 Mar 2023 11:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 12:54:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 14 15:35:42 2023
Response via : Initial Calibration

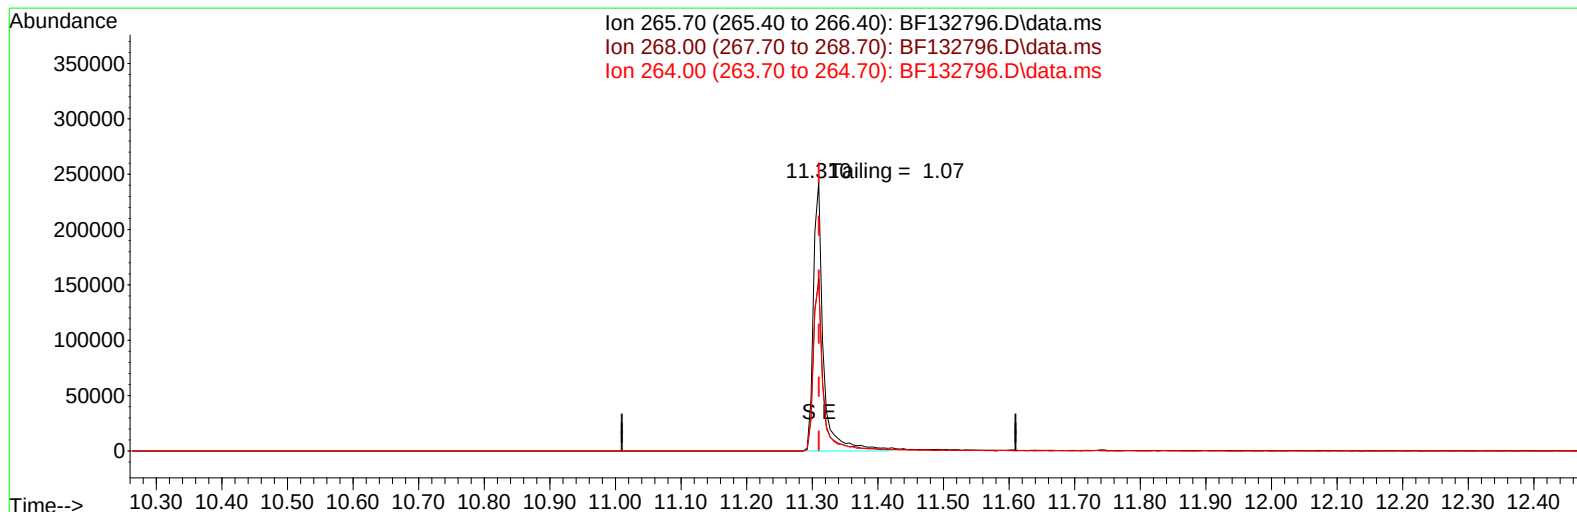

TIC: BF132796.D\data.ms

(70) Pentachlorophenol (C)




11.310min (-0.000) 502082.54 ng

response 263107

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.04
264.00	63.60	62.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031523\
Data File : BF132796.D
Acq On : 15 Mar 2023 11:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 12:54:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 14 15:35:42 2023
Response via : Initial Calibration

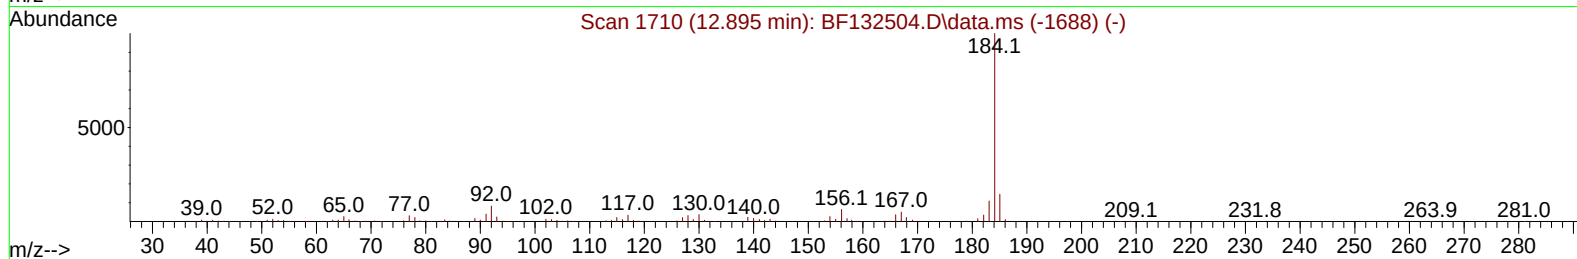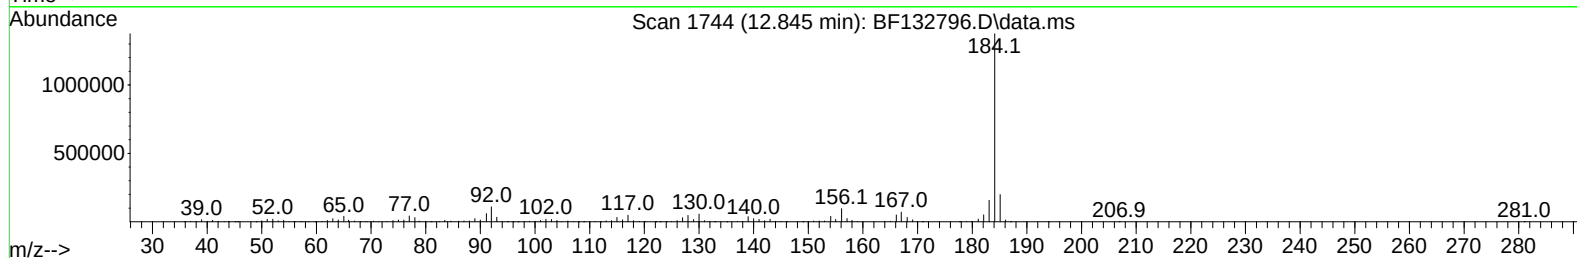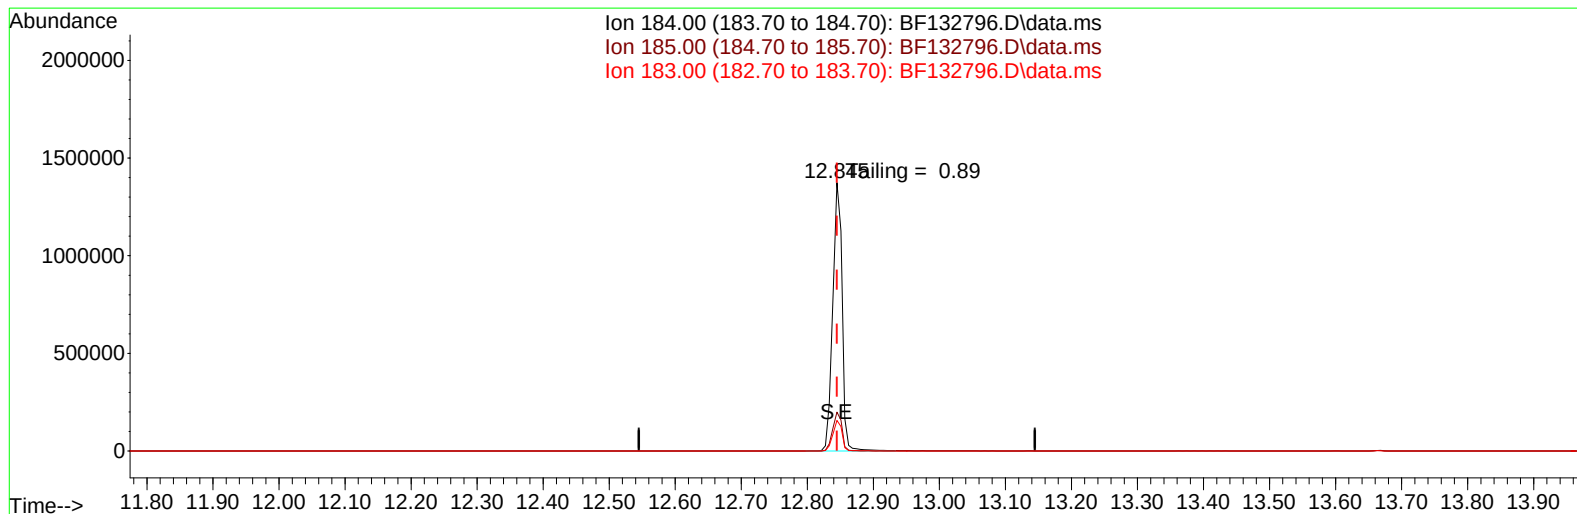

TIC: BF132796.D\data.ms

(77) Benzidine

12.845min (-0.000) 119300.77 ng

response 1362033

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.52
183.00	10.90	11.41
0.00	0.00	0.00