


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031523\
Data File : BF132796.D
Acq On : 15 Mar 2023 11:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 14 15:35:42 2023

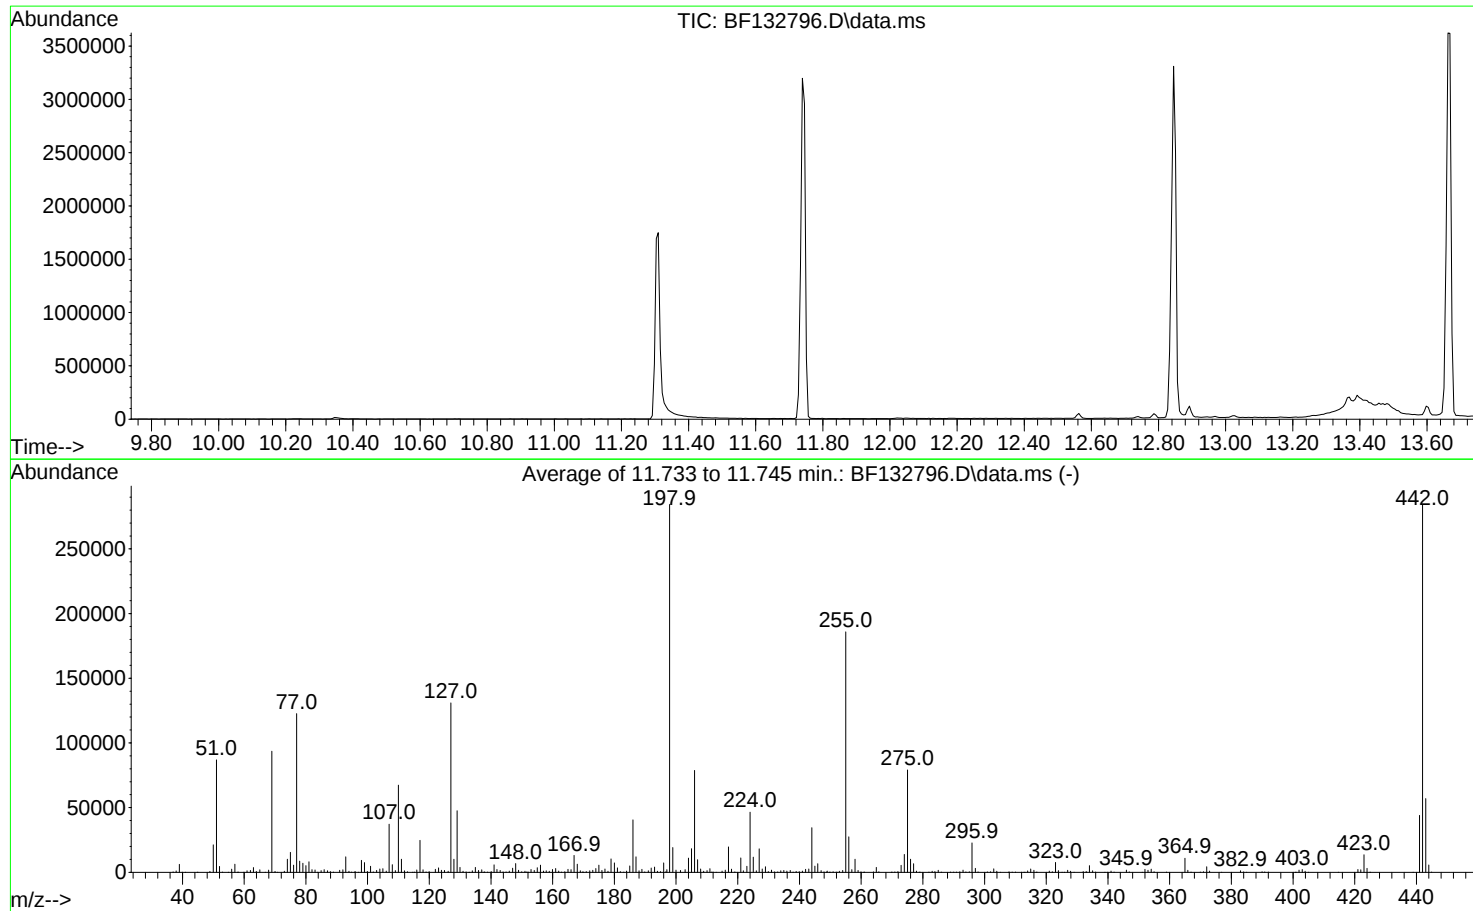




AutoFind: Scans 1555, 1556, 1557; Background Corrected with Scan 1550

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	86931	PASS
68	69	0.00	2	1.8	1688	PASS
69	198	0.00	100	32.9	93547	PASS
70	69	0.00	2	0.7	636	PASS
127	198	10	80	46.0	130931	PASS
197	198	0.00	2	0.7	2071	PASS
198	198	100	100	100.0	284373	PASS
199	198	5	9	6.7	19107	PASS
275	198	10	60	27.8	79112	PASS
365	198	1	100	3.8	10802	PASS
441	198	0.01	100	15.4	43935	PASS
442	442	50	100	100.0	283917	PASS
443	442	15	24	20.1	57011	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031523\
 Data File : BF132796.D
 Acq On : 15 Mar 2023 11:23
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 15 12:54:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 14 15:35:42 2023
 Response via : Initial Calibration

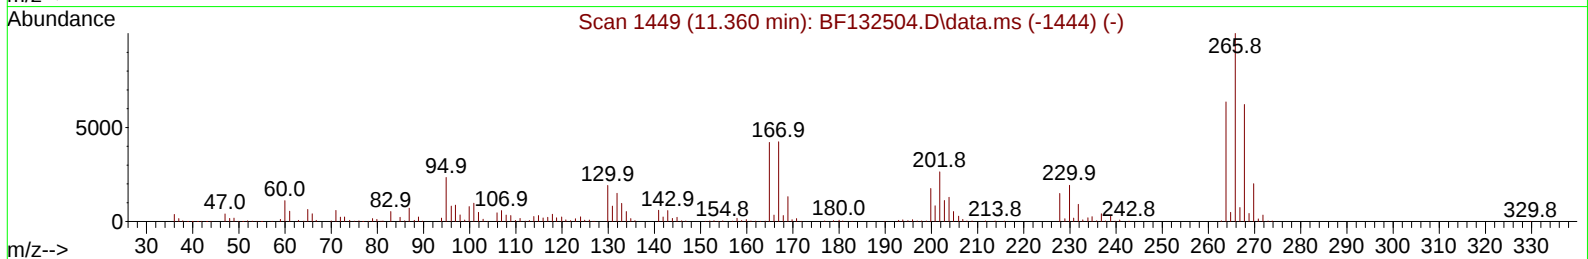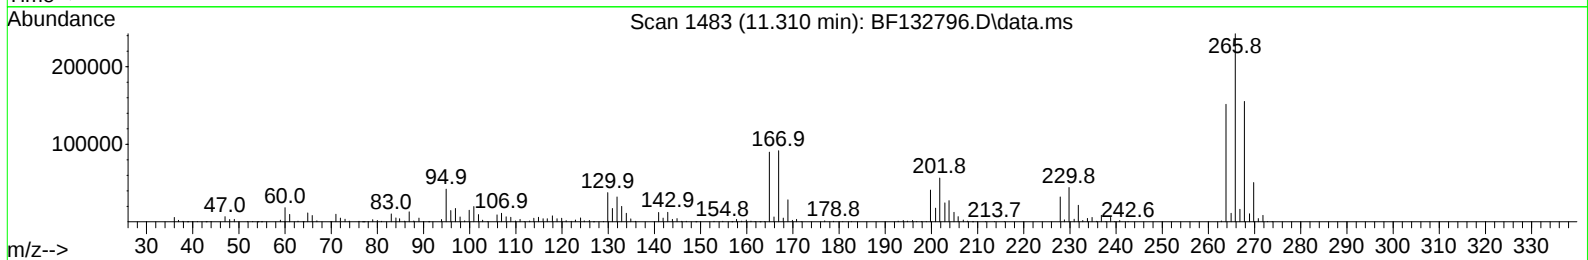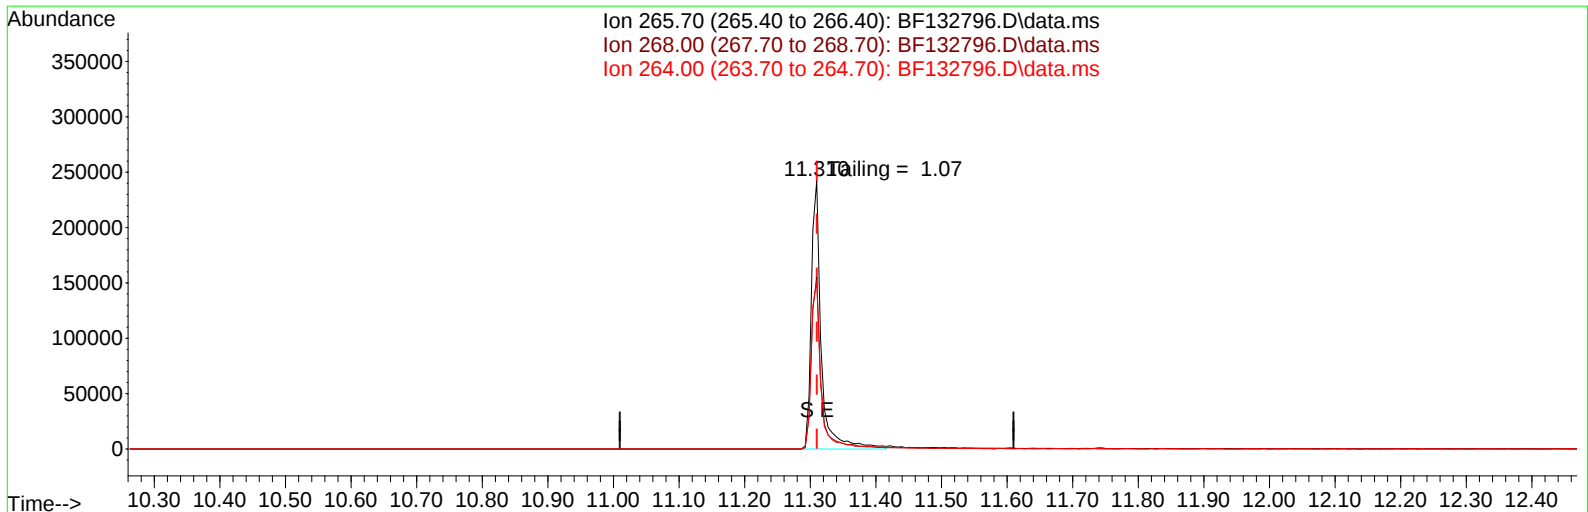

TIC: BF132796.D\data.ms

(70) Pentachlorophenol (C)

11.310min (-0.000) 502082.54 ng




response 263107

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.04
264.00	63.60	62.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031523\
Data File : BF132796.D
Acq On : 15 Mar 2023 11:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 15 12:54:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 14 15:35:42 2023
Response via : Initial Calibration

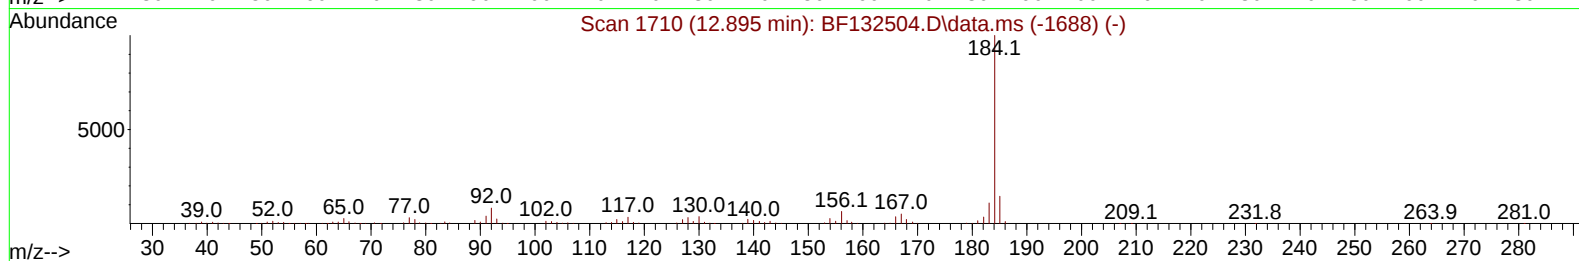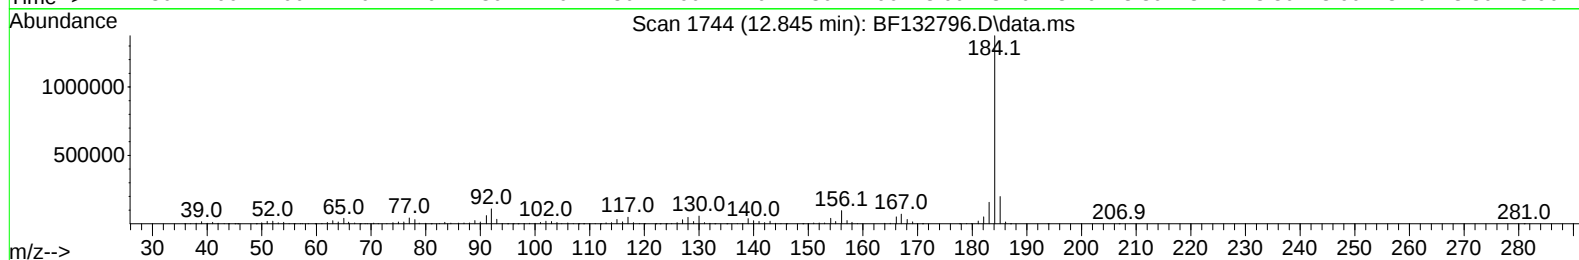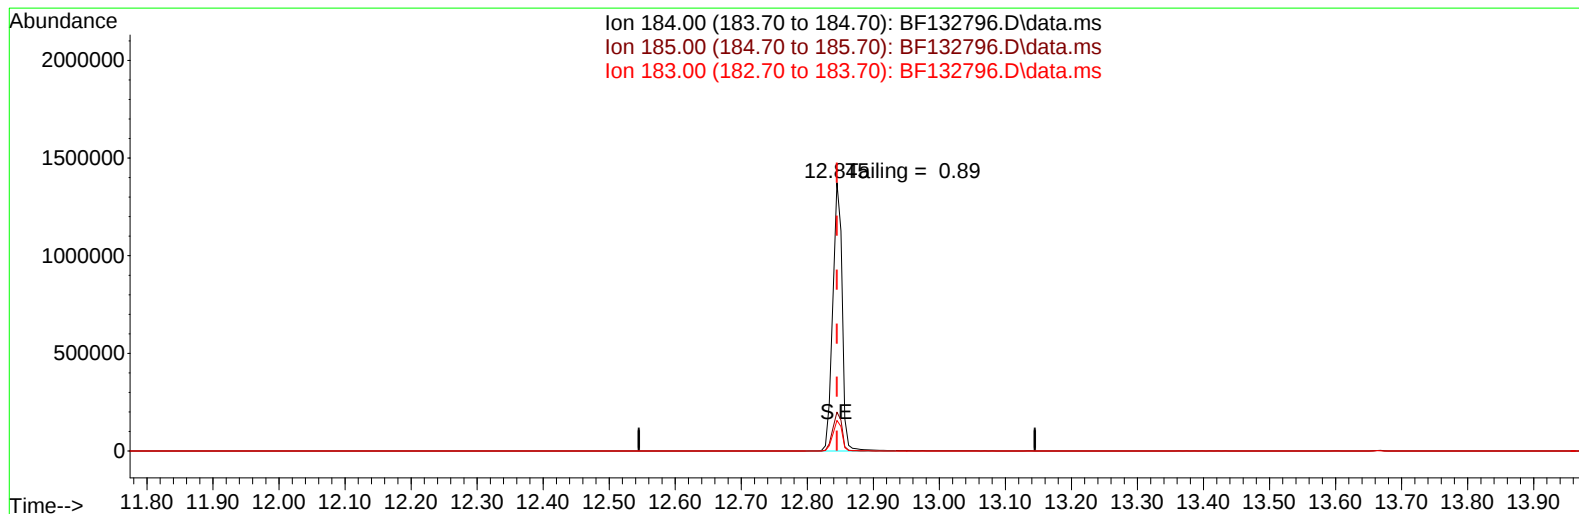

TIC: BF132796.D\data.ms

(77) Benzidine

12.845min (-0.000) 119300.77 ng

response 1362033

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.52
183.00	10.90	11.41
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/15/2023	BNA_F	<u>BF132796.D</u>
Compound Name	Response	Retention Time
DDT	736828	13.668
DDD	20931	13.368
DDE	2712	13.027
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23643	760471	3.11

Instrument :
BNA_F
ClientSampleId :
DFTPP