
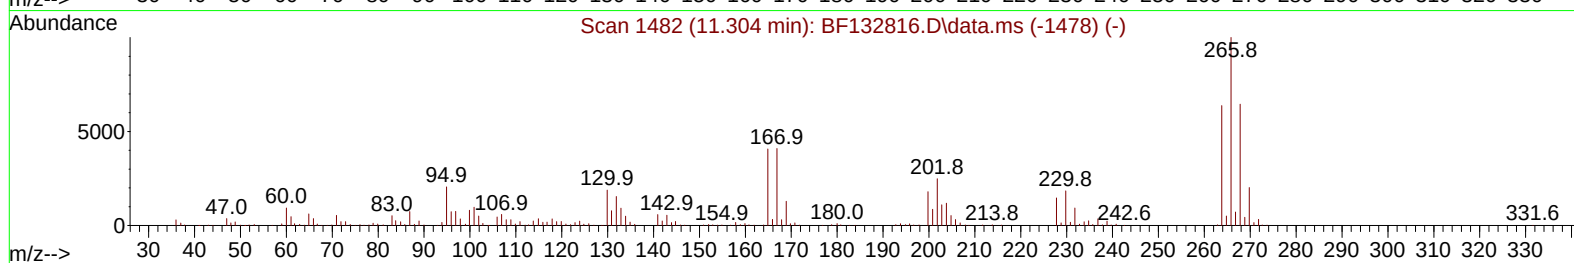
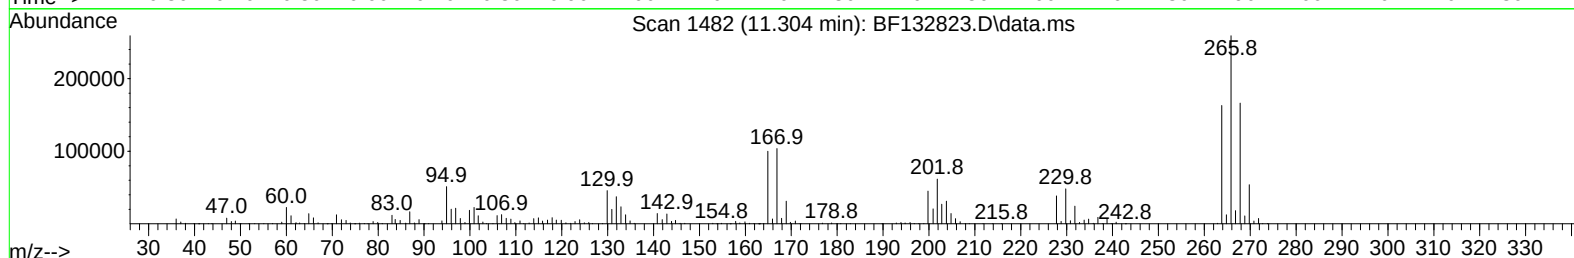


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031723\
 Data File : BF132823.D
 Acq On : 17 Mar 2023 14:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 05:59:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 17 03:35:59 2023
 Response via : Initial Calibration

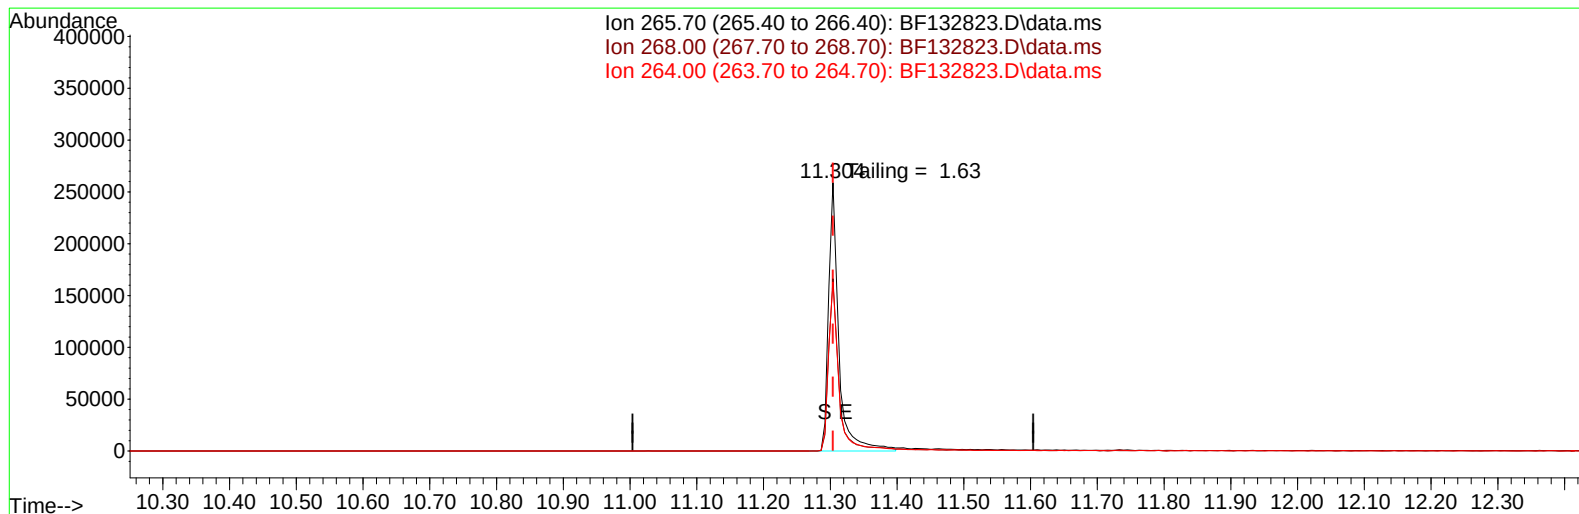

TIC: BF132823.D\data.ms

(70) Pentachlorophenol (C)




11.304min (-0.000) 51433.48 ng

response 281609

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.19
264.00	63.70	62.95
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031723\  
Data File : BF132823.D  
Acq On    : 17 Mar 2023  14:30  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Mar 18 05:59:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 17 03:35:59 2023
Response via : Initial Calibration

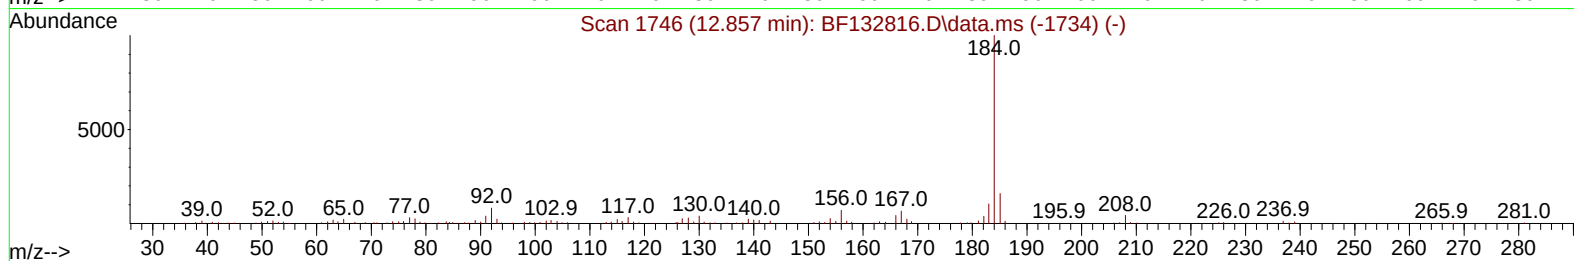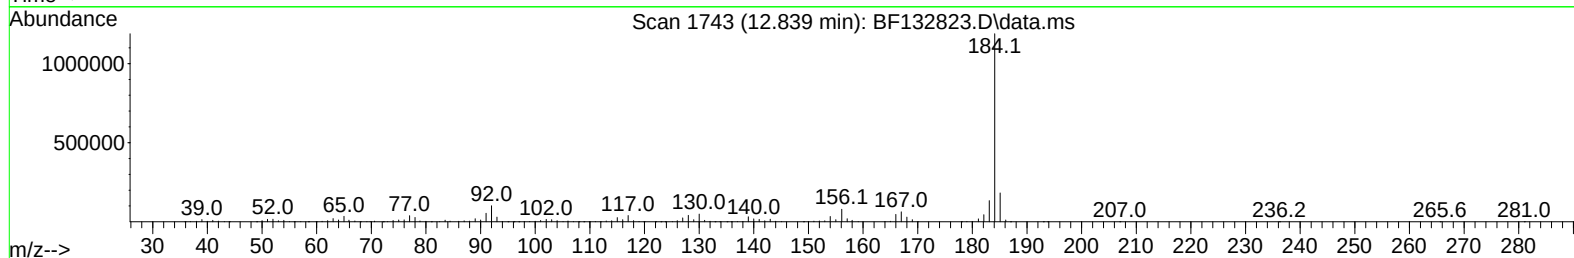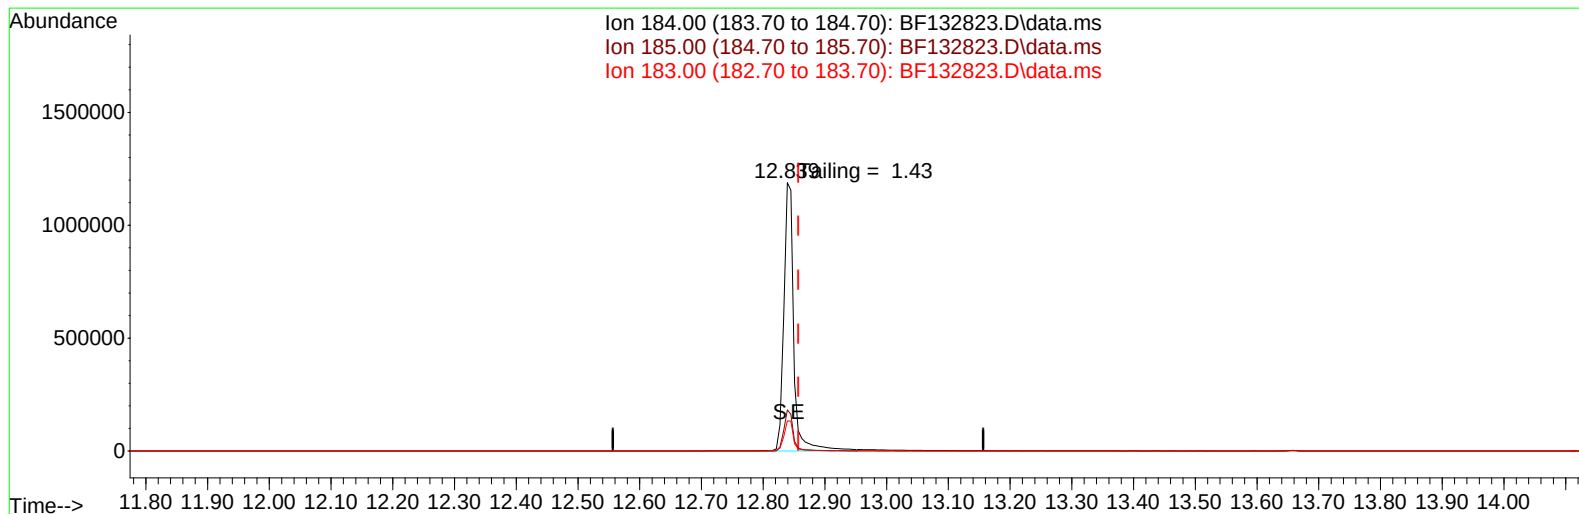

TIC: BF132823.D\data.ms

(77) Benzidine

12.839min (-0.018) 474006.13 ng

response **1349049**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	15.33
183.00	10.30	11.22
0.00	0.00	0.00