


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031723\
 Data File : BF132823.D
 Acq On : 17 Mar 2023 14:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 17 03:35:59 2023

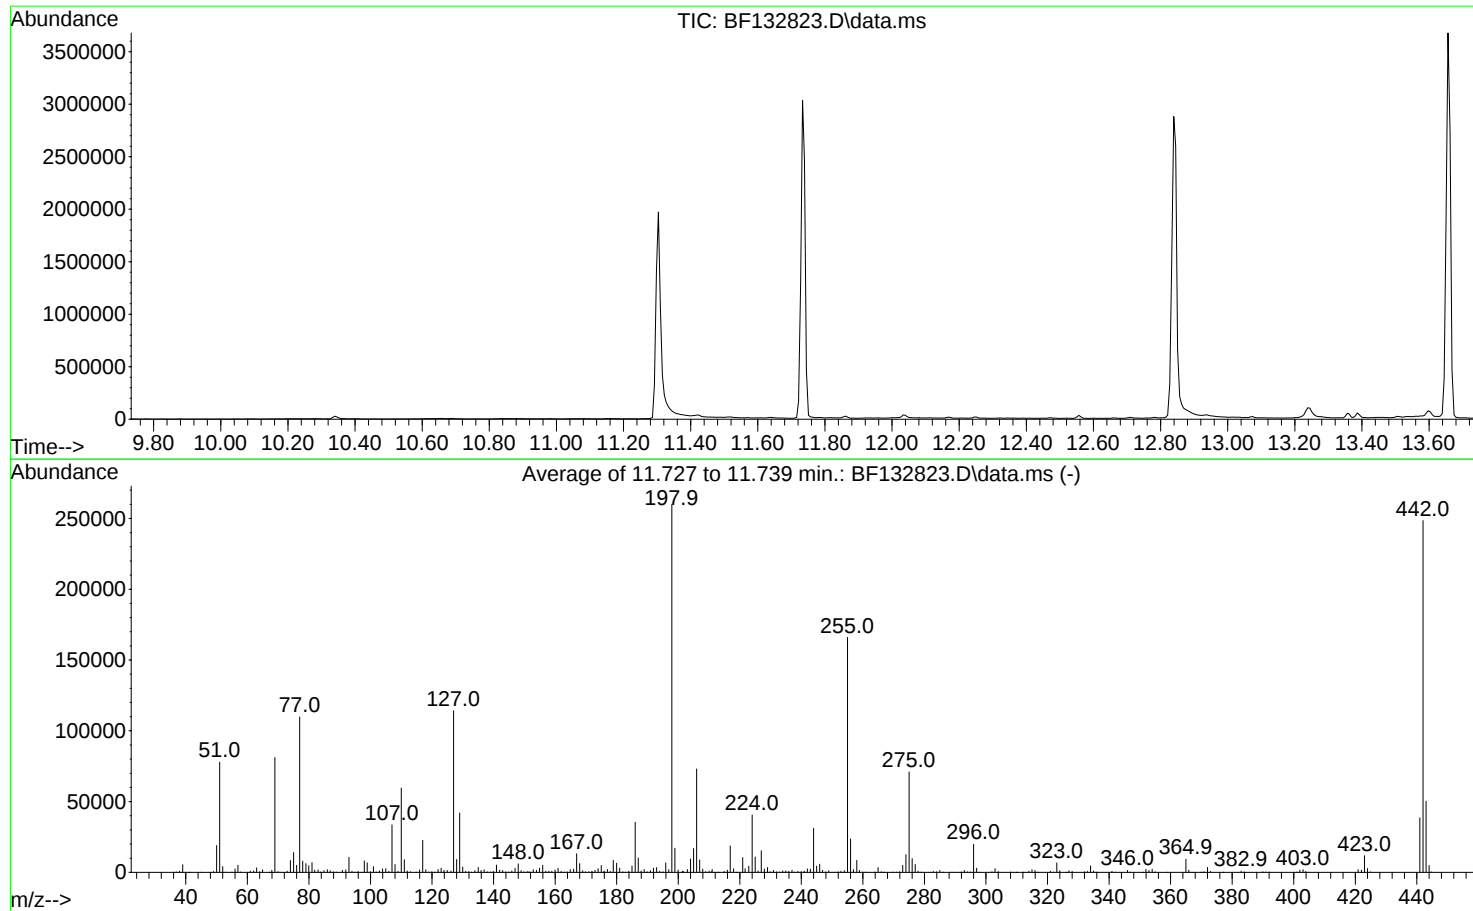

AutoFind: Scans 1554, 1555, 1556; Background Corrected with Scan 1549

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	77928	PASS
68	69	0.00	2	1.8	1497	PASS
69	198	0.00	100	31.2	81135	PASS
70	69	0.00	2	0.8	612	PASS
127	198	10	80	43.9	114173	PASS
197	198	0.00	2	0.8	1974	PASS
198	198	100	100	100.0	259883	PASS
199	198	5	9	6.6	17049	PASS
275	198	10	60	27.3	71008	PASS
365	198	1	100	3.6	9262	PASS
441	198	0.01	100	14.8	38534	PASS
442	442	50	100	100.0	248549	PASS
443	442	15	24	20.2	50256	PASS