
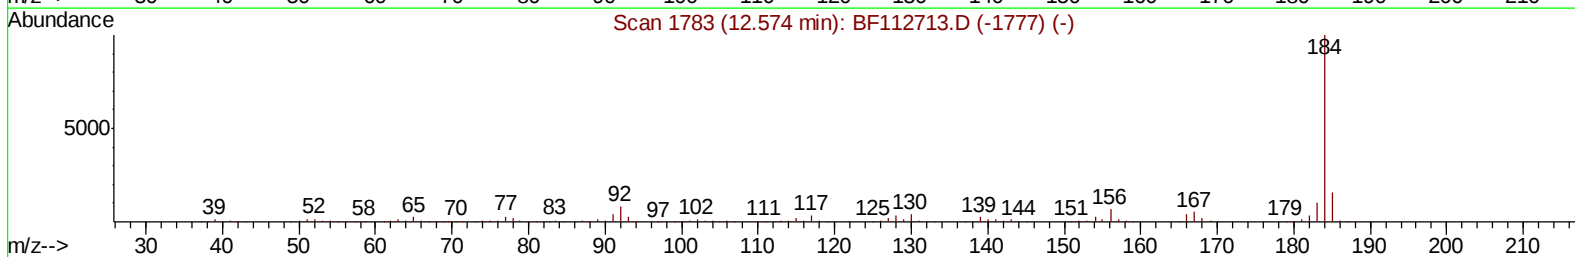
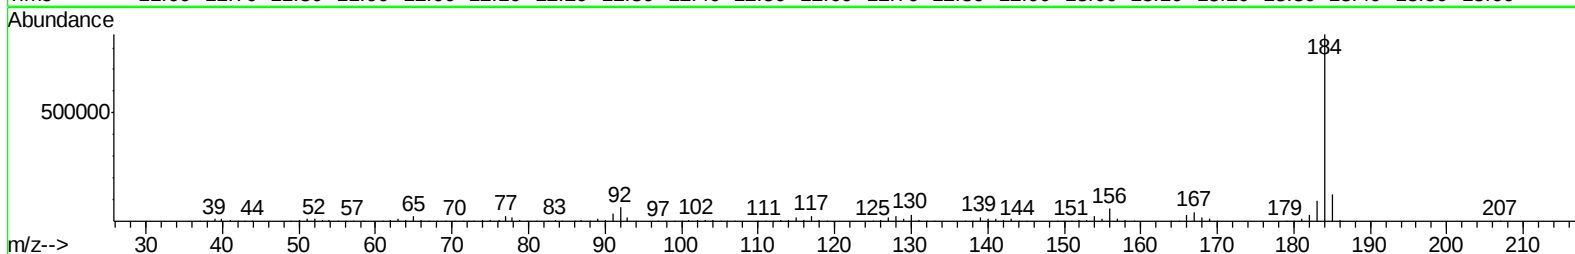


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031819\
Data File : BF113083.D
Acq On : 18 Mar 2019 11:49
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 01:01:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 13 03:42:55 2019
Response via : Initial Calibration

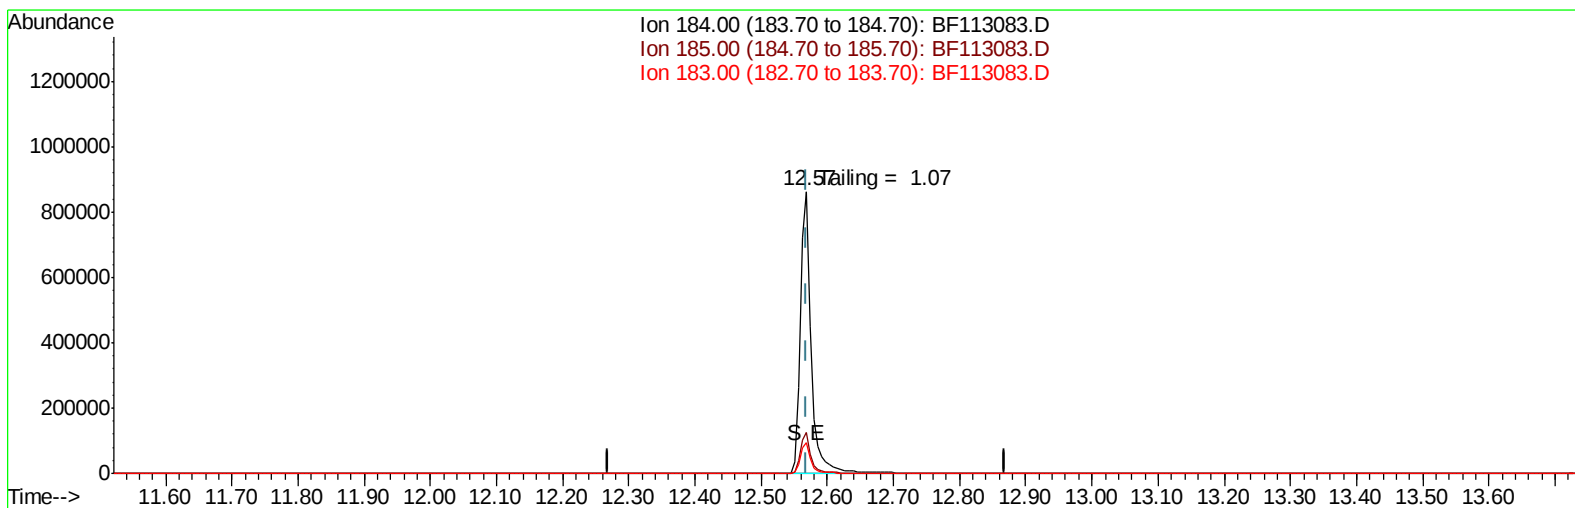

TIC: BF113083.D

(77) Benzidine




12.568min (-0.000) 0.00ng

response 994793

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.41
183.00	10.70	11.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031819\
Data File : BF113083.D
Acq On : 18 Mar 2019 11:49
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 01:01:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 13 03:42:55 2019
Response via : Initial Calibration

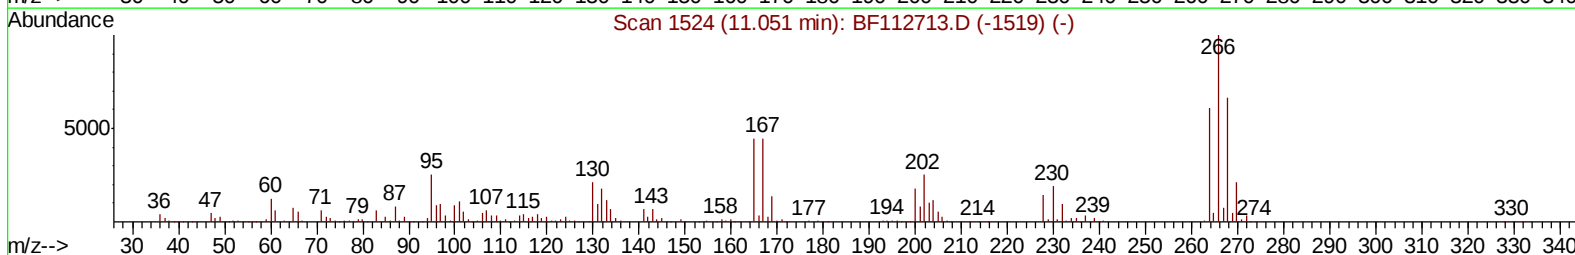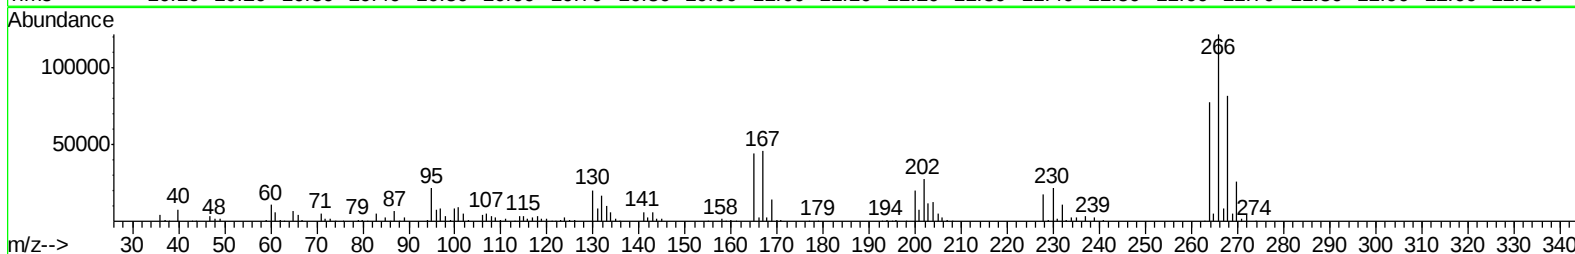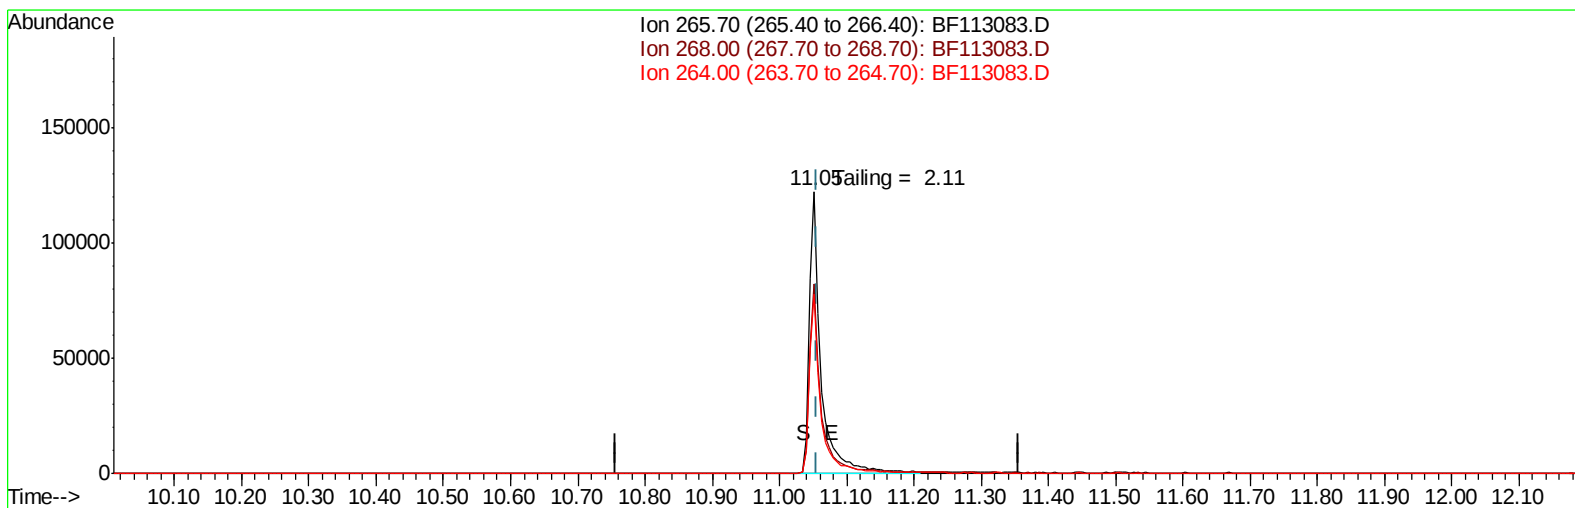

TIC: BF113083.D

(70) Pentachlorophenol (C)

11.051min (-0.006) 32506.17ng

response 150838

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	67.09
264.00	61.10	63.87
0.00	0.00	0.00