
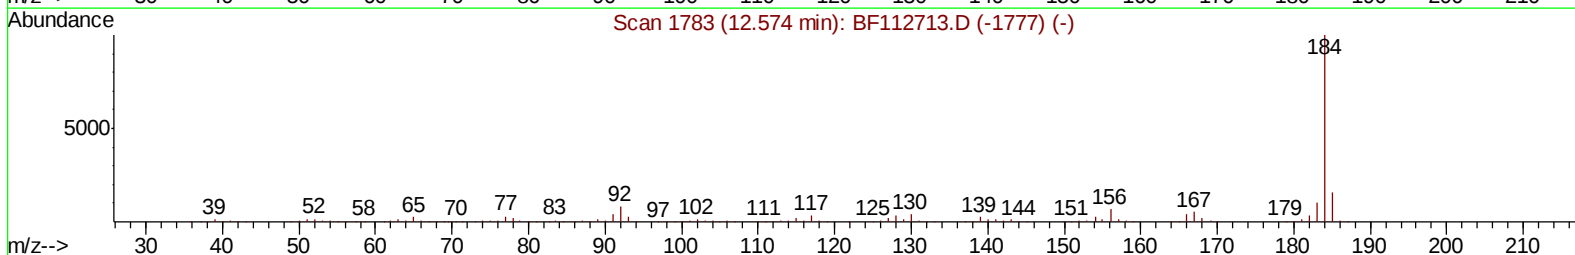
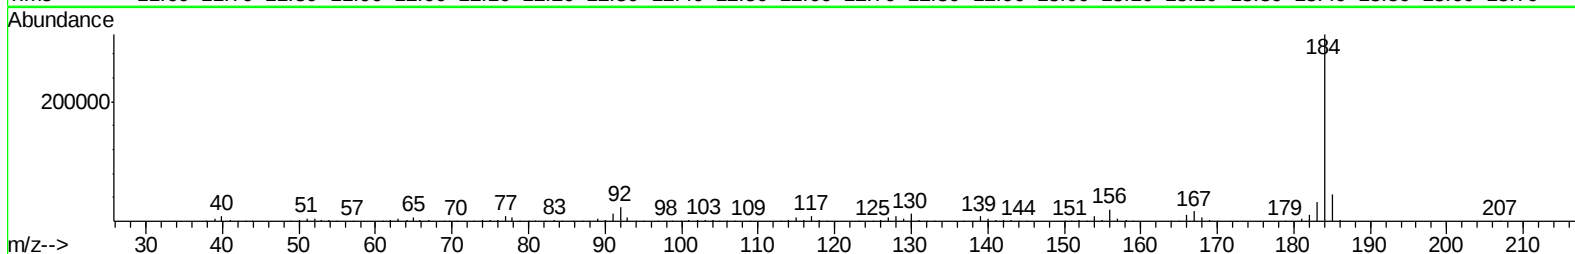


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031819\
Data File : BF113108.D
Acq On : 18 Mar 2019 23:50
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 01:02:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 13 03:42:55 2019
Response via : Initial Calibration

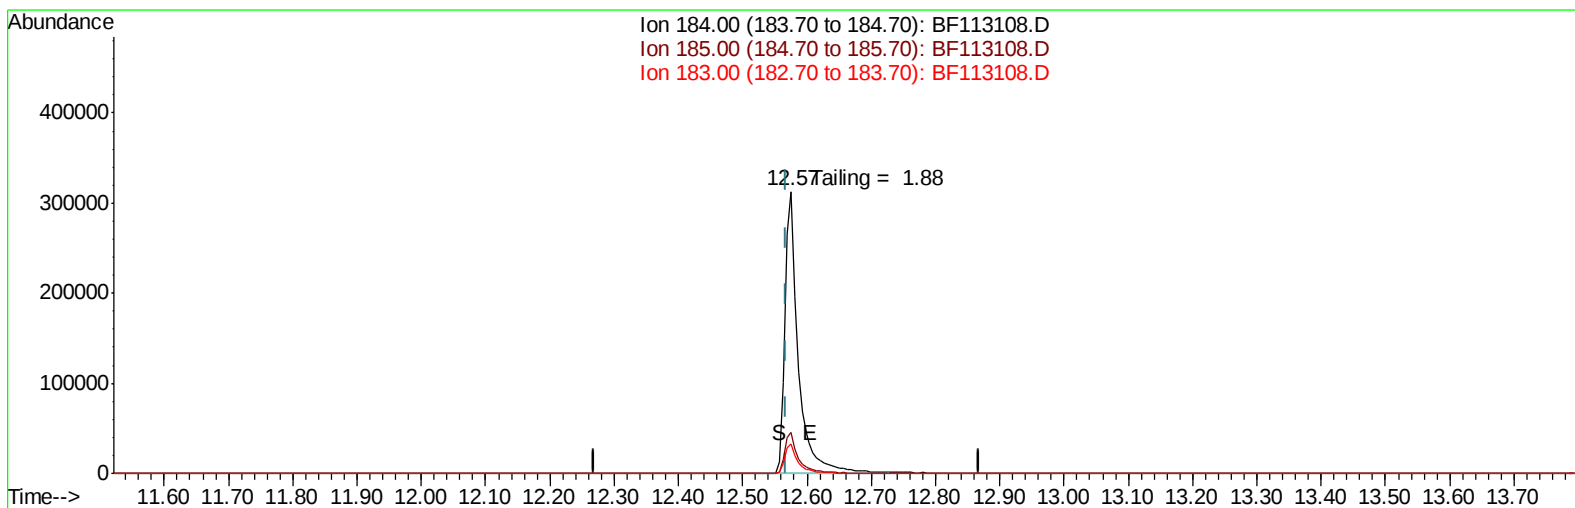

TIC: BF113108.D

(77) Benzidine




12.574min (+0.006) 7660.11ng

response 455443

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.62
183.00	10.70	10.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031819\
Data File : BF113108.D
Acq On : 18 Mar 2019 23:50
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 01:02:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 13 03:42:55 2019
Response via : Initial Calibration

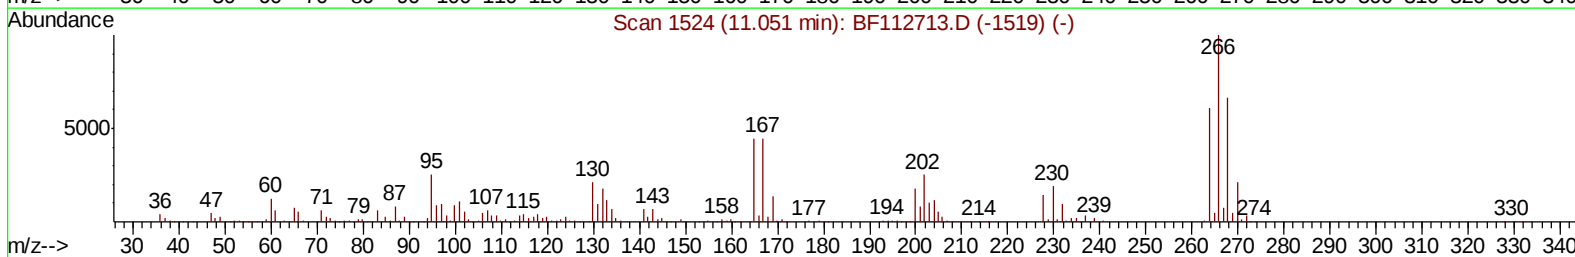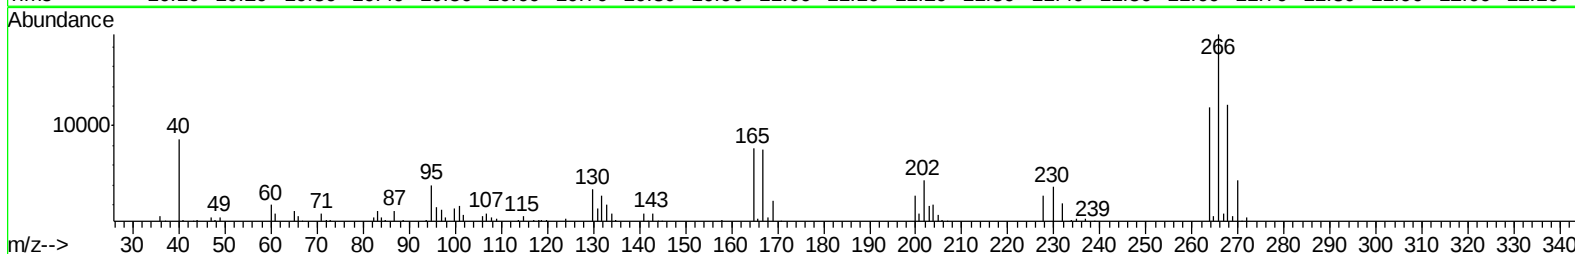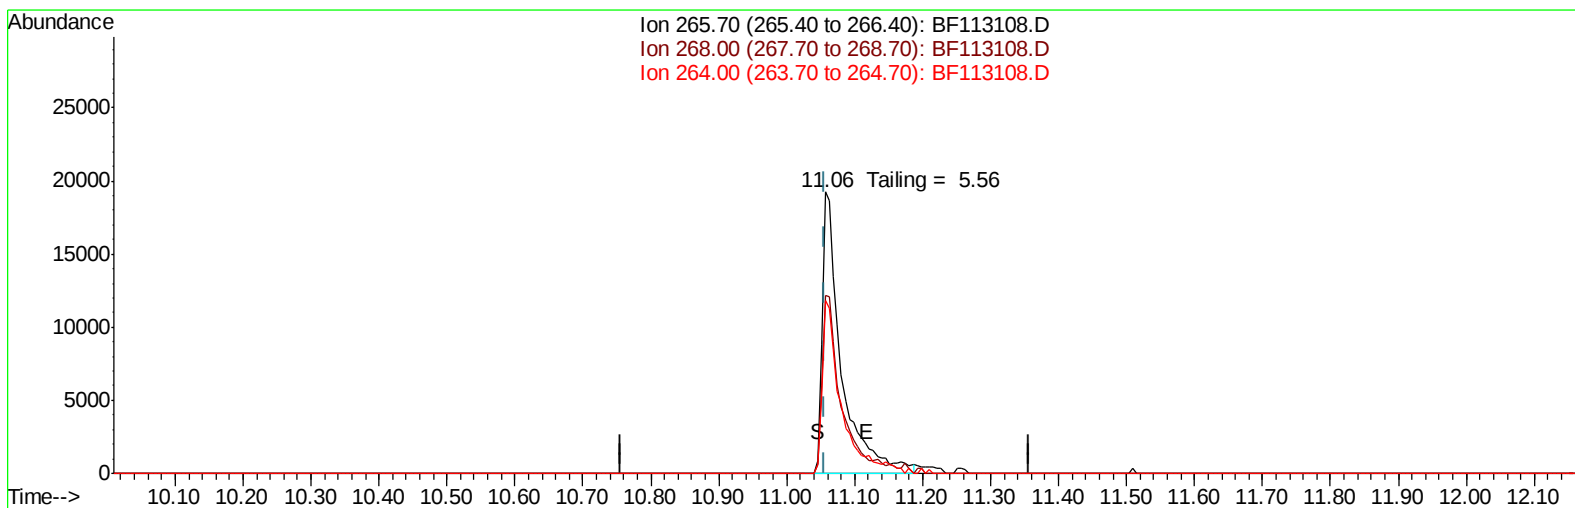

TIC: BF113108.D

(70) Pentachlorophenol (C)

11.057min (-0.000) 9331.31ng

response 37431

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	63.04
264.00	61.10	65.45
0.00	0.00	0.00