

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF031819\
 Data File : BF113117.D
 Acq On : 19 Mar 2019 4:08
 Operator : JU/SJ
 Sample : K1947-06
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PST-025-B035-031319

Quant Time: Mar 19 07:15:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 13 03:42:55 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	121922	20.00	ng	0.00
21) Naphthalene-d8	8.01	136	410865	20.00	ng	0.00
39) Acenaphthene-d10	9.76	164	171130	20.00	ng	0.00
64) Phenanthrene-d10	11.24	188	326553	20.00	ng	0.00
76) Chrysene-d12	13.87	240	324028	20.00	ng	0.00
87) Perylene-d12	15.28	264	226688	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.35	112	865541	110.43	ng	0.00
7) Phenol-d6	6.38	99	1085756	110.28	ng	0.00
23) Nitrobenzene-d5	7.29	82	656627	95.63	ng	0.00
42) 2,4,6-Tribromophenol	10.55	330	275000	151.37	ng	0.00
45) 2-Fluorobiphenyl	9.09	172	1136574	125.45	ng	0.00
79) Terphenyl-d14	12.82	244	1134619	67.88	ng	0.00
Target Compounds						
10) Phenol	6.39	94	43228	3.762	ng	80
50) Dimethylphthalate	9.48	163	168917	13.387	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF031819\
Data File : BF113117.D
Acq On : 19 Mar 2019 4:08
Operator : JU/SJ
Sample : K1947-06
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PST-025-B035-031319

Quant Time: Mar 19 07:15:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 13 03:42:55 2019
Response via : Initial Calibration

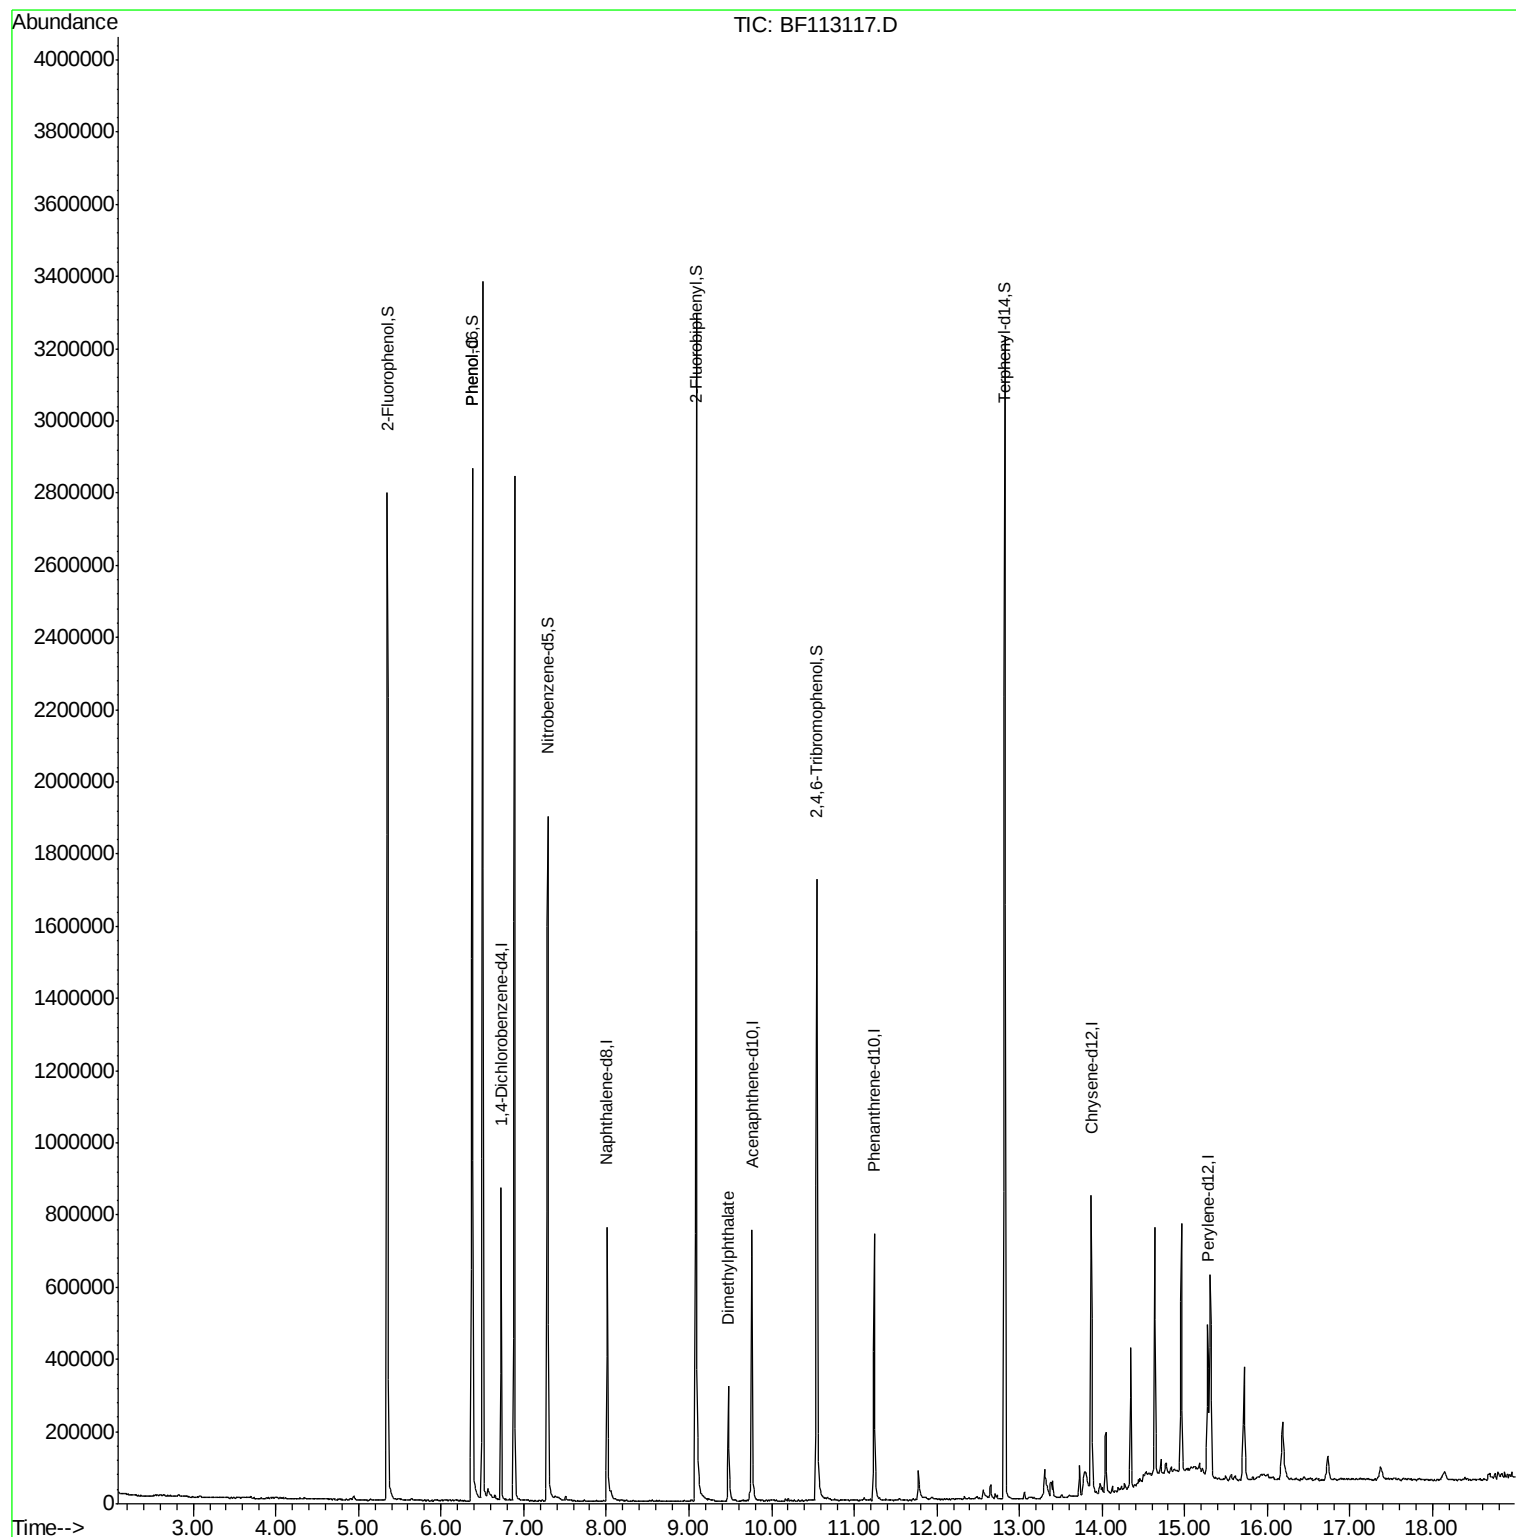

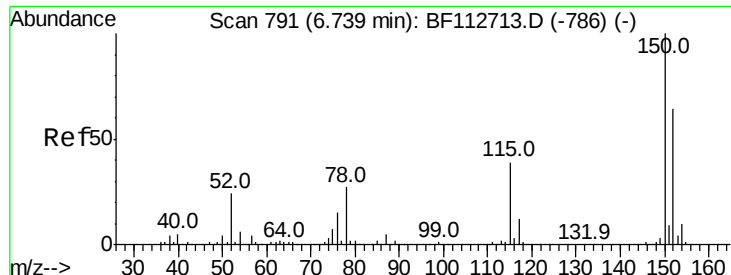


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.73 min Scan# 789
Delta R.T. -0.01 min
Lab File: BF113117.D
Acq: 19 Mar 2019 4:08

Instrument :
BNA_F
ClientSampleId :
PST-025-B035-031319

Tot Ion:152 Resp: 121922
Ion Ratio Lower Upper
152 100
150 155.0 124.2 186.2
115 59.3 48.2 72.4

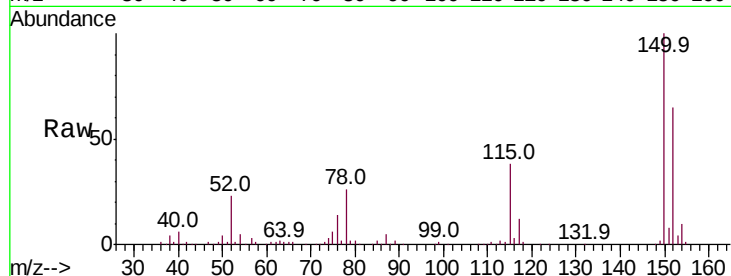


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

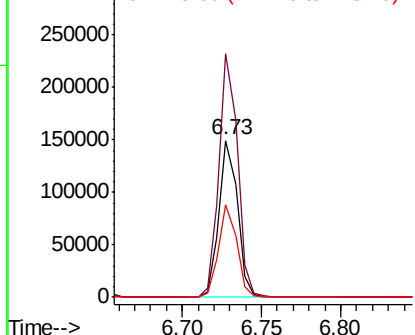



#5


2-Fluorophenol
Concen: 110.430 ng
RT: 5.35 min Scan# 555
Delta R.T. 0.01 min
Lab File: BF113117.D
Acq: 19 Mar 2019 4:08

Tgt Ion:112 Resp: 865541
Ion Ratio Lower Upper
112 100
64 61.1 47.6 71.4
63 32.0 24.4 36.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

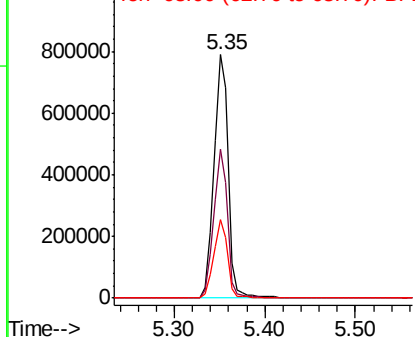



#7

Phenol-d6

Concen: 110.277 ng

RT: 6.38 min Scan# 730

Delta R.T. 0.01 min

Lab File: BF113117.D

Acq: 19 Mar 2019 4:08

Instrument :

BNA_F

ClientSampleId :

PST-025-B035-031319


Tot Ion: 99 Resp: 1085756

Ion Ratio Lower Upper




99 100

42 18.8 16.3 24.5

71 33.5 26.2 39.4



Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

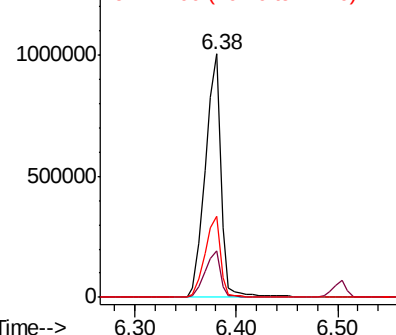

#10

Phenol

Concen: 3.762 ng

RT: 6.39 min Scan# 731

Delta R.T. -0.01 min

Lab File: BF113117.D

Acq: 19 Mar 2019 4:08


Tgt Ion: 94 Resp: 43228

Ion Ratio Lower Upper



94 100


65 34.1 10.5 50.5

66 61.6 22.6 62.6



Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

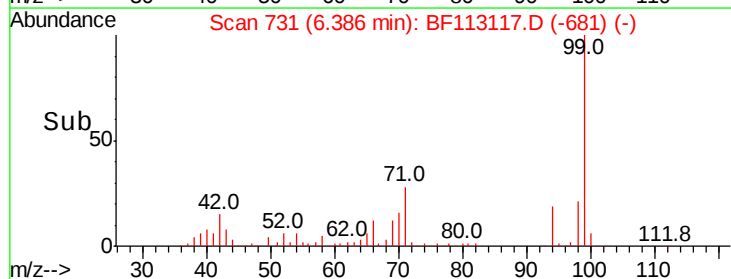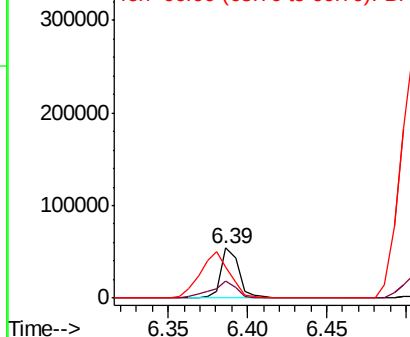

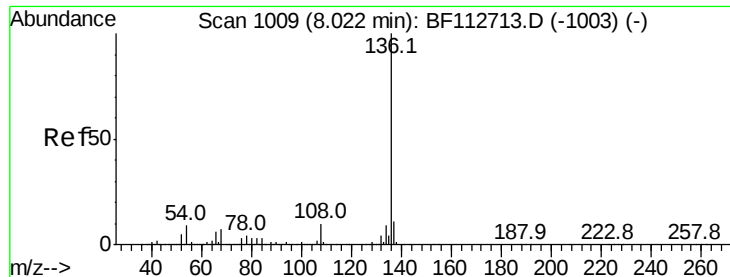

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.01 min Scan# 1007

Delta R.T. -0.01 min

Lab File: BF113117.D

Acq: 19 Mar 2019 4:08

Instrument :

BNA_F

ClientSampleId :

PST-025-B035-031319

Tot Ion:136 Resp: 410865


Ion Ratio Lower Upper

136 100

137 10.9 8.9 13.3

54 8.0 7.3 10.9

68 5.7 5.4 8.2



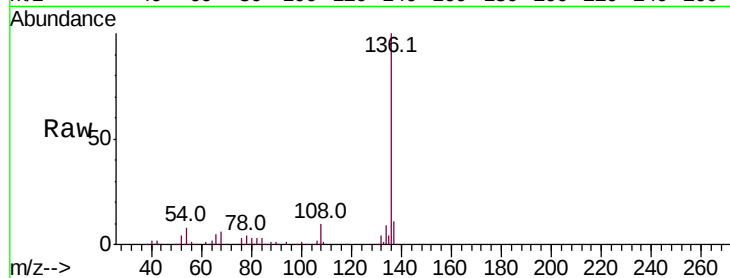


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

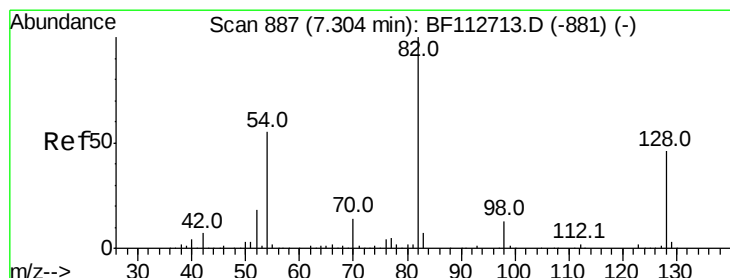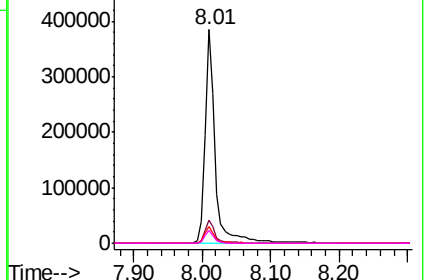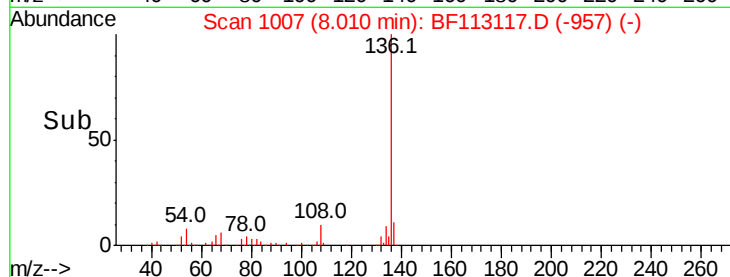

#23

Nitrobenzene-d5

Concen: 95.630 ng

RT: 7.29 min Scan# 885

Delta R.T. -0.01 min

Lab File: BF113117.D

Acq: 19 Mar 2019 4:08


Tgt Ion: 82 Resp: 656627

Ion Ratio Lower Upper

82 100

128 47.0 36.3 54.5



54 52.6 43.7 65.5

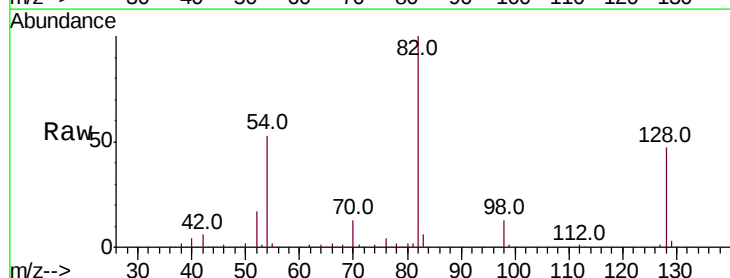


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

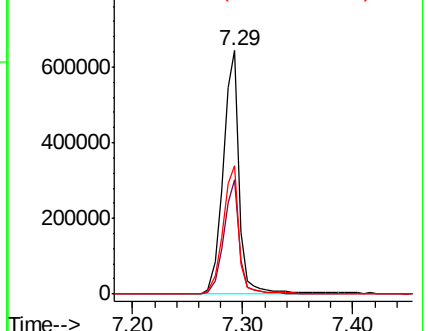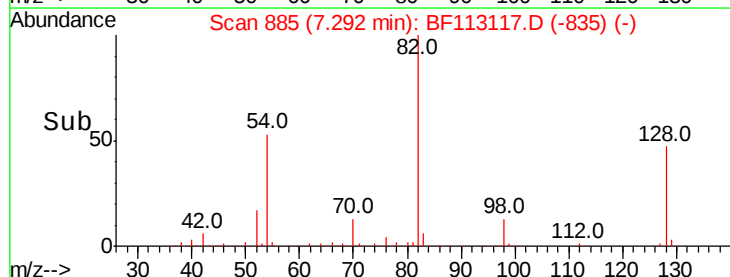







#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.76 min Scan# 1305
Delta R.T. -0.01 min
Lab File: BF113117.D
Acq: 19 Mar 2019 4:08

Instrument :
BNA_F
ClientSampleId :
PST-025-B035-031319

Tot Ion	Ratio	Lower	Upper
164	100		
162	102.6	80.6	120.8
160	46.0	36.0	54.0

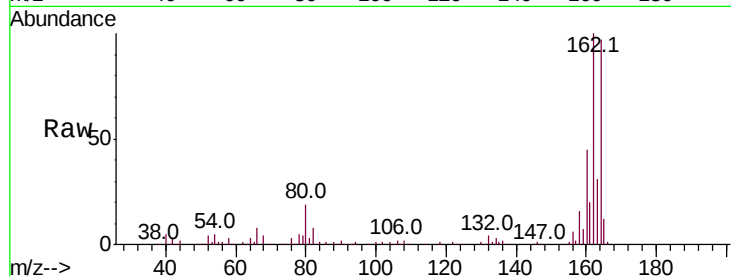


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E


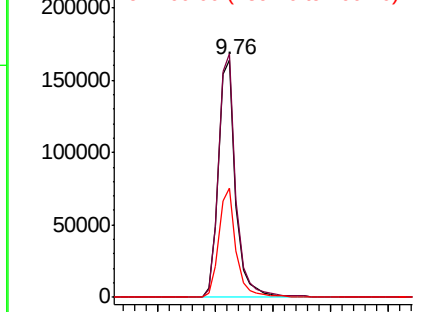



#42
2,4,6-Tribromophenol
Concen: 151.368 ng
RT: 10.55 min Scan# 1439
Delta R.T. -0.00 min
Lab File: BF113117.D
Acq: 19 Mar 2019 4:08

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.6	76.2	114.4
141	28.6	27.0	40.6



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

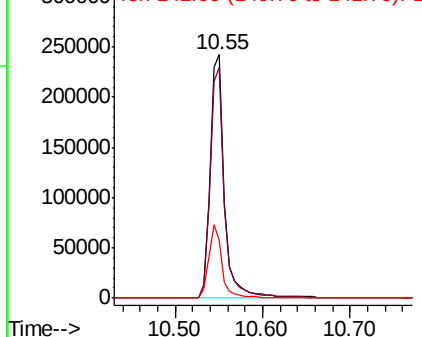


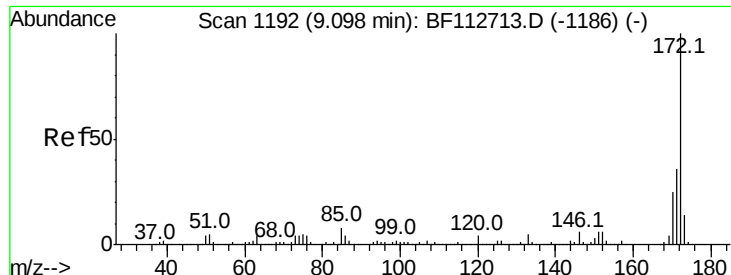




#45
2-Fluorobiphenyl
Concen: 125.453 ng
RT: 9.09 min Scan# 1190
Delta R.T. -0.01 min
Lab File: BF113117.D
Acq: 19 Mar 2019 4:08

Instrument :
BNA_F
ClientSampleId :
PST-025-B035-031319

Tot Ion:172 Resp: 1136574
Ion Ratio Lower Upper
172 100
171 35.6 29.0 43.4
170 24.5 20.0 30.0

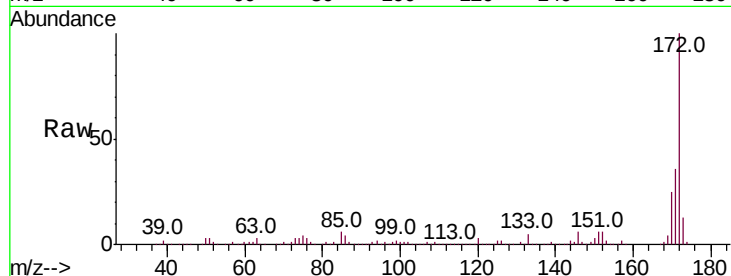


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

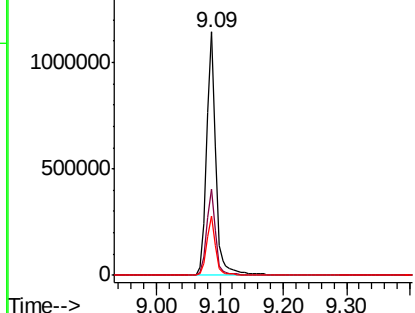




#50
Dimethylphthalate
Concen: 13.387 ng
RT: 9.48 min Scan# 1257
Delta R.T. -0.02 min
Lab File: BF113117.D
Acq: 19 Mar 2019 4:08

Tgt Ion:163 Resp: 168917
Ion Ratio Lower Upper
163 100
194 4.0 3.0 4.4
164 9.7 8.4 12.6



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E



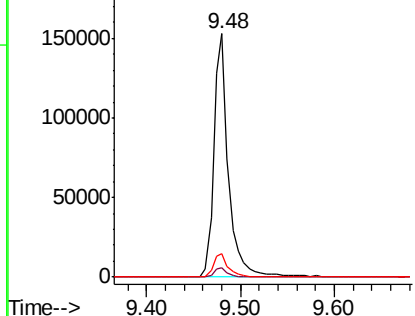



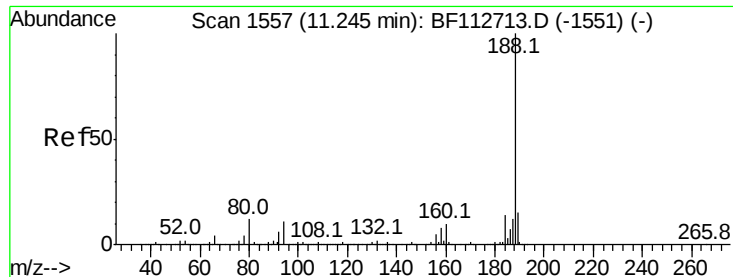

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.24 min Scan# 1556
Delta R.T. -0.01 min
Lab File: BF113117.D
Acq: 19 Mar 2019 4:08




Instrument :
BNA_F
ClientSampleId :
PST-025-B035-031319


Tot Ion:188 Resp: 326553
Ion Ratio Lower Upper
188 100
94 8.9 9.0 13.4#
80 9.3 9.2 13.8

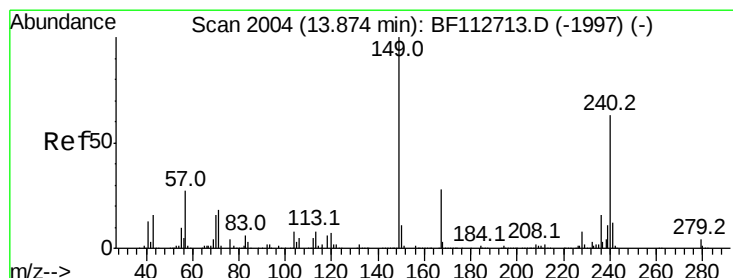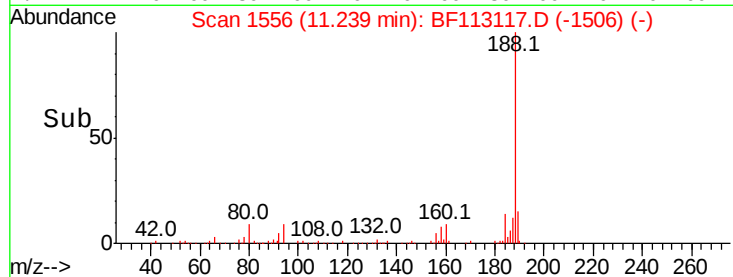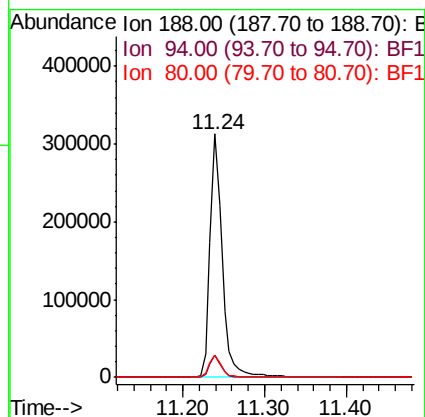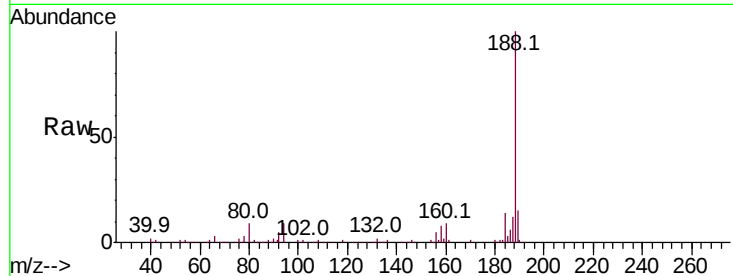

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.87 min Scan# 2003
Delta R.T. -0.00 min
Lab File: BF113117.D
Acq: 19 Mar 2019 4:08

Tgt Ion:240 Resp: 324028
Ion Ratio Lower Upper
240 100
120 10.9 8.9 13.3
236 26.1 20.7 31.1

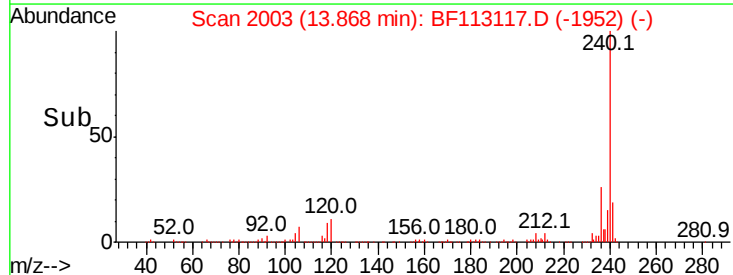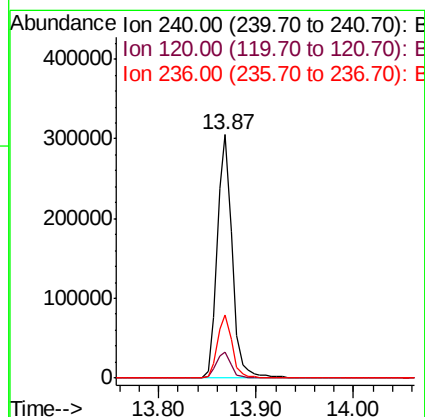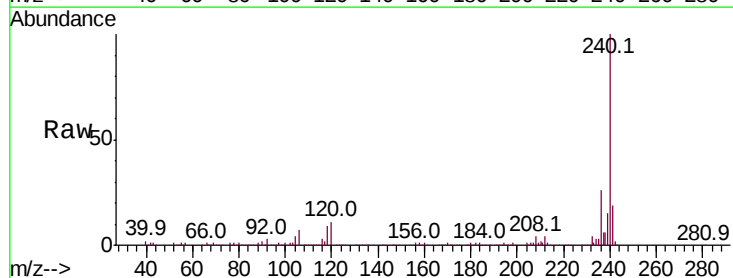

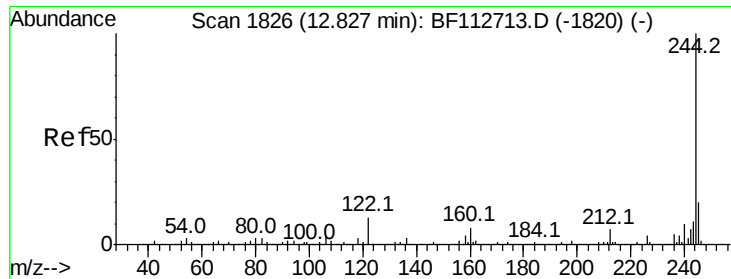

#79

Terphenyl-d14

Concen: 67.879 ng

RT: 12.82 min Scan# 1825

Delta R.T. -0.00 min

Lab File: BF113117.D

Acq: 19 Mar 2019 4:08

Instrument :

BNA_F

ClientSampleId :

PST-025-B035-031319


Tot Ion:244 Resp: 1134619

Ion Ratio Lower Upper

244 100

212 6.7 5.6 8.4




122 11.1 10.5 15.7



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

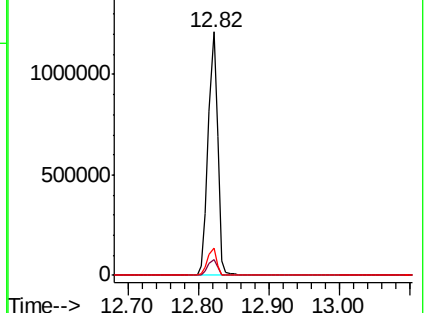

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.28 min Scan# 2243

Delta R.T. 0.01 min

Lab File: BF113117.D

Acq: 19 Mar 2019 4:08


Tgt Ion:264 Resp: 226688

Ion Ratio Lower Upper

264 100

260 24.4 18.7 28.1

265 21.5 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

