

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031819\
 Data File : BF113103.D
 Acq On : 18 Mar 2019 21:06
 Operator : JU/SJ
 Sample : K1691-13 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-031519-C

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.339	549	553	564	rBV	344727	372478	28.48%	3.652%
2	6.369	725	728	739	rBV	359415	396285	30.30%	3.885%
3	6.498	747	750	758	rBV	474731	411596	31.47%	4.035%
4	6.728	785	789	800	rBV	952304	815384	62.34%	7.994%
5	6.886	812	816	825	rBV	362246	362438	27.71%	3.553%
6	7.286	881	884	891	rBV	199960	220837	16.88%	2.165%
7	8.010	1003	1007	1014	rBV	1047110	977285	74.72%	9.581%
8	8.616	1106	1110	1115	rBV2	14815	18314	1.40%	0.180%
9	9.086	1186	1190	1201	rBV	425585	531431	40.63%	5.210%
10	9.175	1201	1205	1209	rVB3	13541	20335	1.55%	0.199%
11	9.480	1254	1257	1262	rBV2	25939	39510	3.02%	0.387%
12	9.763	1301	1305	1319	rBV	1156714	1219970	93.27%	11.961%
13	10.310	1395	1398	1401	rBV2	14177	15380	1.18%	0.151%
14	10.421	1414	1417	1422	rVB2	14604	15954	1.22%	0.156%
15	10.545	1435	1438	1451	rBV	265437	315293	24.11%	3.091%
16	10.674	1457	1460	1461	rBV2	25190	25226	1.93%	0.247%
17	11.121	1533	1536	1537	rBV2	17196	16184	1.24%	0.159%
18	11.151	1538	1541	1544	rVB2	22830	25414	1.94%	0.249%
19	11.239	1552	1556	1567	rBV	1228936	1307967	100.00%	12.823%
20	11.316	1567	1569	1572	rVB	28578	26263	2.01%	0.257%
21	11.474	1591	1596	1598	rBV4	14621	17125	1.31%	0.168%
22	11.739	1639	1641	1644	rBV	17056	20032	1.53%	0.196%
23	11.774	1644	1647	1652	rVV2	36244	44499	3.40%	0.436%
24	11.851	1657	1660	1663	rBV	42283	46831	3.58%	0.459%
25	12.292	1732	1735	1737	rBV	28854	27617	2.11%	0.271%
26	12.321	1737	1740	1741	rBV3	27199	26229	2.01%	0.257%
27	12.445	1758	1761	1765	rBV	203437	204038	15.60%	2.000%
28	12.674	1797	1800	1803	rBV	189813	159061	12.16%	1.559%
29	12.815	1821	1824	1834	rVB	534385	537892	41.12%	5.274%
30	13.868	1999	2003	2010	rBV	1206570	1291051	98.71%	12.658%
31	15.280	2239	2243	2247	rBV	554611	691918	52.90%	6.784%


Sum of corrected areas: 10199837

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF031819\
Data File : BF113103.D
Acq On : 18 Mar 2019 21:06
Operator : JU/SJ
Sample : K1691-13 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-031519-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

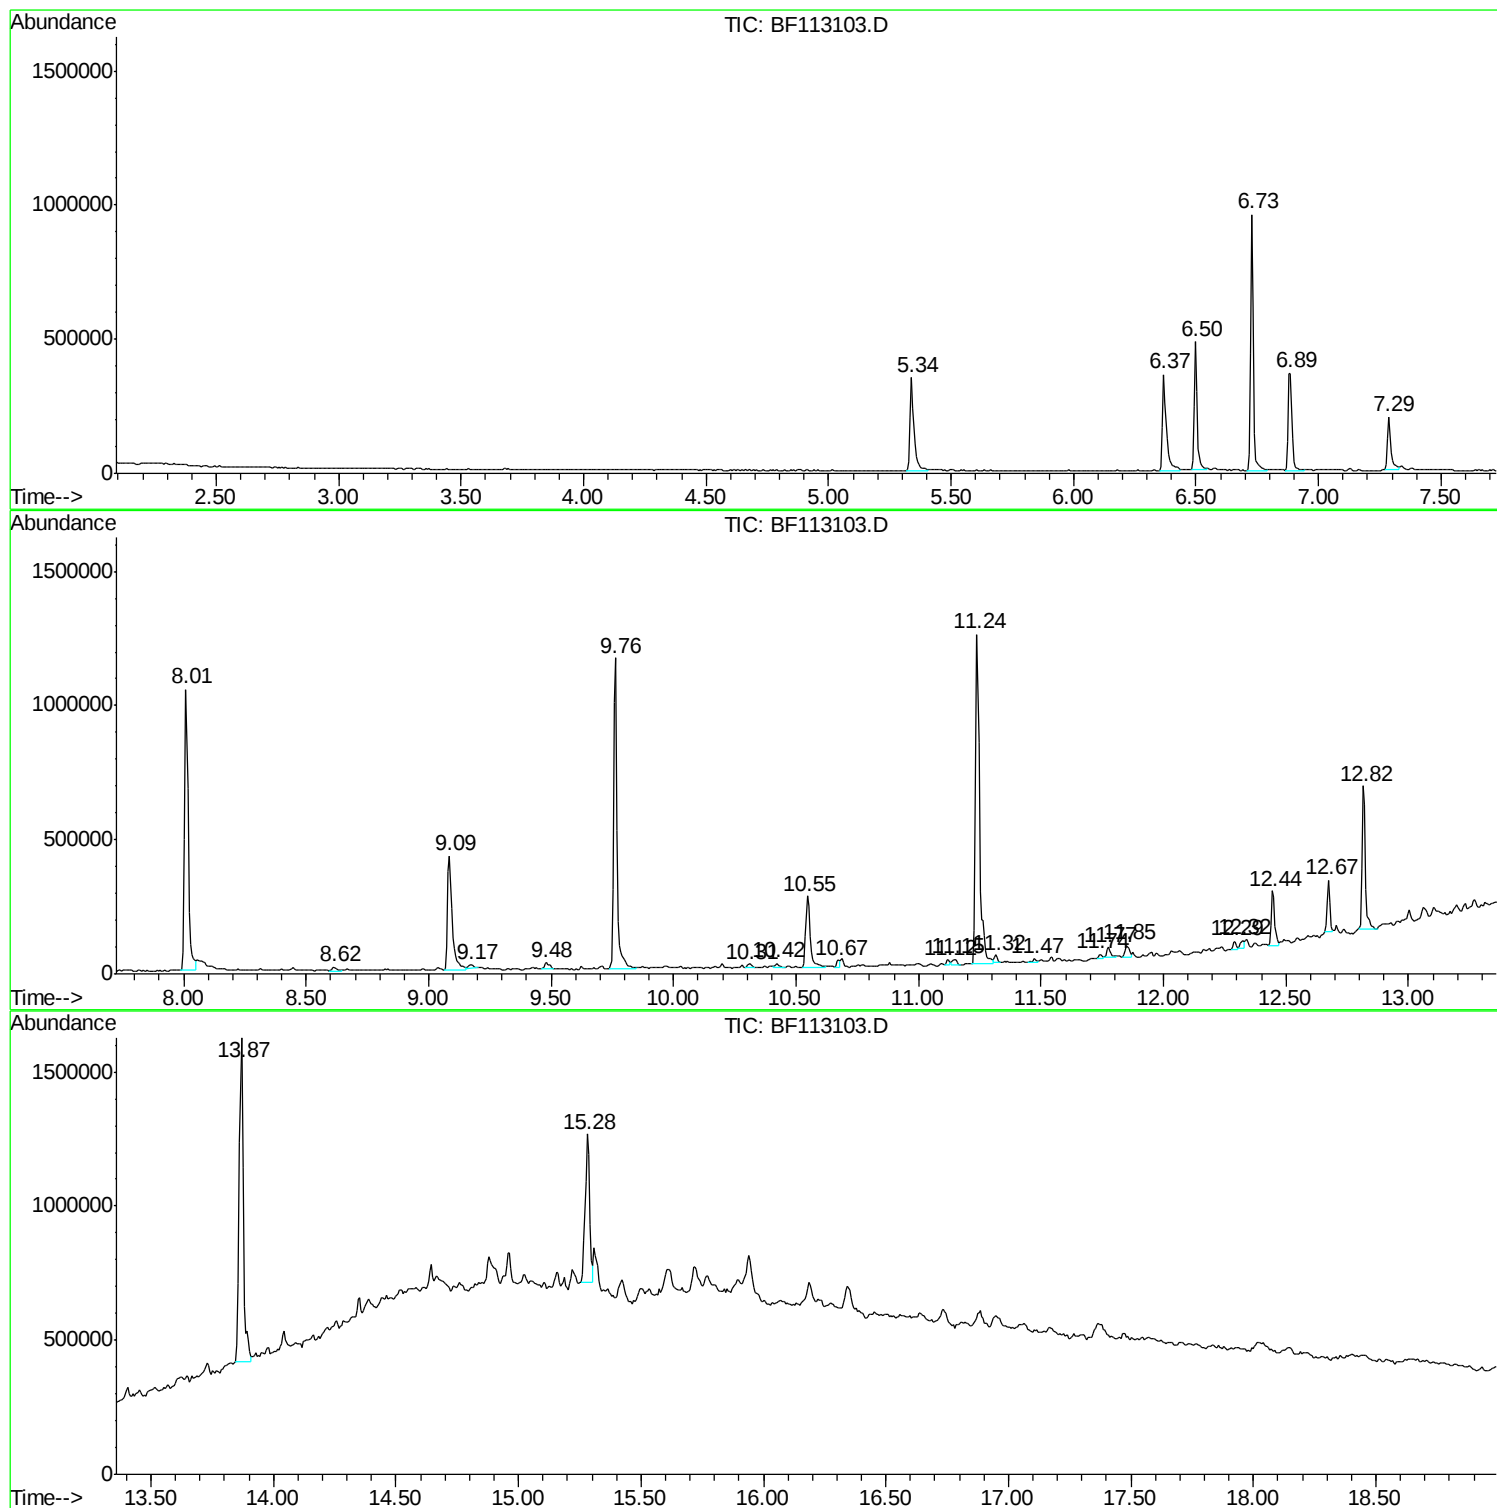

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF031819\
Data File : BF113103.D
Acq On : 18 Mar 2019 21:06
Operator : JU/SJ
Sample : K1691-13 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-031519-C










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.50 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.50	10.10 ng	411596	1,4-Dichlorobenzene-d4	6.73

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Amphetaminil	250	C17H18N2	017590-01-1	12
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
5		5-Aminoindole	132	C8H8N2	005192-03-0	9

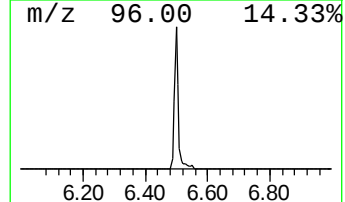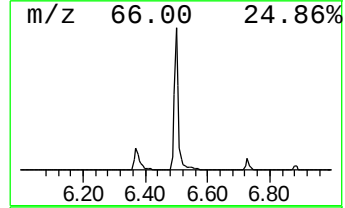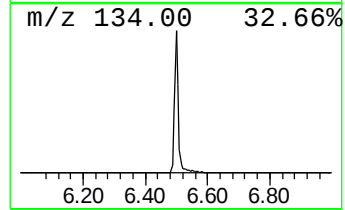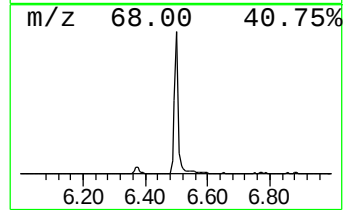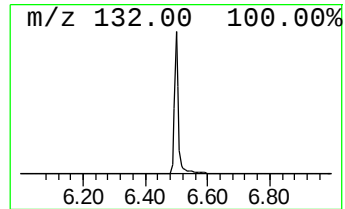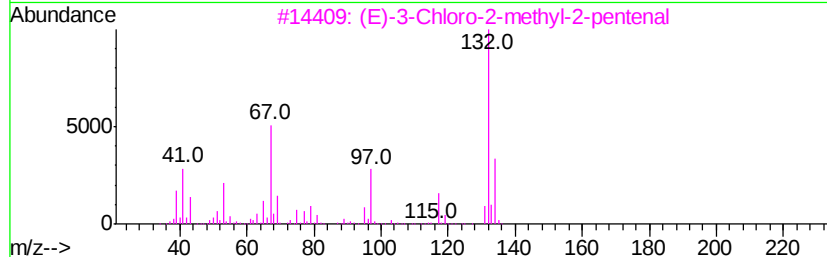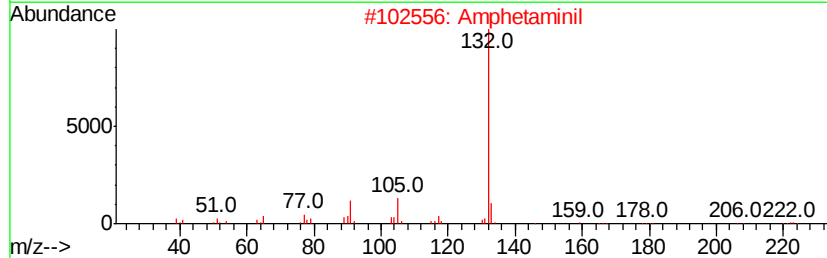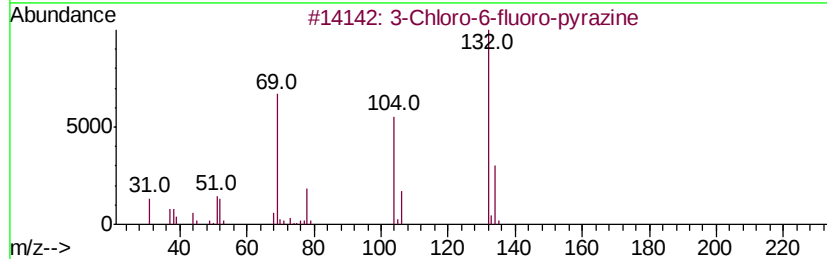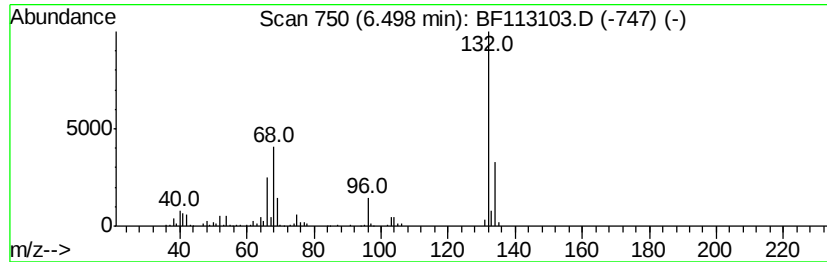

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031819\
Data File : BF113103.D
Acq On : 18 Mar 2019 21:06
Operator : JU/SJ
Sample : K1691-13 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-031519-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.50	6.50	10.1	ng	411596	1	6.73	815384	20.0