

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031819\
 Data File : BF113105.D
 Acq On : 18 Mar 2019 22:01
 Operator : JU/SJ
 Sample : K1691-17 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-031519-E

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.340	549	553	564	rBV	410708	453707	36.70%	4.071%
2	6.369	725	728	747	rBV	510863	576451	46.63%	5.172%
3	6.498	747	750	760	rBV	672921	575547	46.56%	5.164%
4	6.728	786	789	801	rBV	1056688	918266	74.28%	8.239%
5	6.887	812	816	834	rVB	524778	499460	40.40%	4.481%
6	7.287	880	884	891	rBV	275949	306275	24.77%	2.748%
7	8.010	1004	1007	1014	rBV	1043649	1034751	83.70%	9.284%
8	9.086	1186	1190	1203	rBV	556472	673883	54.51%	6.046%
9	9.481	1254	1257	1262	rBV	29651	38531	3.12%	0.346%
10	9.763	1301	1305	1319	rBV	1110215	1182116	95.62%	10.606%
11	10.545	1434	1438	1446	rBV	309497	372449	30.13%	3.342%
12	10.675	1457	1460	1468	rVB3	24517	39527	3.20%	0.355%
13	11.122	1533	1536	1538	rBV	18839	17991	1.46%	0.161%
14	11.145	1538	1540	1545	rVB3	16395	19009	1.54%	0.171%
15	11.239	1552	1556	1567	rBV	1199146	1236249	100.00%	11.091%
16	11.316	1567	1569	1573	rVB	19611	23250	1.88%	0.209%
17	11.775	1645	1647	1654	rBV5	25163	38193	3.09%	0.343%
18	11.851	1658	1660	1663	rBV	21966	17101	1.38%	0.153%
19	11.945	1674	1676	1679	rVB2	20318	18771	1.52%	0.168%
20	12.286	1732	1734	1738	rBV3	14669	18305	1.48%	0.164%
21	12.445	1758	1761	1767	rBV	130927	137477	11.12%	1.233%
22	12.674	1797	1800	1803	rBV	123020	116626	9.43%	1.046%
23	12.704	1803	1805	1808	rVB2	35156	31411	2.54%	0.282%
24	12.816	1821	1824	1833	rBV	663867	696456	56.34%	6.248%
25	13.063	1863	1866	1870	rBV3	42932	55338	4.48%	0.496%
26	13.404	1921	1924	1926	rBV	51249	52265	4.23%	0.469%
27	13.868	1999	2003	2007	rBV	1242777	1230716	99.55%	11.042%
28	15.280	2239	2243	2247	rBV	616423	765853	61.95%	6.871%


Sum of corrected areas: 11145974

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF031819\
Data File : BF113105.D
Acq On : 18 Mar 2019 22:01
Operator : JU/SJ
Sample : K1691-17 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-031519-E

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

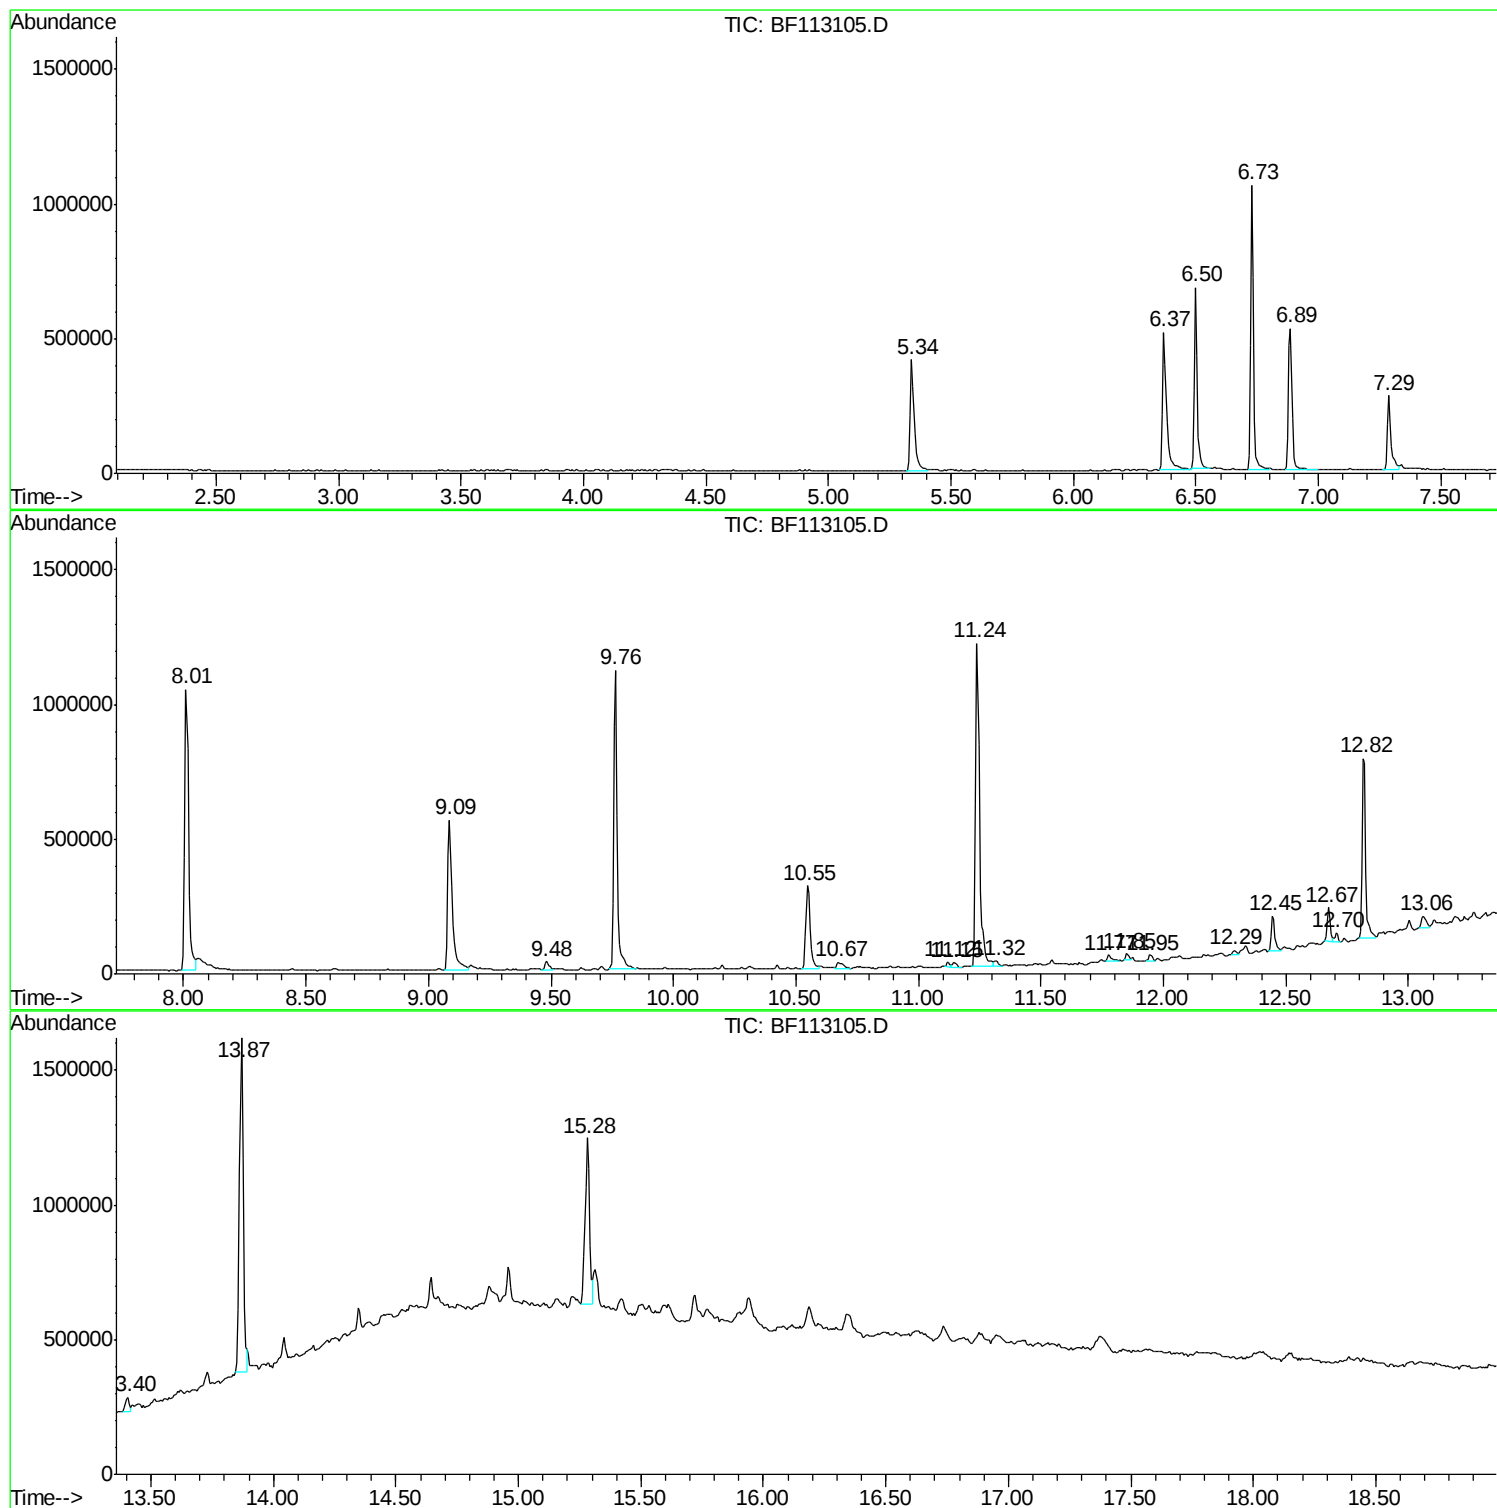

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF031819\
 Data File : BF113105.D
 Acq On : 18 Mar 2019 22:01
 Operator : JU/SJ
 Sample : K1691-17 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-031519-E










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
 TIC Integration Parameters: LSCINT.P

 Peak Number 1 unknown6.50 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.50	12.54 ng	575547	1,4-Dichlorobenzene-d4	6.73

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		Tranvlcypromine-propionyl	189	C12H15NO	1000123-86-3	10
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

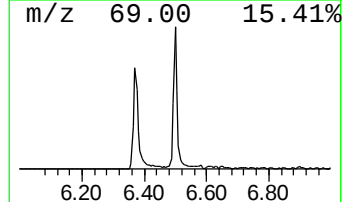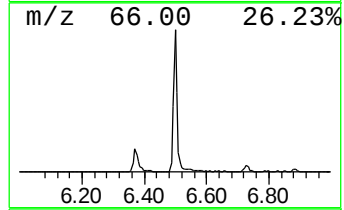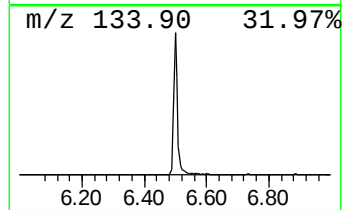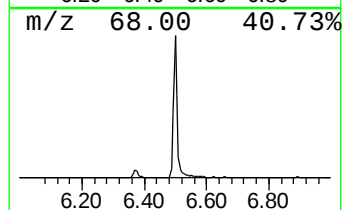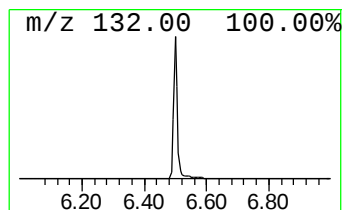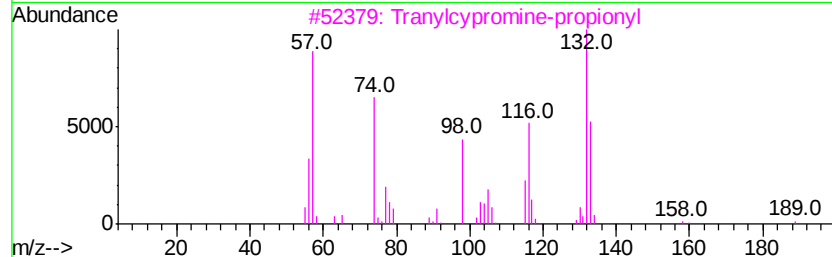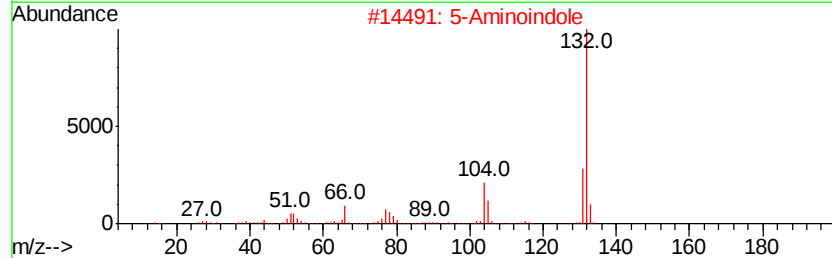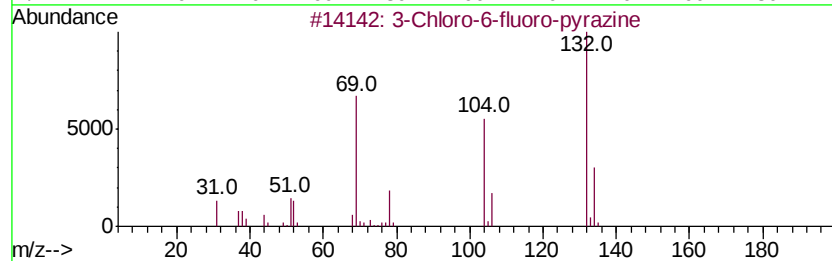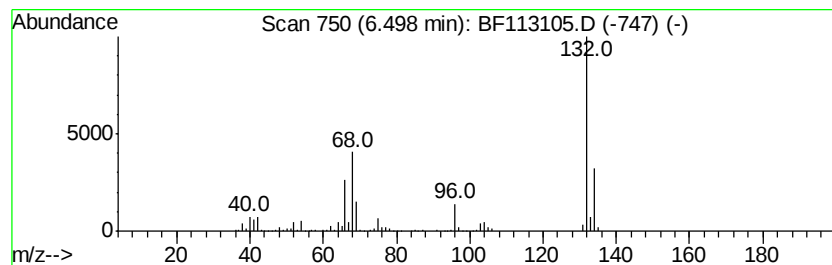

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031819\
Data File : BF113105.D
Acq On : 18 Mar 2019 22:01
Operator : JU/SJ
Sample : K1691-17 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-031519-E

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.50	6.50	12.5	ng	575547	1	6.73	918266	20.0