


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031819\
 Data File : BF113083.D
 Acq On : 18 Mar 2019 11:49
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 13 03:42:55 2019

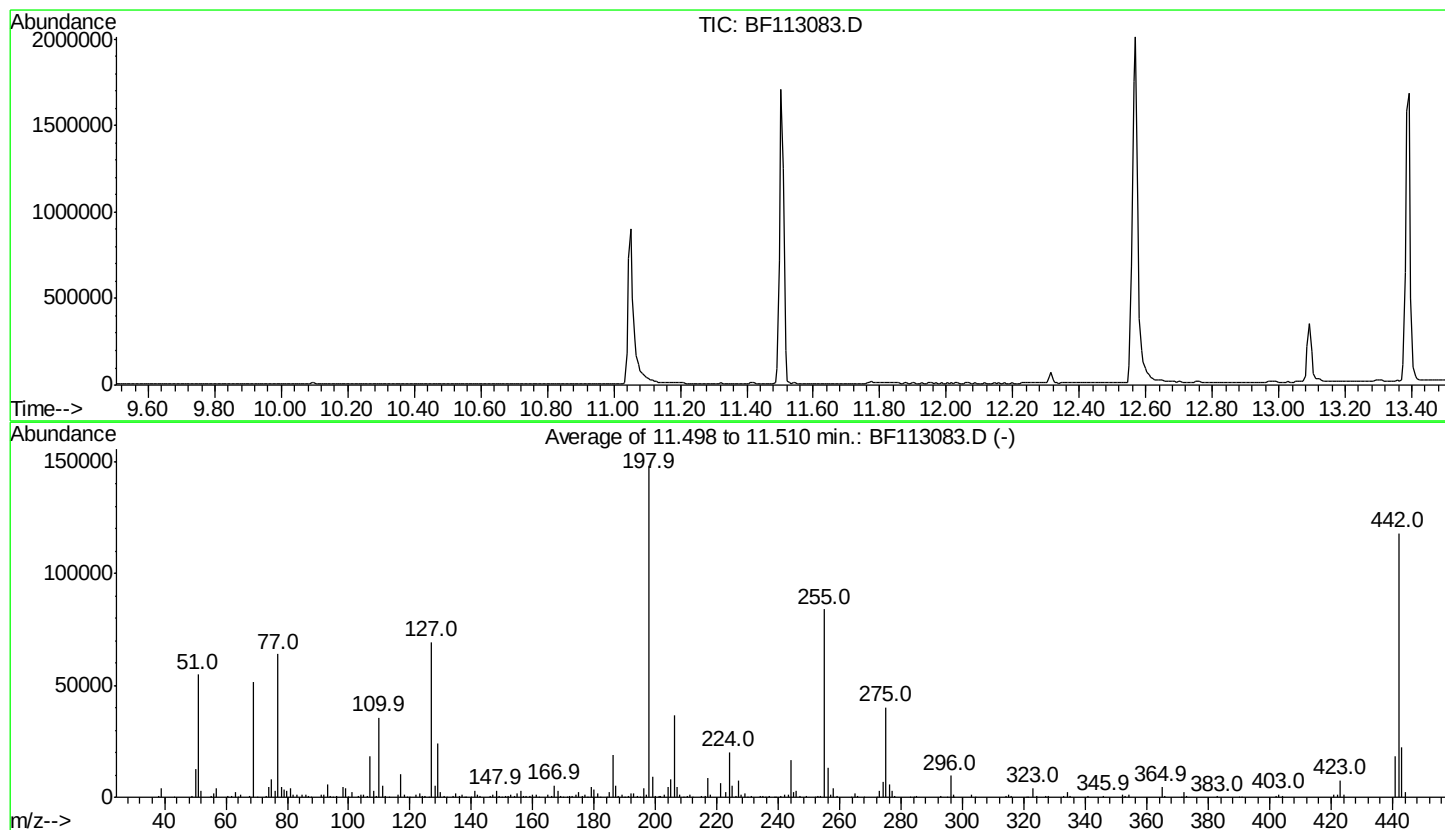

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	54893	PASS
68	69	0.00	2	1.5	796	PASS
69	198	0.00	100	34.9	51661	PASS
70	69	0.00	2	0.3	154	PASS
127	198	10	80	46.9	69450	PASS
197	198	0.00	2	0.6	937	PASS
198	198	100	100	100.0	148168	PASS
199	198	5	9	6.3	9402	PASS
275	198	10	60	27.1	40208	PASS
365	198	1	100	3.1	4659	PASS
441	198	0.01	100	12.4	18384	PASS
442	198	50	100	79.7	118090	PASS
443	442	15	24	19.0	22404	PASS