
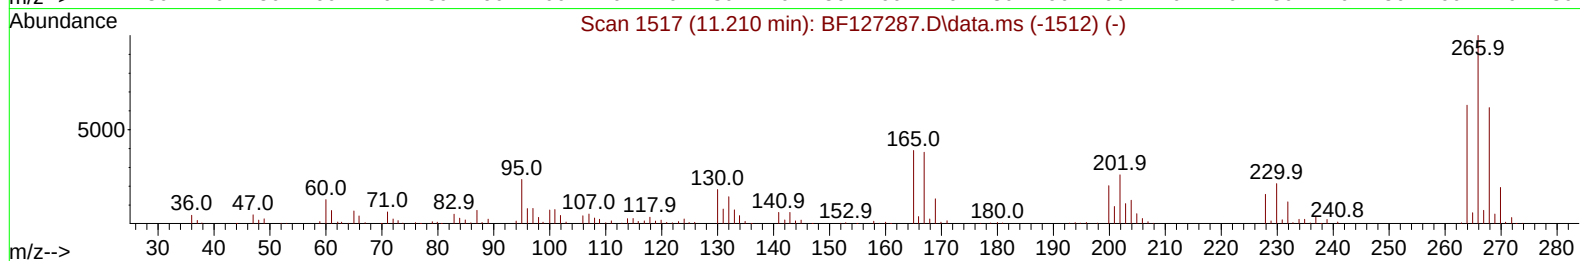
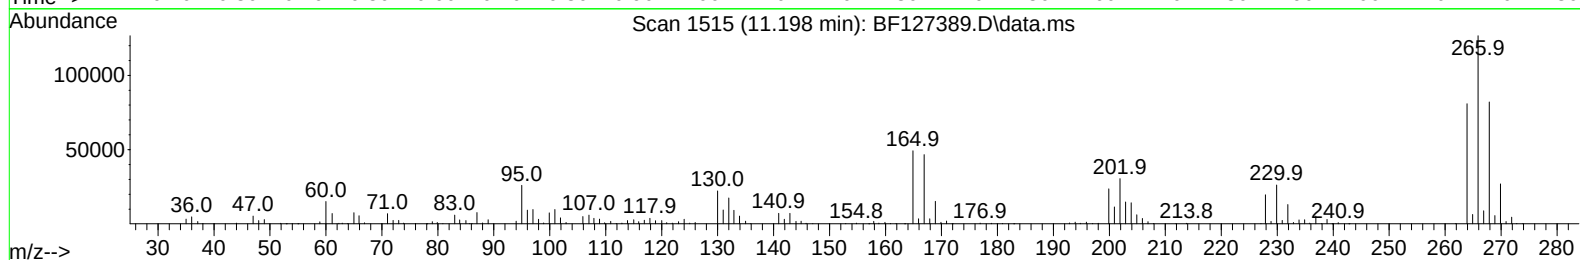


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031822\
Data File : BF127389.D
Acq On : 18 Mar 2022 13:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 03:21:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 19 01:50:04 2022
Response via : Initial Calibration

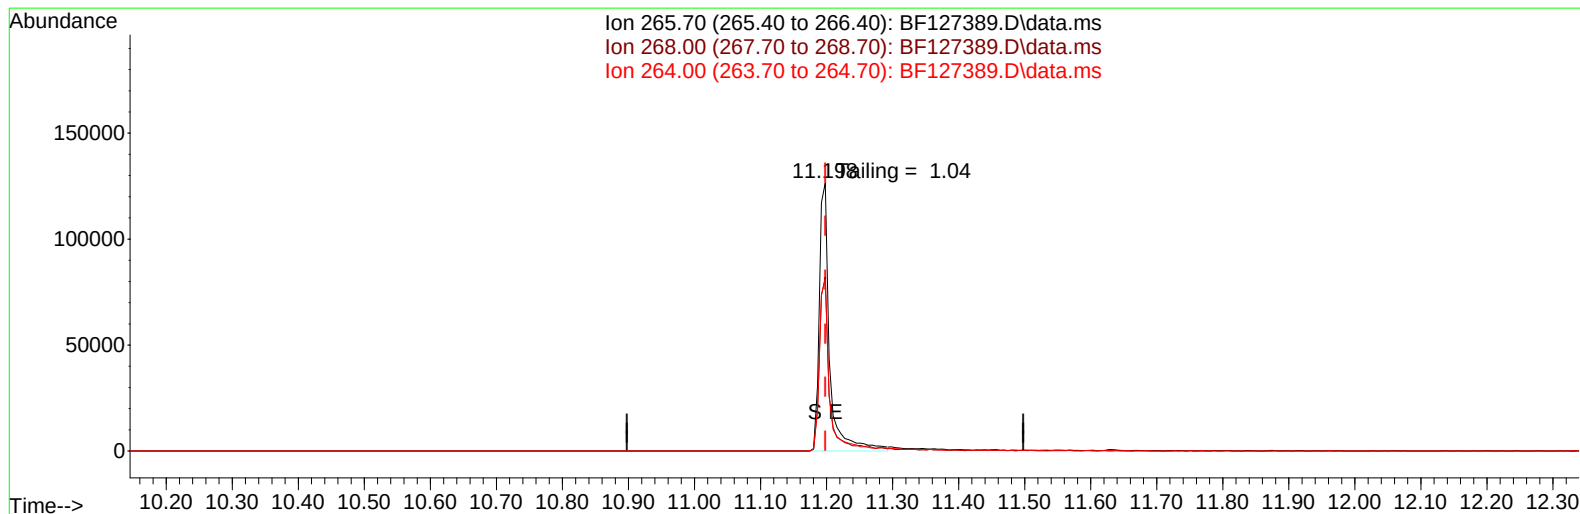

TIC: BF127389.D\data.ms




(70) Pentachlorophenol (C)

11.198min (-0.000) 31011.78 ng

response 143933

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	64.82
264.00	63.00	63.89
0.00	0.00	0.00

Quant Time: Mar 19 03:21:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 19 01:50:04 2022
Response via : Initial Calibration

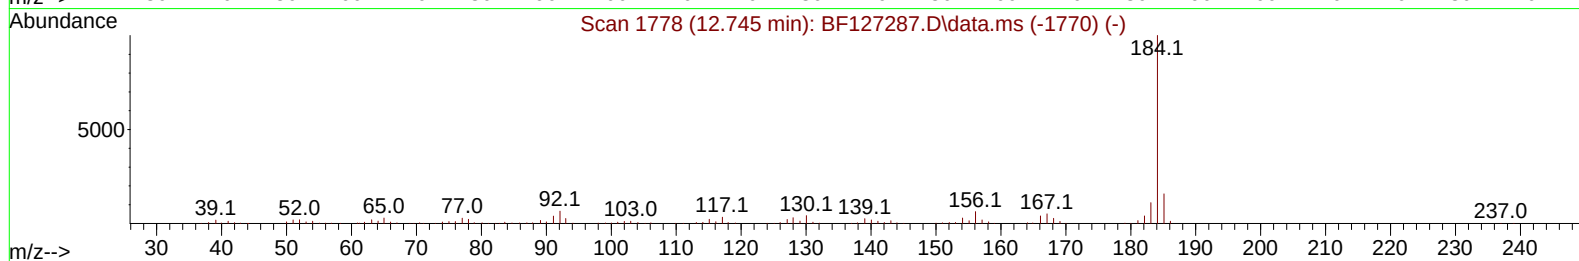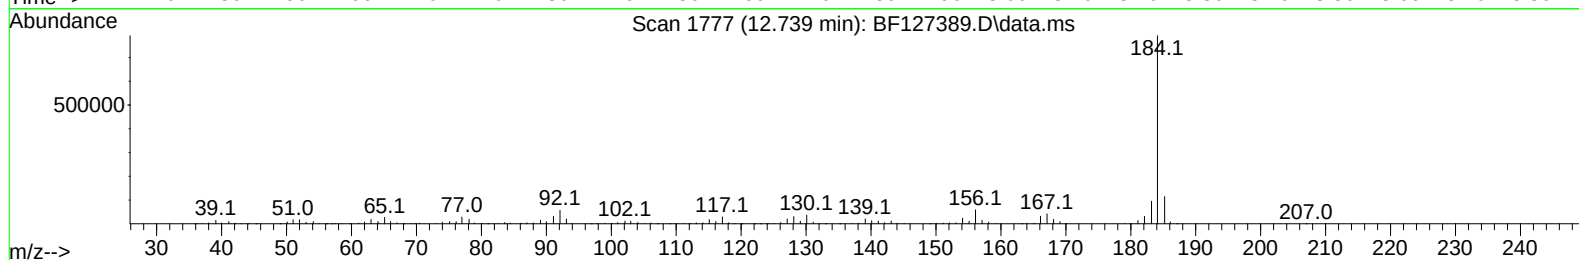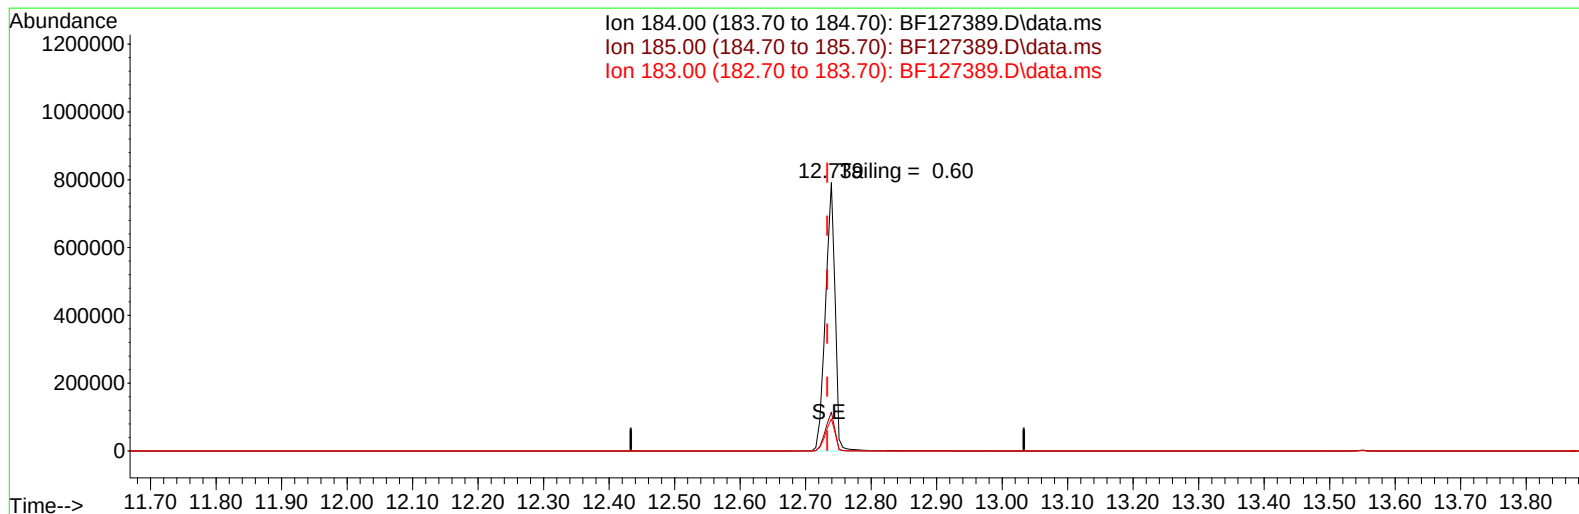

TIC: BF127389.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 0.00 ng

response **810537**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.50
183.00	10.20	12.01
0.00	0.00	0.00