

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031822\
 Data File : BF127392.D
 Acq On : 18 Mar 2022 15:22
 Operator : CG\JU
 Sample : N1949-15
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CP-BH1-031422-4-6-DUP

Quant Time: Mar 19 01:51:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 19 01:50:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.857	152	77353	20.000	ng	0.00
21) Naphthalene-d8	8.140	136	292202	20.000	ng	0.00
39) Acenaphthene-d10	9.898	164	178432	20.000	ng	0.00
64) Phenanthrene-d10	11.386	188	332084	20.000	ng	# 0.00
76) Chrysene-d12	14.033	240	238162	20.000	ng	#-0.01
86) Perylene-d12	15.522	264	188248	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.481	112	425071	88.339	ng	0.00
7) Phenol-d6	6.493	99	583632	88.170	ng	0.00
23) Nitrobenzene-d5	7.422	82	405817	57.356	ng	-0.01
42) 2,4,6-Tribromophenol	10.692	330	169547	88.269	ng	0.00
45) 2-Fluorobiphenyl	9.216	172	719734	57.028	ng	0.00
79) Terphenyl-d14	12.975	244	882893	63.835	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031822\
Data File : BF127392.D
Acq On : 18 Mar 2022 15:22
Operator : CG\JU
Sample : N1949-15
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CP-BH1-031422-4-6-DUP

Quant Time: Mar 19 01:51:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 19 01:50:04 2022
Response via : Initial Calibration



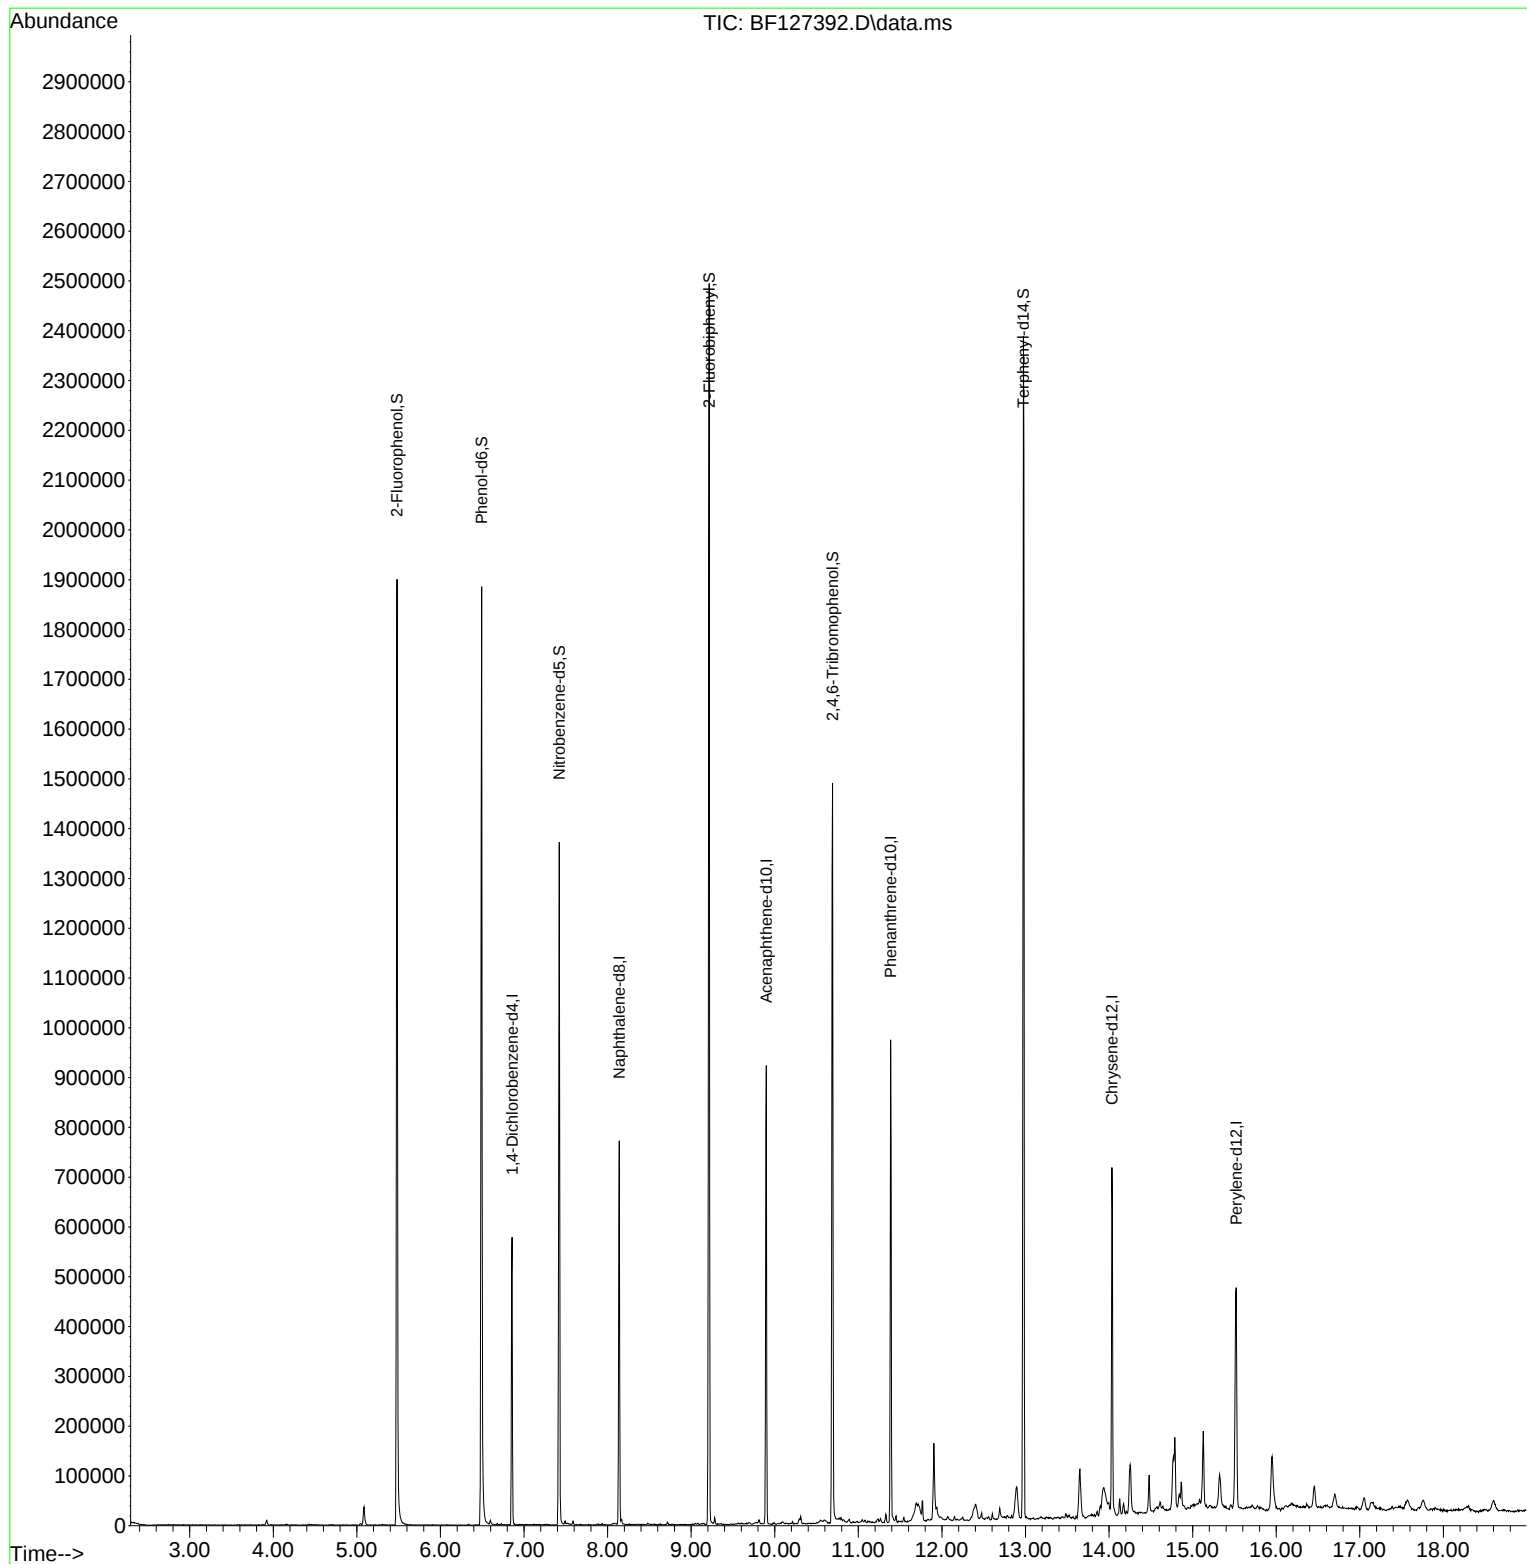


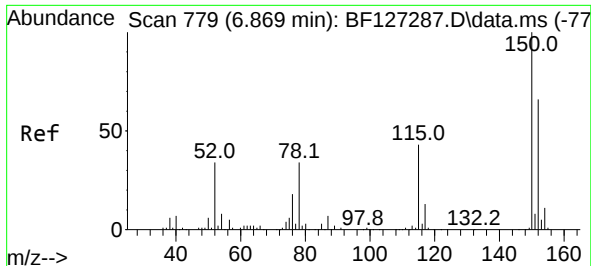

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.857 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF127392.D
Acq: 18 Mar 2022 15:22




Instrument :
BNA_F
ClientSampleId :
CP-BH1-031422-4-6-DUP


Tgt Ion:152 Resp: 77353
Ion Ratio Lower Upper
152 100
150 143.6 128.1 192.1
115 59.9 56.7 85.1

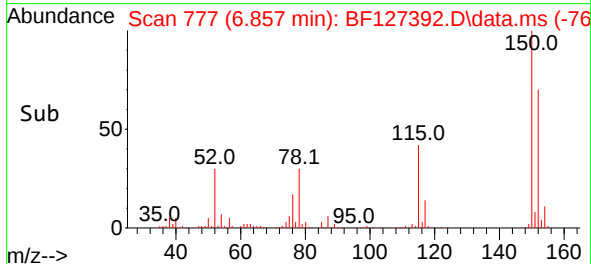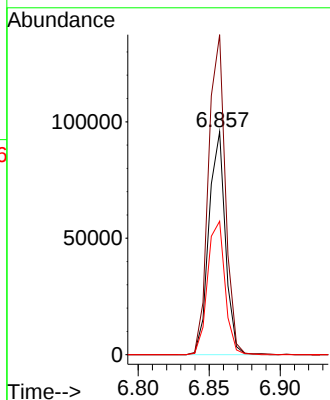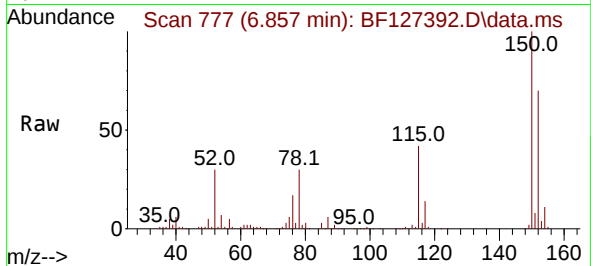

#5
2-Fluorophenol
Concen: 88.339 ng
RT: 5.481 min Scan# 543
Delta R.T. 0.000 min
Lab File: BF127392.D
Acq: 18 Mar 2022 15:22

Tgt Ion:112 Resp: 425071
Ion Ratio Lower Upper
112 100
64 77.2 49.5 74.3#
63 41.0 23.9 35.9#

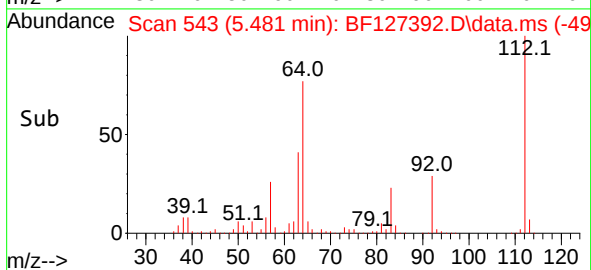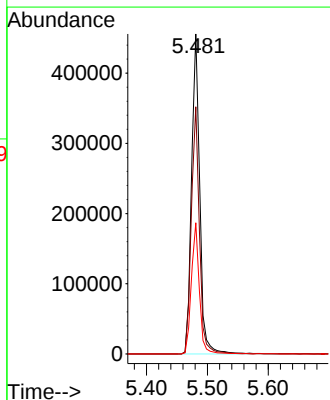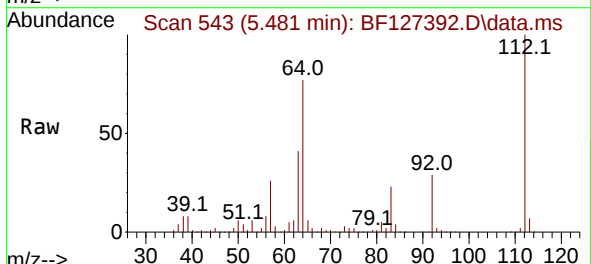

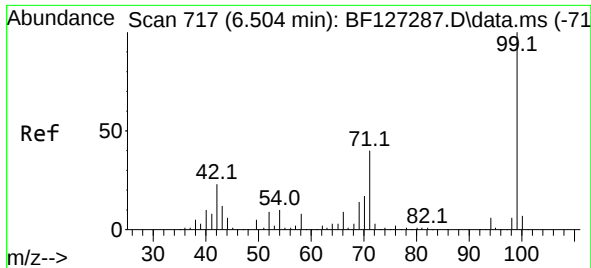

#7

Phenol-d6

Concen: 88.170 ng

RT: 6.493 min Scan# 71

Delta R.T. -0.006 min

Lab File: BF127392.D

Acq: 18 Mar 2022 15:22

Instrument :

BNA_F

ClientSampleId :

CP-BH1-031422-4-6-DUP





Tgt Ion: 99 Resp: 583632

Ion Ratio Lower Upper

99 100

42 23.8 14.2 21.4#

71 39.3 24.3 36.5#

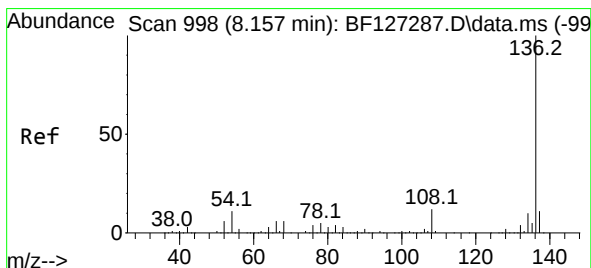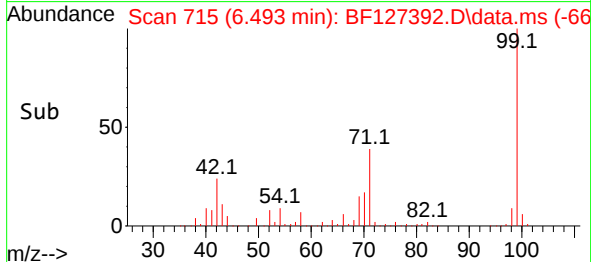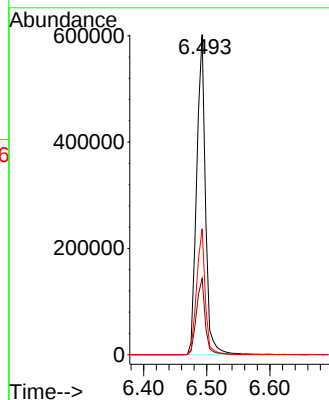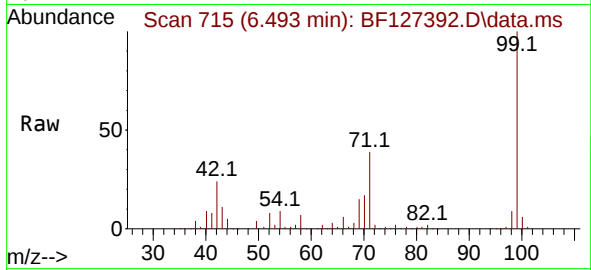

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.140 min Scan# 995

Delta R.T. -0.006 min

Lab File: BF127392.D

Acq: 18 Mar 2022 15:22

Tgt Ion: 136 Resp: 292202




Ion Ratio Lower Upper


136 100

137 10.7 8.6 13.0

54 11.1 7.8 11.6

68 6.4 6.3 9.5

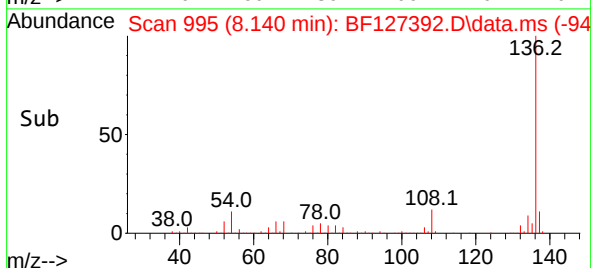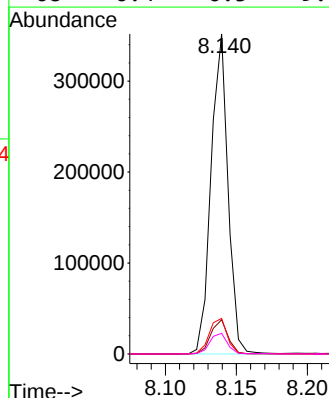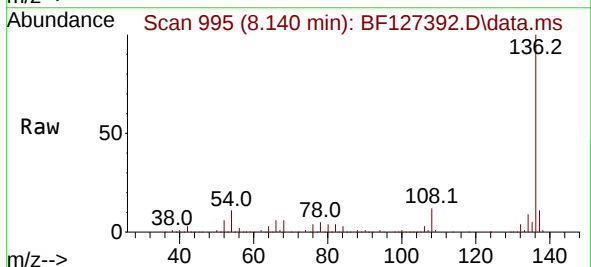

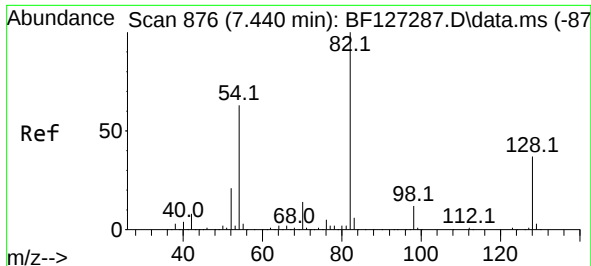

#23

Nitrobenzene-d5

Concen: 57.356 ng

RT: 7.422 min Scan# 81

Delta R.T. -0.012 min

Lab File: BF127392.D

Acq: 18 Mar 2022 15:22

Instrument :

BNA_F

ClientSampleId :

CP-BH1-031422-4-6-DUP





Tgt Ion: 82 Resp: 405817

Ion Ratio Lower Upper

82 100

128 36.8 32.7 49.1

54 62.9 41.7 62.5#

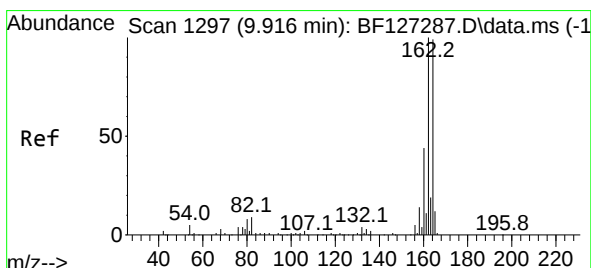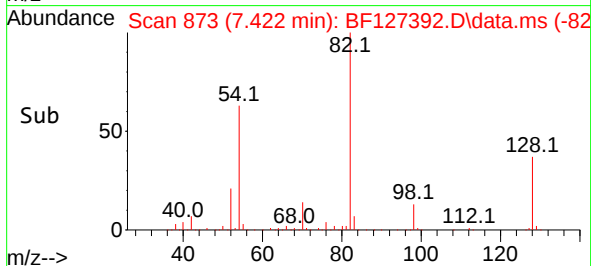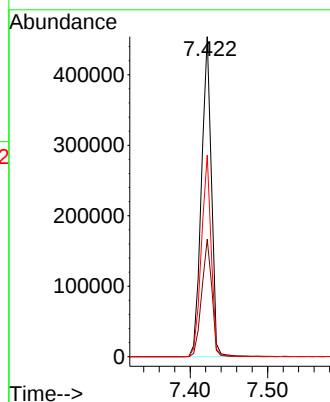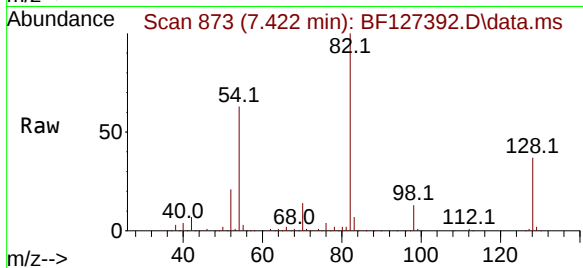

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.898 min Scan# 1294

Delta R.T. -0.006 min

Lab File: BF127392.D

Acq: 18 Mar 2022 15:22




Tgt Ion: 164 Resp: 178432


Ion Ratio Lower Upper

164 100

162 102.3 81.4 122.0

160 45.0 36.6 54.8

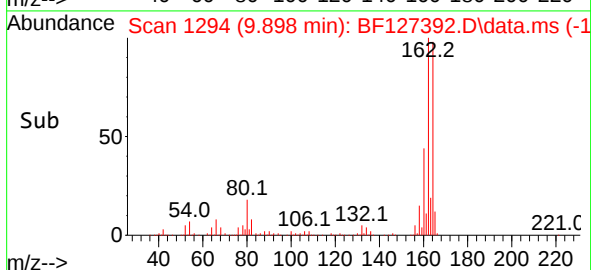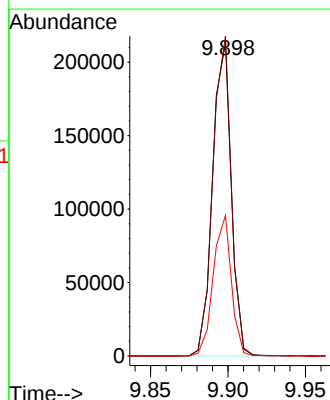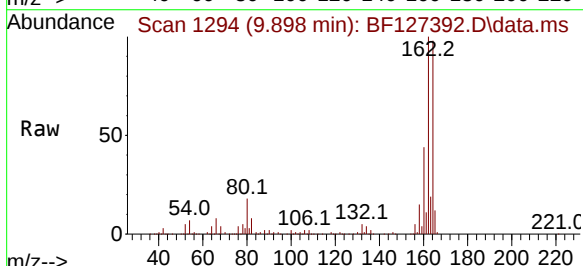

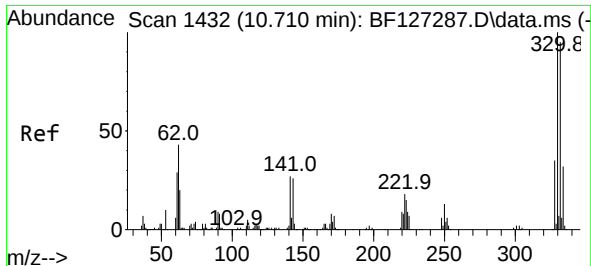

#42

2,4,6-Tribromophenol

Concen: 88.269 ng

RT: 10.692 min Scan# 1429

Delta R.T. -0.006 min

Lab File: BF127392.D


Acq: 18 Mar 2022 15:22

Instrument :

BNA_F

ClientSampleId :

CP-BH1-031422-4-6-DUP

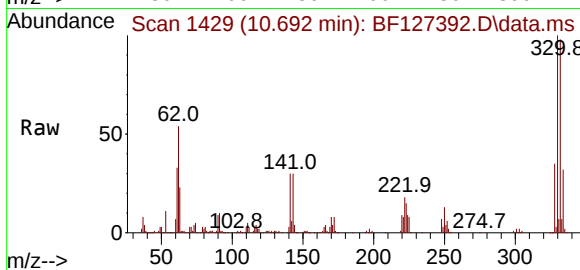




Tgt Ion:330 Resp: 169547

Ion Ratio Lower Upper

330 100

332 96.4 76.0 114.0

141 33.5 30.1 45.1

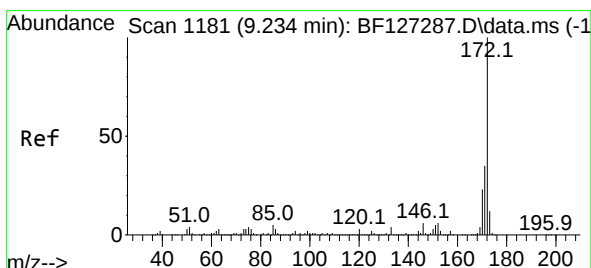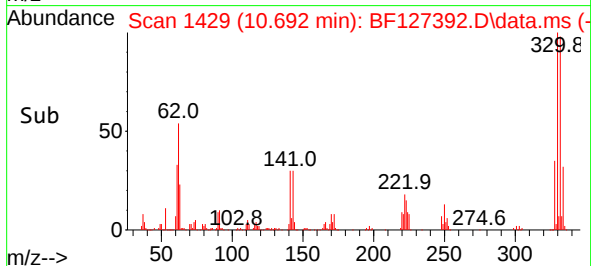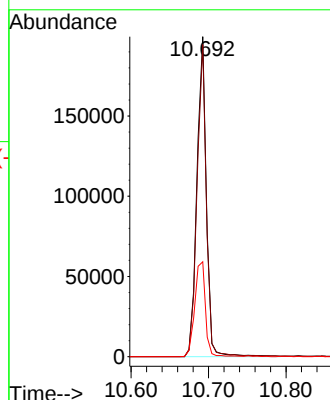

#45

2-Fluorobiphenyl

Concen: 57.028 ng

RT: 9.216 min Scan# 1178

Delta R.T. -0.006 min

Lab File: BF127392.D

Acq: 18 Mar 2022 15:22




Tgt Ion:172 Resp: 719734


Ion Ratio Lower Upper

172 100

171 35.7 28.3 42.5

170 23.4 19.0 28.6


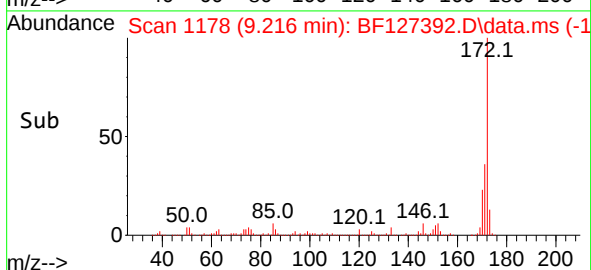
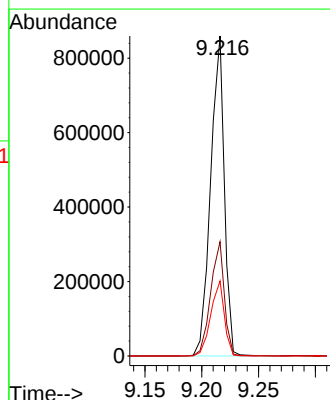
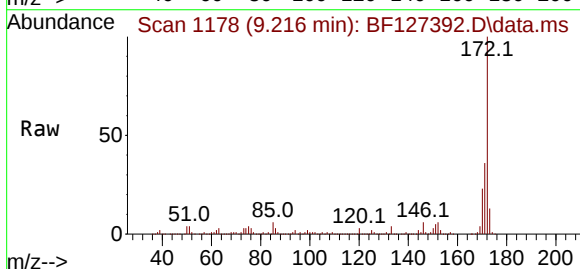


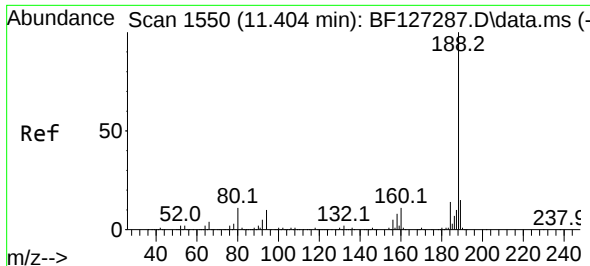

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.386 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF127392.D
Acq: 18 Mar 2022 15:22




Instrument :
BNA_F
ClientSampleId :
CP-BH1-031422-4-6-DUP


Tgt Ion:188 Resp: 332084
Ion Ratio Lower Upper
188 100
94 9.8 10.1 15.1#
80 10.7 11.8 17.6#

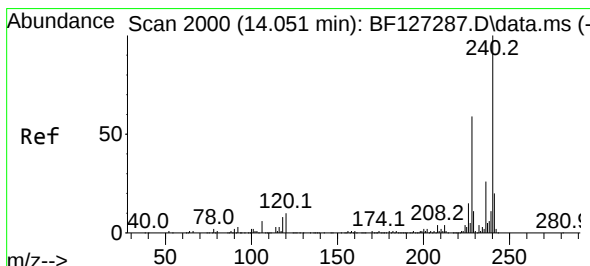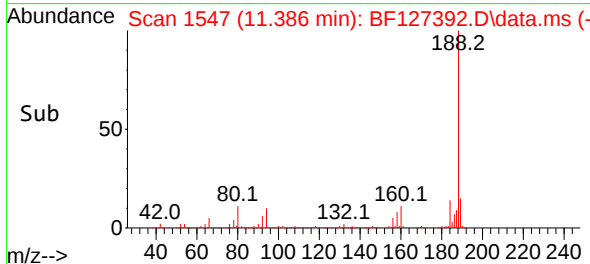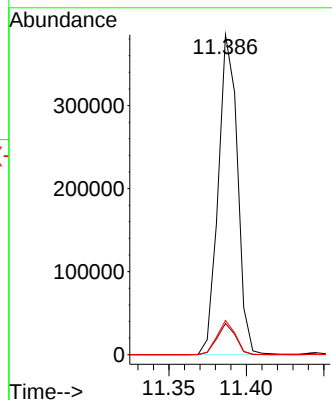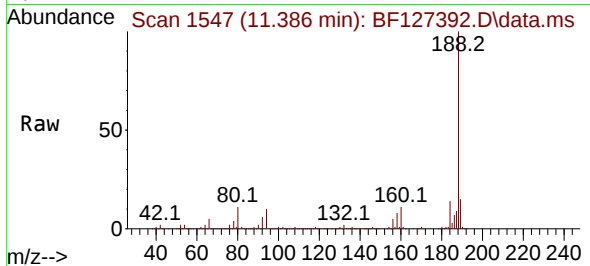

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.033 min Scan# 1997
Delta R.T. -0.012 min
Lab File: BF127392.D
Acq: 18 Mar 2022 15:22


Tgt Ion:240 Resp: 238162
Ion Ratio Lower Upper
240 100
120 8.3 14.4 21.6#
236 26.9 20.5 30.7

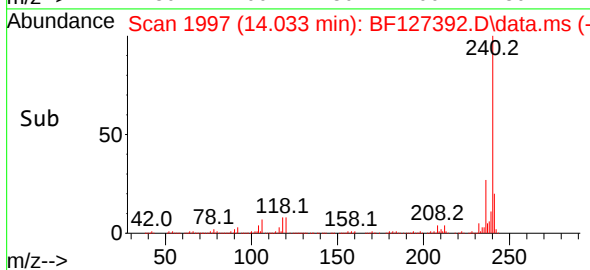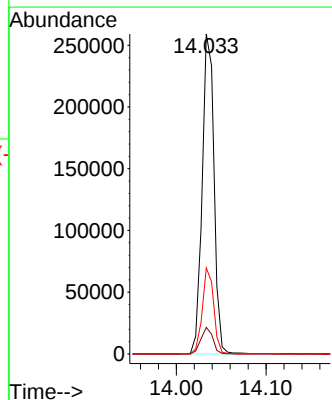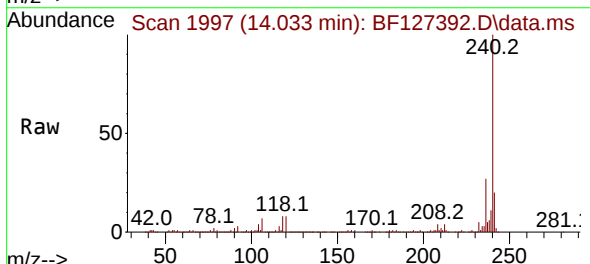



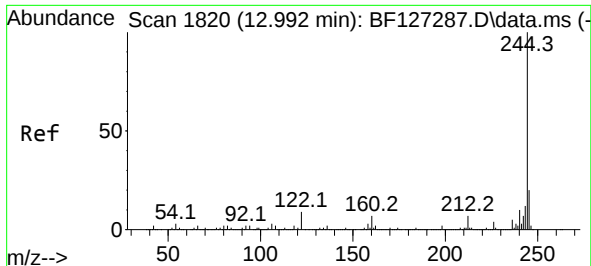


#79
 Terphenyl-d14
 Concen: 63.835 ng
 RT: 12.975 min Scan# 1817
 Delta R.T. -0.006 min
 Lab File: BF127392.D
 Acq: 18 Mar 2022 15:22

Instrument :
 BNA_F
 ClientSampleId :
 CP-BH1-031422-4-6-DUP

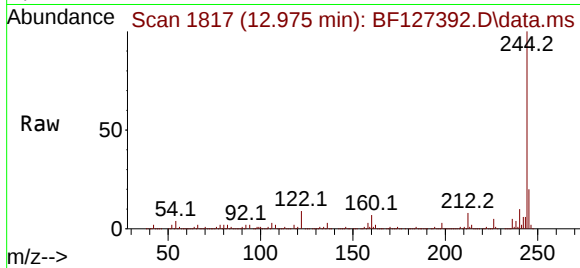

Tgt Ion:244 Resp: 882893
 Ion Ratio Lower Upper
 244 100
 212 7.6 5.0 7.4#
 122 9.4 13.3 19.9#

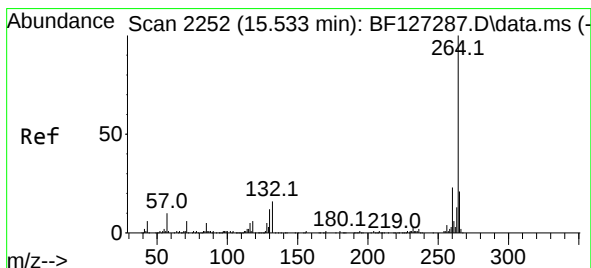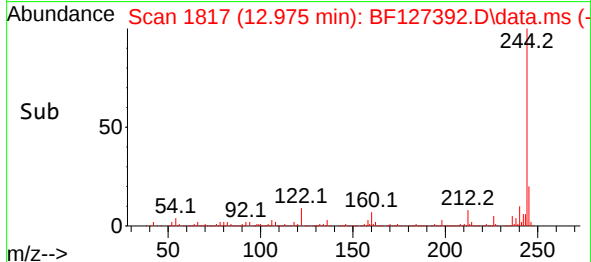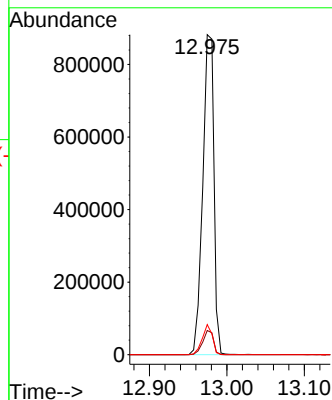

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.522 min Scan# 2250
 Delta R.T. 0.000 min
 Lab File: BF127392.D
 Acq: 18 Mar 2022 15:22

Tgt Ion:264 Resp: 188248
 Ion Ratio Lower Upper
 264 100
 260 23.5 19.2 28.8
 265 20.8 17.4 26.2

