

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031822\
 Data File : BF127397.D
 Acq On : 18 Mar 2022 17:50
 Operator : CG\JU
 Sample : N1709-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PPSP-B8-30.0-30.5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127397.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.087	473	476	482	rBV	27074	33901	1.36%	0.205%
2	5.481	539	543	559	rBV	1783804	1828565	73.42%	11.050%
3	6.492	710	715	731	rBV	1956981	1957202	78.58%	11.827%
4	6.857	773	777	783	rBV	562691	483251	19.40%	2.920%
5	6.910	783	786	793	rBV	46962	45380	1.82%	0.274%
6	7.422	869	873	876	rBV	1487186	1258424	50.52%	7.605%
7	8.045	976	979	991	rBV	29545	81039	3.25%	0.490%
8	8.139	991	995	998	rBV	832777	633266	25.43%	3.827%
9	9.216	1172	1178	1181	rBV	2607017	2219446	89.11%	13.412%
10	9.480	1220	1223	1231	rBV	247280	208196	8.36%	1.258%
11	9.892	1290	1293	1297	rBV	859660	778895	31.27%	4.707%
12	10.292	1356	1361	1362	rBV	32241	27939	1.12%	0.169%
13	10.686	1424	1428	1432	rBV	1551817	1487212	59.71%	8.987%
14	11.327	1534	1537	1540	rVB	63615	46747	1.88%	0.282%
15	11.386	1543	1547	1551	rBV	1021757	857285	34.42%	5.181%
16	11.545	1571	1574	1581	rBV2	37069	40253	1.62%	0.243%
17	11.763	1608	1611	1615	rVB	46123	40480	1.63%	0.245%
18	11.904	1631	1635	1639	rBV2	38468	46138	1.85%	0.279%
19	11.939	1639	1641	1646	rVB	34869	31772	1.28%	0.192%
20	12.151	1674	1677	1680	rBV	91628	68529	2.75%	0.414%
21	12.527	1738	1741	1744	rBV	66104	53810	2.16%	0.325%
22	12.974	1812	1817	1820	rBV	2745569	2490711	100.00%	15.051%
23	13.957	1974	1984	1988	rBV9	14538	51921	2.08%	0.314%
24	14.033	1993	1997	2001	rVB	763854	654496	26.28%	3.955%
25	14.339	2046	2049	2052	rBV	52354	42979	1.73%	0.260%
26	14.786	2122	2125	2129	rVB	32188	32094	1.29%	0.194%
27	14.862	2135	2138	2142	rBV	52839	52058	2.09%	0.315%
28	15.127	2179	2183	2188	rVB	42680	46553	1.87%	0.281%
29	15.515	2243	2249	2260	rVB	495536	663617	26.64%	4.010%
30	15.945	2317	2322	2327	rVB	52514	75247	3.02%	0.455%
31	16.456	2403	2409	2414	rBV	43344	75012	3.01%	0.453%
32	17.051	2504	2510	2520	rVB4	33080	72843	2.92%	0.440%
33	17.756	2625	2630	2642	rVB4	26261	62982	2.53%	0.381%




Sum of corrected areas: 16548243

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031822\
Data File : BF127397.D
Acq On : 18 Mar 2022 17:50
Operator : CG\JU
Sample : N1709-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PPSP-B8-30.0-30.5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

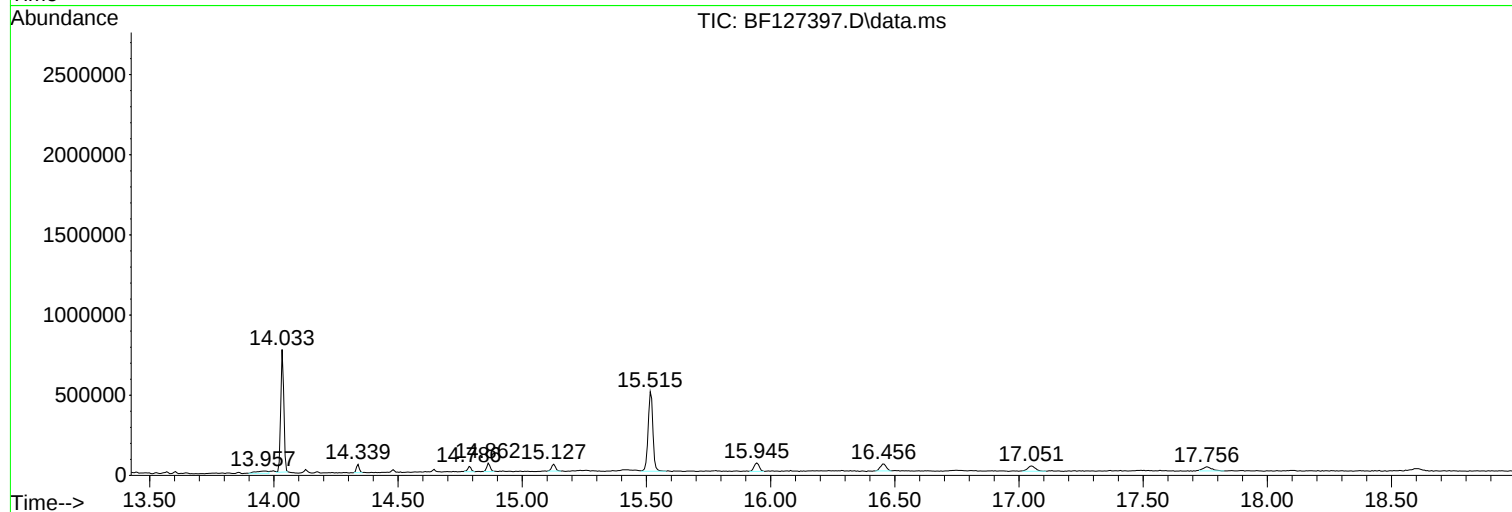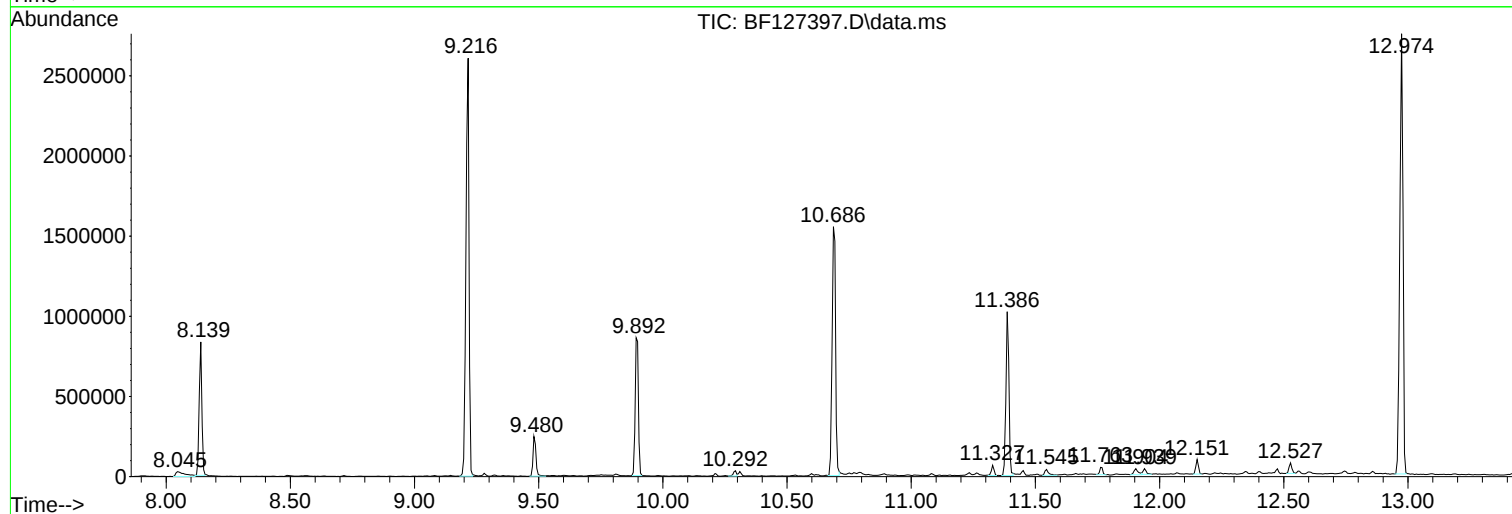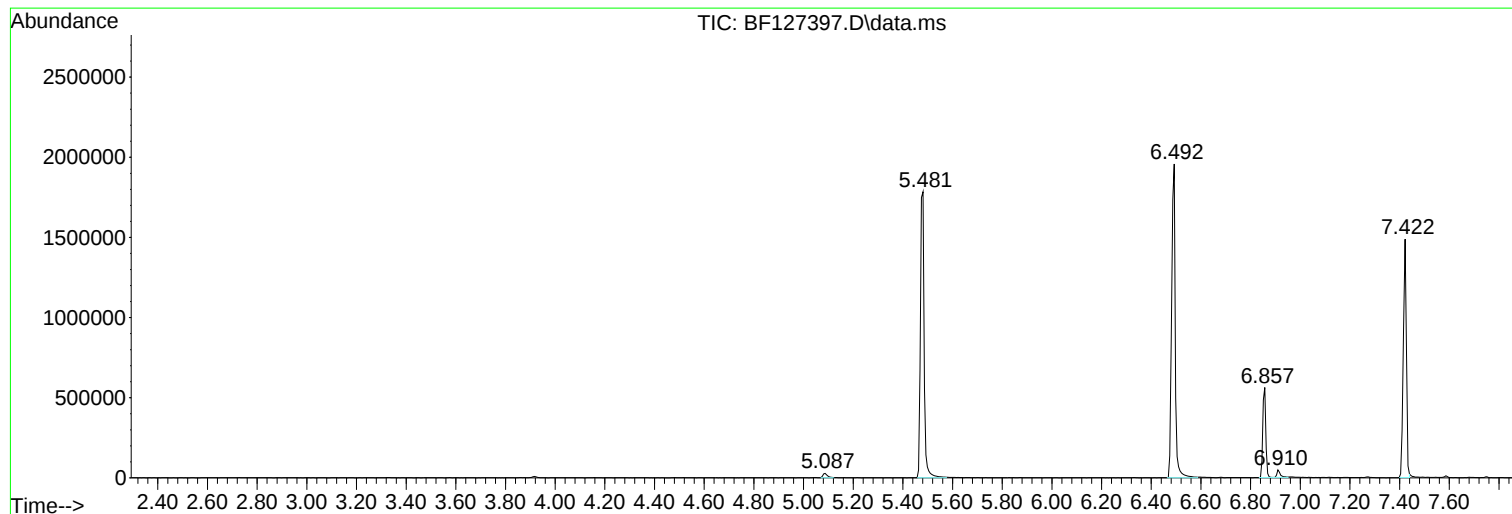

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031822\
Data File : BF127397.D
Acq On : 18 Mar 2022 17:50
Operator : CG\JU
Sample : N1709-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PPSP-B8-30.0-30.5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031822\
Data File : BF127397.D
Acq On : 18 Mar 2022 17:50
Operator : CG\JU
Sample : N1709-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PPSP-B8-30.0-30.5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------