

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031822\
 Data File : BF127404.D
 Acq On : 18 Mar 2022 21:17
 Operator : CG\JU
 Sample : N1709-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PPSP-B17-23.5-24.0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127404.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.893	439	443	449	rVB	266455	316725	3.37%	0.135%
2	4.975	449	457	459	rBV2	370454	548832	5.85%	0.234%
3	5.004	459	462	466	rVB	329613	376100	4.01%	0.161%
4	5.057	466	471	474	rBV	559410	630781	6.72%	0.270%
5	5.257	499	505	508	rBV2	612071	851789	9.07%	0.364%
6	5.287	508	510	514	rVB3	189260	224887	2.40%	0.096%
7	5.340	514	519	521	rBV2	590721	653474	6.96%	0.279%
8	5.363	521	523	526	rVV	522076	399178	4.25%	0.171%
9	5.440	533	536	539	rVV	940908	877582	9.35%	0.375%
10	5.475	539	542	550	rVB	2223194	2363068	25.17%	1.010%
11	5.540	550	553	556	rBV	319939	316778	3.37%	0.135%
12	5.616	563	566	571	rBV3	550294	898336	9.57%	0.384%
13	5.663	571	574	577	rVV	993886	844082	8.99%	0.361%
14	5.704	577	581	587	rVV2	789416	1069062	11.39%	0.457%
15	5.757	587	590	597	rVB	1879523	1964789	20.93%	0.839%
16	5.875	603	610	613	rBV3	1286918	1799404	19.17%	0.769%
17	5.916	613	617	621	rBV3	786718	1347794	14.36%	0.576%
18	6.010	628	633	637	rVB3	1372185	2328816	24.81%	0.995%
19	6.051	637	640	643	rBV2	734752	816009	8.69%	0.349%
20	6.104	643	649	655	rBV2	3228029	5525376	58.86%	2.361%
21	6.157	655	658	660	rVB2	1933323	1774380	18.90%	0.758%
22	6.193	660	664	666	rBV3	522566	688305	7.33%	0.294%
23	6.216	666	668	670	rVB	443758	360001	3.83%	0.154%
24	6.240	670	672	676	rVB2	493608	506574	5.40%	0.216%
25	6.293	676	681	683	rBV2	2052022	2777610	29.59%	1.187%
26	6.334	683	688	689	rBV2	792889	1250330	13.32%	0.534%
27	6.351	689	691	694	rVB	2106481	2085888	22.22%	0.891%
28	6.387	694	697	700	rBV2	3375510	4311792	45.93%	1.842%
29	6.446	704	707	709	rBV	2019157	1854468	19.75%	0.792%
30	6.498	712	716	719	rVB2	1688300	1974691	21.03%	0.844%
31	6.534	719	722	723	rBV	785224	686673	7.31%	0.293%
32	6.604	728	734	738	rBV6	1774219	3755250	40.00%	1.604%
33	6.634	738	739	745	rVB3	1603977	2073765	22.09%	0.886%
34	6.693	745	749	752	rBV3	4487773	5834926	62.15%	2.493%
35	6.746	756	758	760	rBV2	569693	536637	5.72%	0.229%
36	6.798	760	767	768	rBV6	1032791	1980694	21.10%	0.846%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031822\
 Data File : BF127404.D
 Acq On : 18 Mar 2022 21:17
 Operator : CG\JU
 Sample : N1709-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PPSP-B17-23.5-24.0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	6.816	768	770	773	rBV2	967269	1053655	11.22%	0.450%
38	6.846	773	775	776	rBV	475520	379714	4.04%	0.162%
39	6.875	776	780	784	rVB2	3594585	4956863	52.80%	2.118%
40	6.916	784	787	790	rBV2	1434396	1720394	18.33%	0.735%
41	6.975	790	797	800	rBV6	1337279	2503705	26.67%	1.070%
42	7.010	800	803	807	rVB4	2454501	2845960	30.31%	1.216%
43	7.046	807	809	811	rVB	1164128	942899	10.04%	0.403%
44	7.093	814	817	818	rBV	1129441	1149438	12.24%	0.491%
45	7.116	818	821	822	rBV	1040185	941830	10.03%	0.402%
46	7.140	822	825	828	rVB2	2812221	3055498	32.55%	1.306%
47	7.193	831	834	835	rBV	1206231	991310	10.56%	0.424%
48	7.257	840	845	849	rBV3	3891846	6103854	65.02%	2.608%
49	7.340	855	859	861	rBV2	1364019	1824637	19.44%	0.780%
50	7.363	861	863	865	rVV	1712706	1485095	15.82%	0.635%
51	7.410	865	871	874	rVV2	4582513	6998983	74.55%	2.990%
52	7.440	874	876	880	rVV4	3010011	3647978	38.86%	1.559%
53	7.516	883	889	892	rBV5	3372222	5649569	60.18%	2.414%
54	7.581	892	900	904	rBV3	2413464	5682361	60.53%	2.428%
55	7.651	909	912	914	rVV2	2177151	2875732	30.63%	1.229%
56	7.675	914	916	926	rVB4	3550170	5304240	56.50%	2.266%
57	7.757	926	930	931	rBV2	2093151	2412916	25.70%	1.031%
58	7.781	932	934	935	rVV2	1492073	1388734	14.79%	0.593%
59	7.798	935	937	941	rVV3	1821216	2575871	27.44%	1.101%
60	7.840	941	944	947	rVB3	1786805	2493664	26.56%	1.065%
61	7.875	947	950	952	rBV4	1562046	1708541	18.20%	0.730%
62	7.904	952	955	958	rVV4	1922220	2812716	29.96%	1.202%
63	7.957	962	964	965	rBV	829185	626223	6.67%	0.268%
64	8.034	974	977	980	rVB2	1393773	1471362	15.67%	0.629%
65	8.122	986	992	994	rBV5	2310662	4311387	45.92%	1.842%
66	8.187	1001	1003	1006	rBV2	1331737	1609707	17.15%	0.688%
67	8.216	1006	1008	1013	rVB2	1794380	2685343	28.60%	1.147%
68	8.369	1031	1034	1039	rVB2	2612923	3392191	36.13%	1.449%
69	8.416	1039	1042	1044	rBV	1278713	1236386	13.17%	0.528%
70	8.457	1044	1049	1056	rBV5	2374422	6068613	64.64%	2.593%
71	8.687	1084	1088	1094	rBV4	2307103	4510016	48.04%	1.927%
72	9.210	1172	1177	1183	rVB5	2749836	5094074	54.26%	2.177%
73	9.822	1278	1281	1284	rBV2	1812707	2111706	22.49%	0.902%
74	10.063	1318	1322	1326	rBV2	2055481	4088331	43.55%	1.747%
75	10.210	1343	1347	1354	rVB3	3635475	7319831	77.97%	3.128%
76	10.281	1354	1359	1361	rBV	2866924	4805732	51.19%	2.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031822\
 Data File : BF127404.D
 Acq On : 18 Mar 2022 21:17
 Operator : CG\JU
 Sample : N1709-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PPSP-B17-23.5-24.0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	10.369	1370	1374	1377	rBV3	1951310	3745282	39.89%	1.600%
78	10.745	1436	1438	1442	rBV5	1046690	1641516	17.49%	0.701%
79	10.869	1452	1459	1465	rVB3	4705881	9388076	100.00%	4.011%
80	11.328	1533	1537	1543	rVB4	3592859	6054224	64.49%	2.587%
81	11.475	1558	1562	1568	rVB	2609108	4356892	46.41%	1.862%
82	11.663	1592	1594	1606	rVB8	1979289	4705530	50.12%	2.011%
83	11.945	1638	1642	1645	rBV	1954884	3283510	34.98%	1.403%
84	12.057	1658	1661	1663	rBV	1670024	1862725	19.84%	0.796%
85	12.086	1663	1666	1668	rVB	1922477	2029827	21.62%	0.867%
86	12.175	1678	1681	1684	rVB2	1295415	1409918	15.02%	0.602%
87	12.380	1714	1716	1719	rVB2	1397390	1293672	13.78%	0.553%
88	12.416	1719	1722	1724	rVB	1361583	1250556	13.32%	0.534%
89	12.439	1724	1726	1729	rVB	1126508	859714	9.16%	0.367%
90	12.492	1731	1735	1737	rBV	2529715	3022191	32.19%	1.291%
91	12.569	1746	1748	1751	rBV	970242	1098640	11.70%	0.469%
92	12.792	1784	1786	1788	rBV2	499757	448719	4.78%	0.192%
93	12.822	1789	1791	1795	rVB4	912657	872182	9.29%	0.373%
94	12.886	1798	1802	1805	rVB3	1349575	1746156	18.60%	0.746%
95	12.927	1805	1809	1812	rVB	1432161	1577580	16.80%	0.674%
96	12.969	1813	1816	1819	rVB2	795545	924744	9.85%	0.395%
97	13.004	1819	1822	1824	rVB2	1826512	1599575	17.04%	0.683%
98	13.386	1885	1887	1890	rBV2	220189	272599	2.90%	0.116%
99	14.045	1996	1999	2011	rVB	504172	654056	6.97%	0.279%
100	15.521	2244	2250	2259	rVB	367473	506877	5.40%	0.217%


Sum of corrected areas: 234046666

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031822\
Data File : BF127404.D
Acq On : 18 Mar 2022 21:17
Operator : CG\JU
Sample : N1709-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PPSP-B17-23.5-24.0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

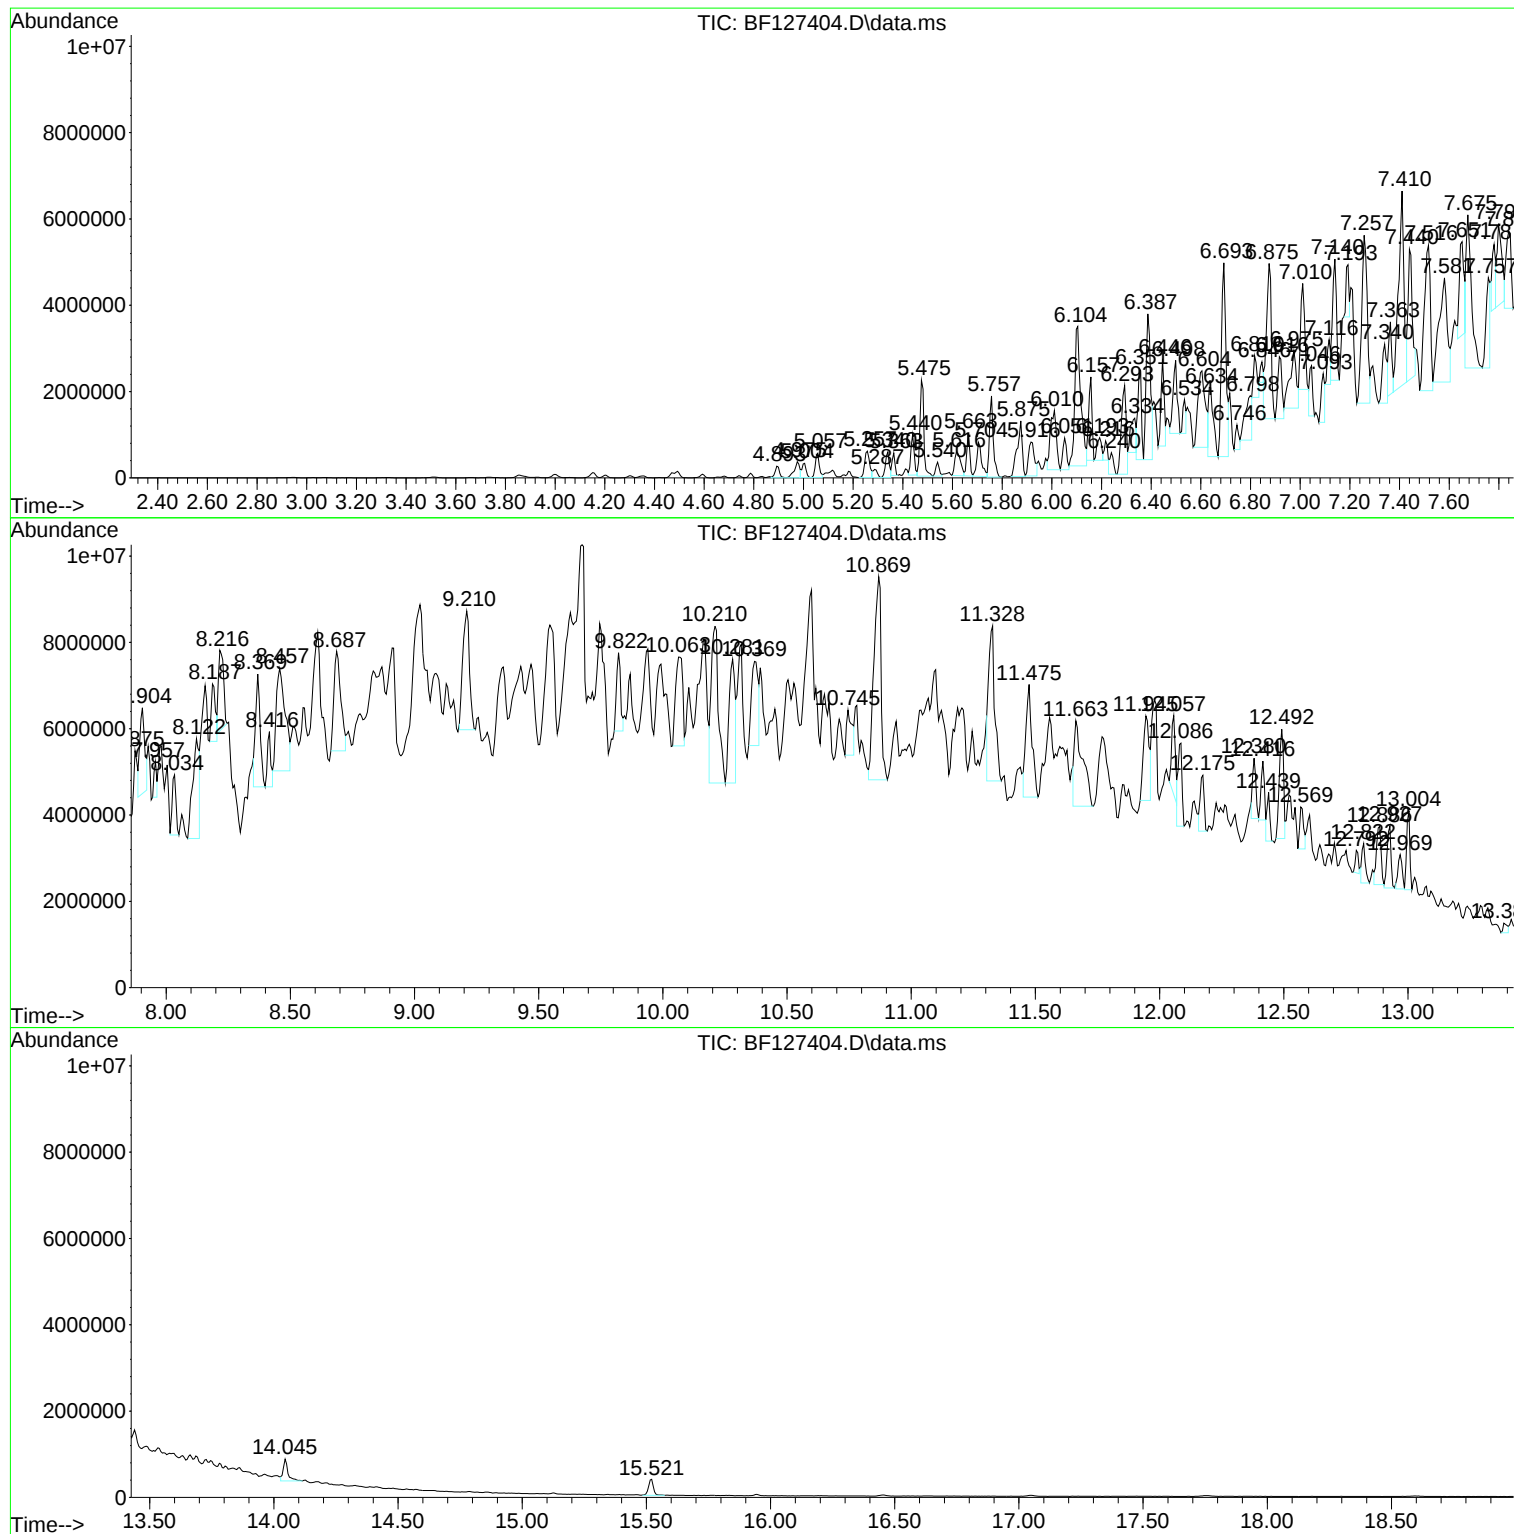

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031822\
Data File : BF127404.D
Acq On : 18 Mar 2022 21:17
Operator : CG\JU
Sample : N1709-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PPSP-B17-23.5-24.0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031822\
Data File : BF127404.D
Acq On : 18 Mar 2022 21:17
Operator : CG\JU
Sample : N1709-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PPSP-B17-23.5-24.0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------