


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031822\
 Data File : BF127389.D
 Acq On : 18 Mar 2022 13:51
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 19 01:50:04 2022

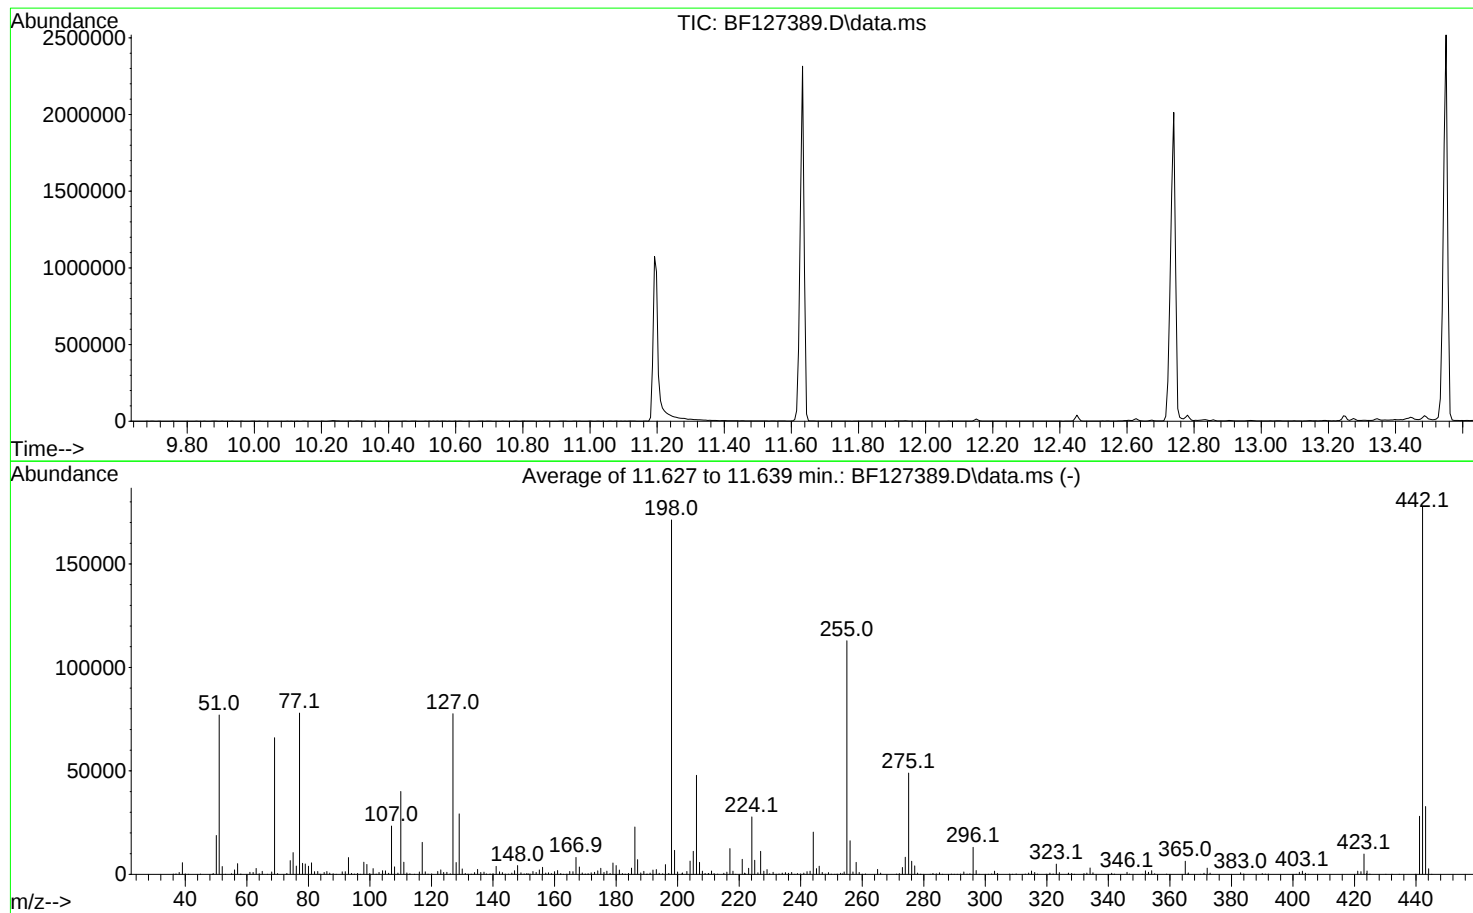




AutoFind: Scans 1588, 1589, 1590; Background Corrected with Scan 1582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	76997	PASS
68	69	0.00	2	1.8	1186	PASS
69	198	0.00	100	38.6	66029	PASS
70	69	0.00	2	0.5	358	PASS
127	198	10	80	45.3	77645	PASS
197	198	0.00	2	0.3	486	PASS
198	198	100	100	100.0	171277	PASS
199	198	5	9	6.8	11603	PASS
275	198	10	60	28.6	48971	PASS
365	198	1	100	3.7	6342	PASS
441	198	0.01	100	16.4	28039	PASS
442	442	50	100	100.0	177747	PASS
443	442	15	24	18.5	32819	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031822\
Data File : BF127389.D
Acq On : 18 Mar 2022 13:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 19 03:21:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 19 01:50:04 2022
Response via : Initial Calibration

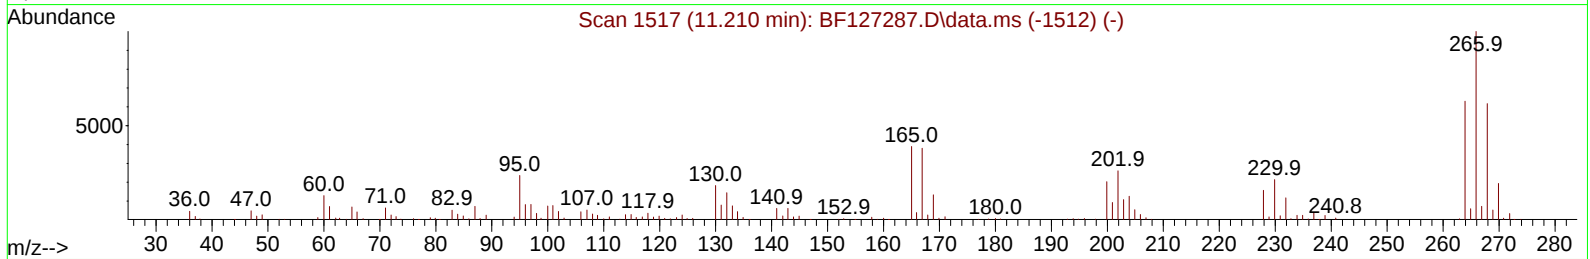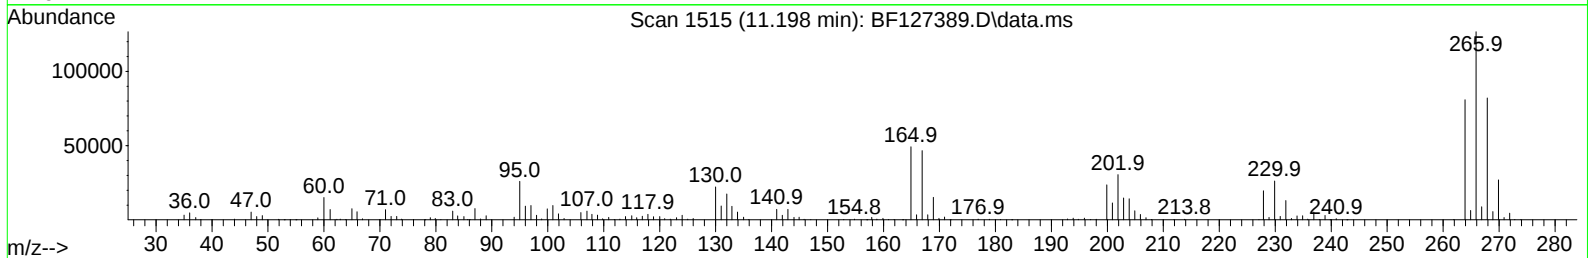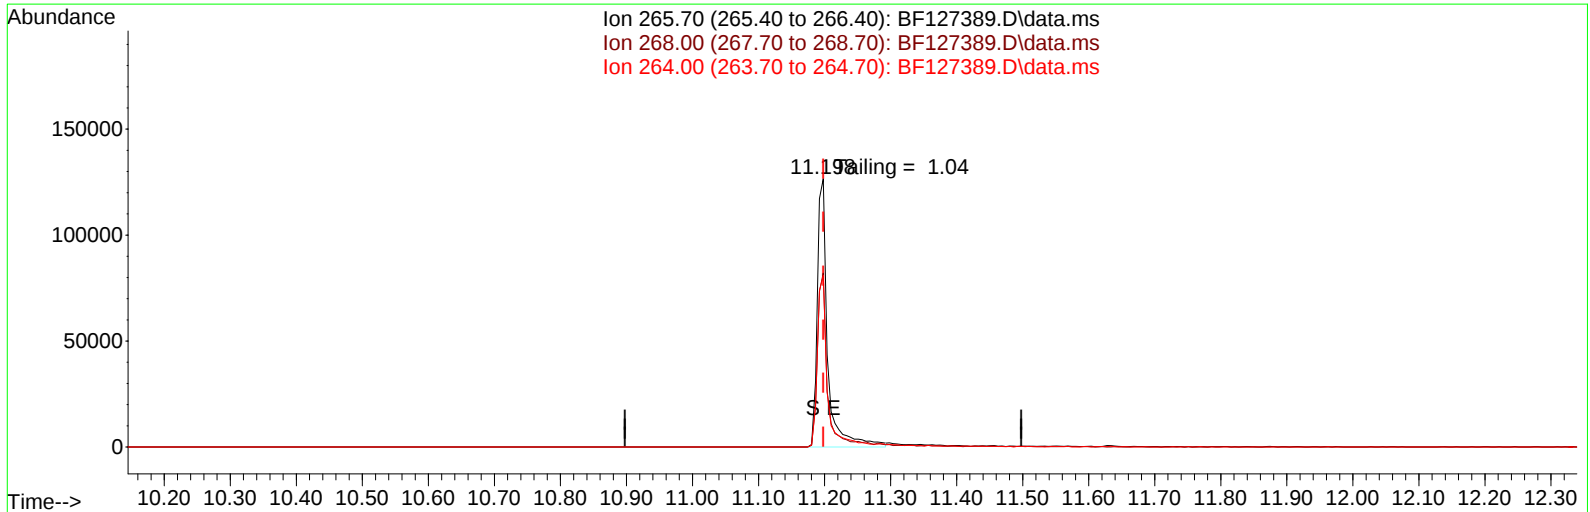

TIC: BF127389.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.000) 31011.78 ng




response 143933

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	64.82
264.00	63.00	63.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031822\
 Data File : BF127389.D
 Acq On : 18 Mar 2022 13:51
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 19 03:21:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 19 01:50:04 2022
 Response via : Initial Calibration

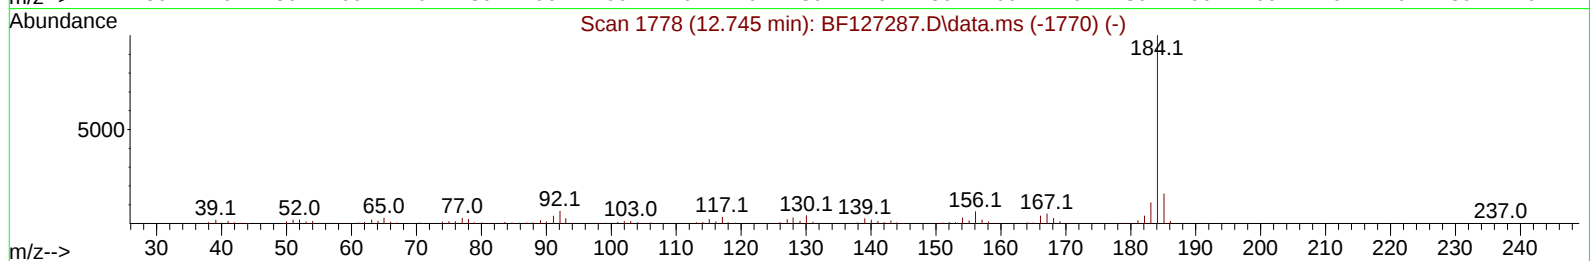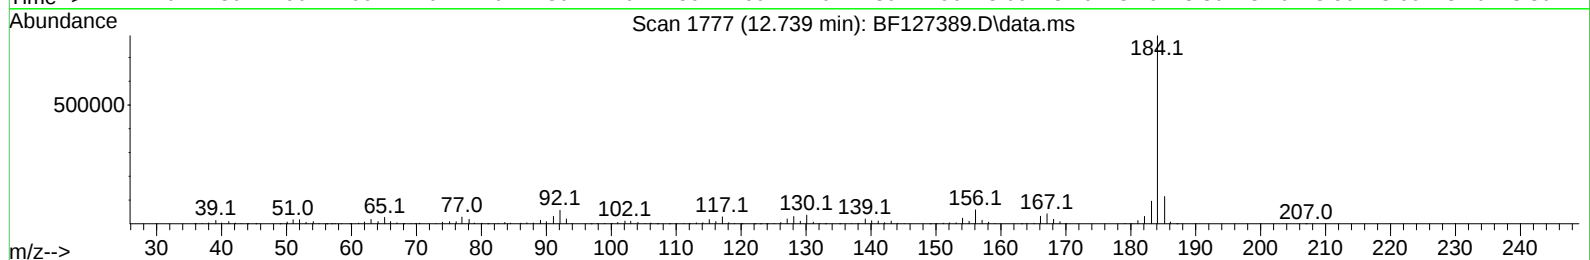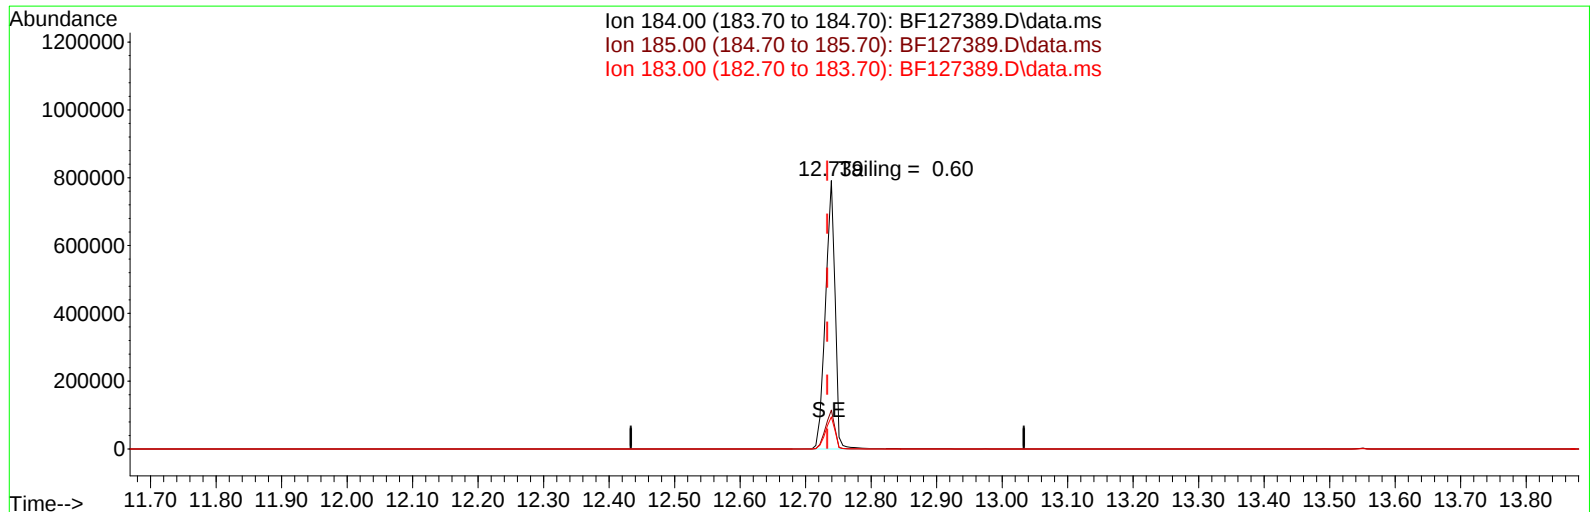

TIC: BF127389.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 0.00 ng

response 810537

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.50
183.00	10.20	12.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/18/2022	BNA_F	<u>BF127389.D</u>
Compound Name	Response	Retention Time
DDT	434556	13.551
DDD	9349	13.245
DDE	384	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9733	444289	2.19

Instrument :
BNA_F
ClientSampleId :
DFTPP