
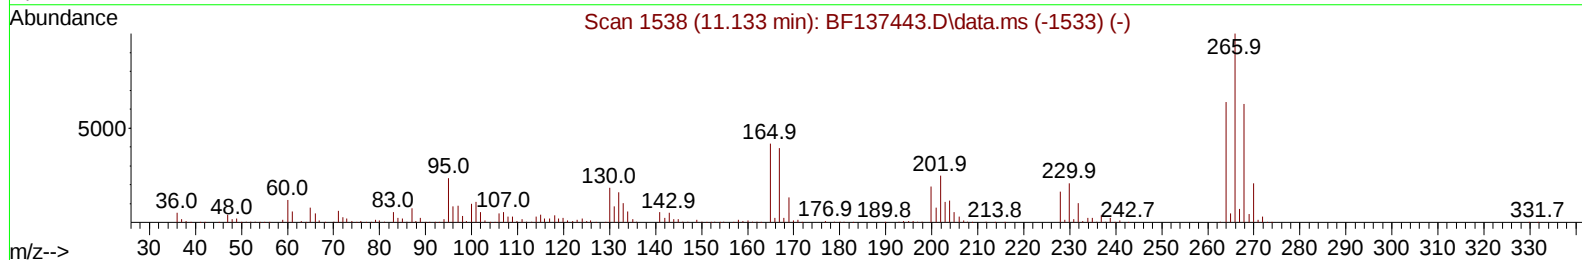
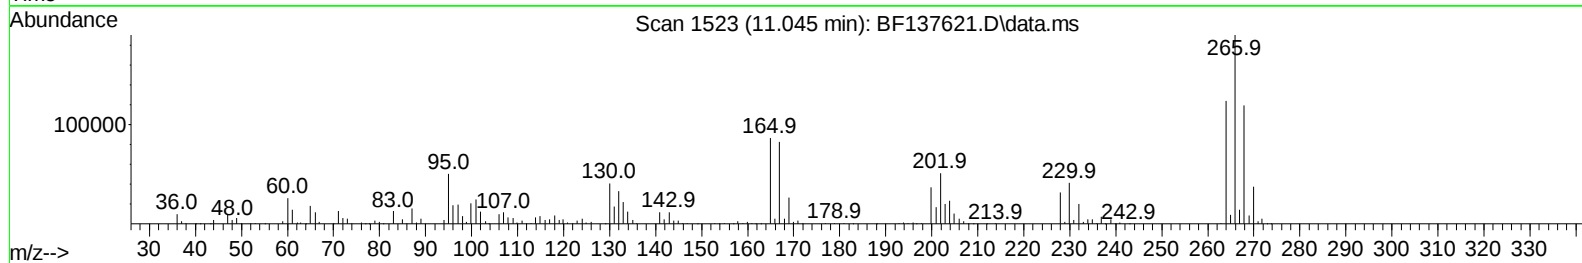


Quant Time: Mar 18 23:55:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

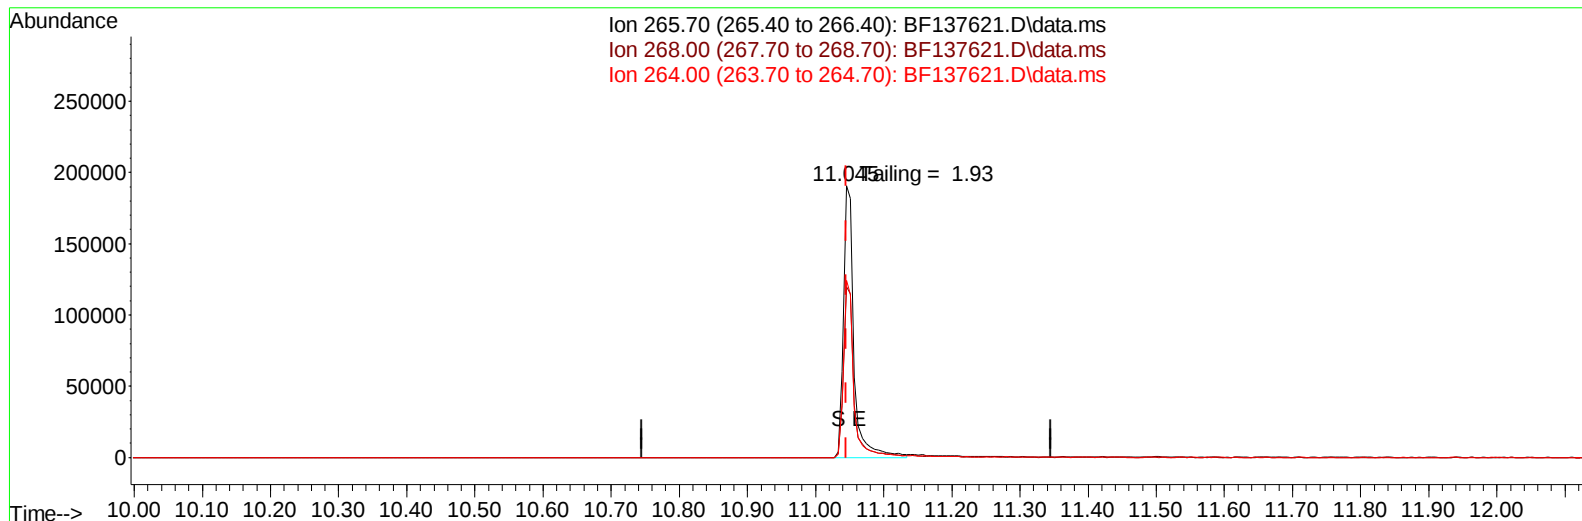

TIC: BF137621.D\data.ms

(70) Pentachlorophenol (C)




11.045min (-0.000) 576294.26 ng

response 203122

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.75
264.00	63.60	65.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031824\
Data File : BF137621.D
Acq On : 18 Mar 2024 10:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 23:55:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

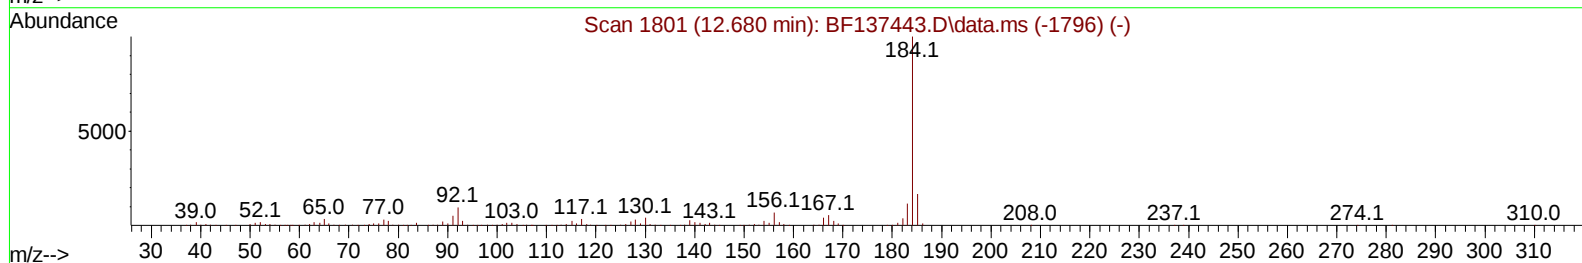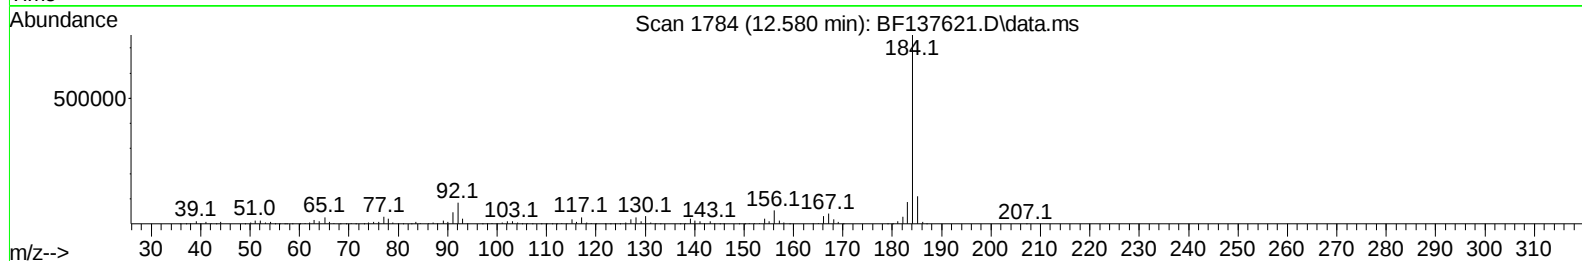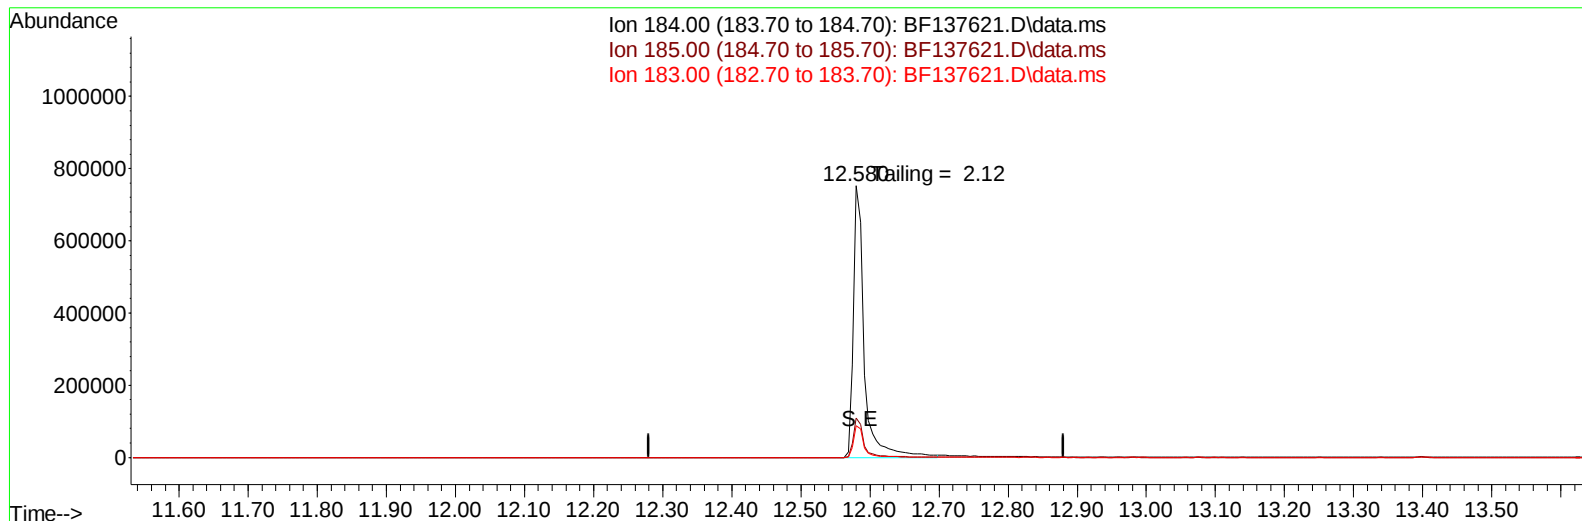

TIC: BF137621.D\data.ms

(77) Benzidine

12.580min (-12.580) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	16.50	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00