

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031824\
 Data File : BF137626.D
 Acq On : 18 Mar 2024 12:34
 Operator : CG\JU
 Sample : PB159633BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB159633BL

Quant Time: Mar 18 13:01:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 14 14:45:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.728	152	213196	20.000	ng	0.00
21) Naphthalene-d8	8.004	136	822536	20.000	ng	0.00
39) Acenaphthene-d10	9.757	164	435299	20.000	ng	0.00
64) Phenanthrene-d10	11.239	188	746900	20.000	ng	0.00
76) Chrysene-d12	13.874	240	480906	20.000	ng	0.00
86) Perylene-d12	15.298	264	393200	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.351	112	1607131	114.170	ng	0.02
7) Phenol-d6	6.369	99	2166776	106.637	ng	0.00
23) Nitrobenzene-d5	7.292	82	1360954	76.879	ng	0.00
42) 2,4,6-Tribromophenol	10.551	330	478011	125.046	ng	0.00
45) 2-Fluorobiphenyl	9.086	172	2175969	78.249	ng	0.00
79) Terphenyl-d14	12.833	244	2424967	69.340	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031824\
Data File : BF137626.D
Acq On : 18 Mar 2024 12:34
Operator : CG\JU
Sample : PB159633BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159633BL

Quant Time: Mar 18 13:01:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration




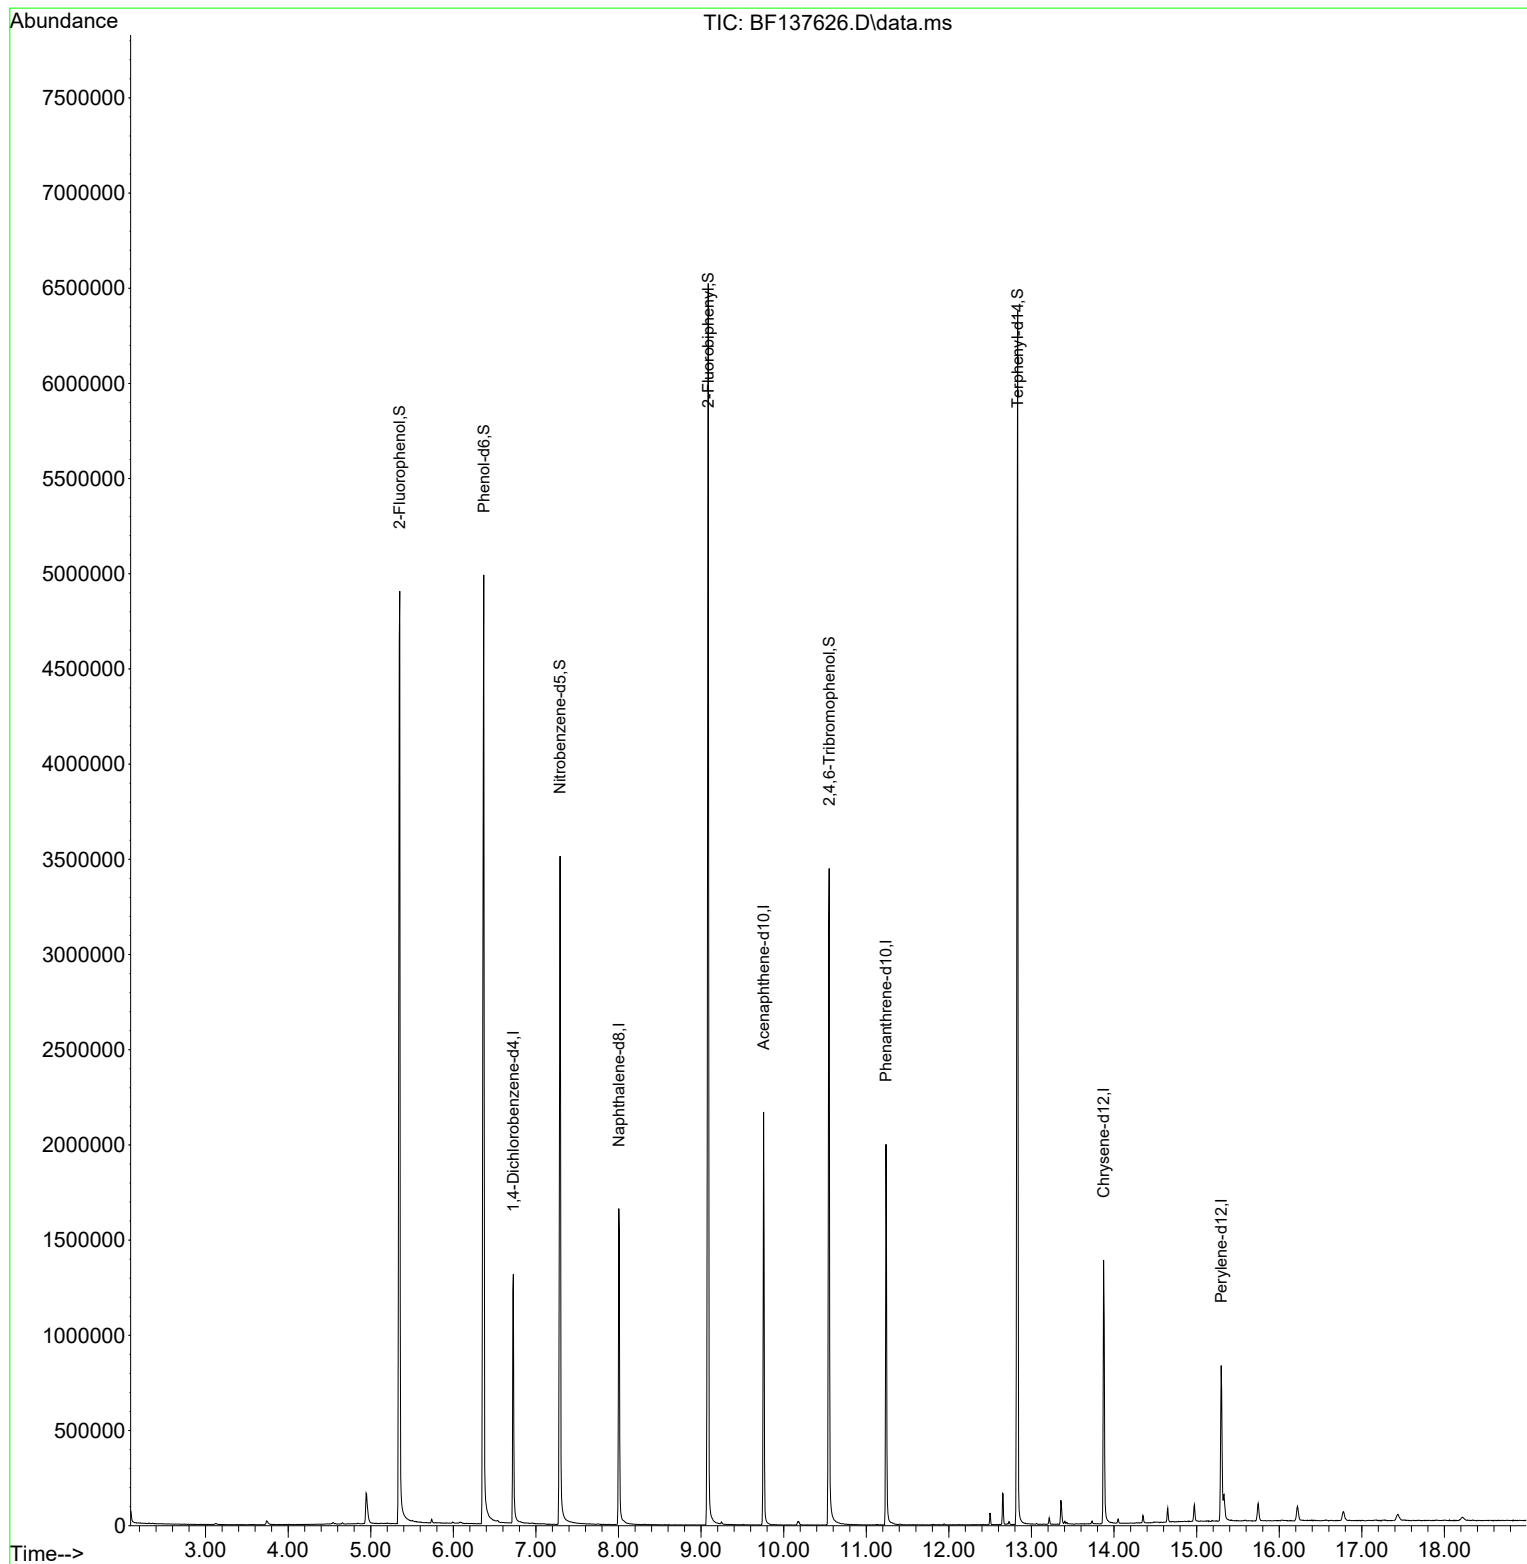




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.728 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF137626.D
Acq: 18 Mar 2024 12:34




Instrument :
BNA_F
ClientSampleId :
PB159633BL


Tgt Ion:152 Resp: 213196
Ion Ratio Lower Upper
152 100
150 156.1 125.8 188.6
115 60.3 48.8 73.2

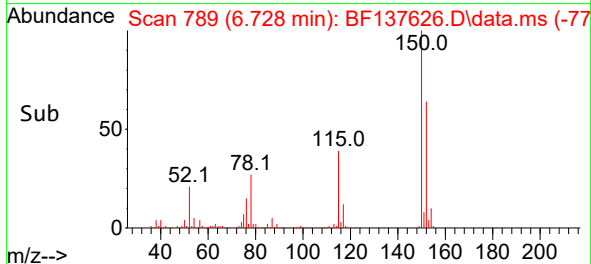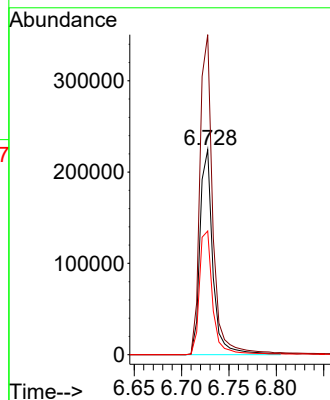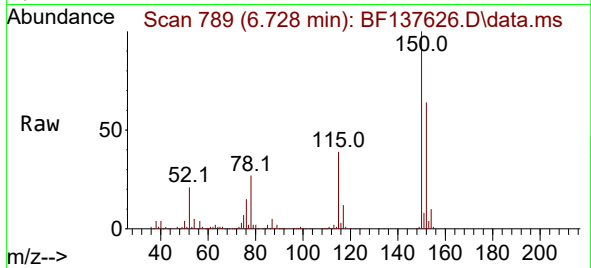

#5
2-Fluorophenol
Concen: 114.170 ng
RT: 5.351 min Scan# 555
Delta R.T. 0.017 min
Lab File: BF137626.D
Acq: 18 Mar 2024 12:34

Tgt Ion:112 Resp: 1607131
Ion Ratio Lower Upper
112 100
64 61.8 53.4 80.2
63 30.8 26.2 39.2


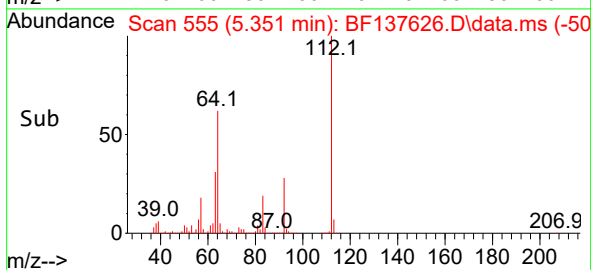
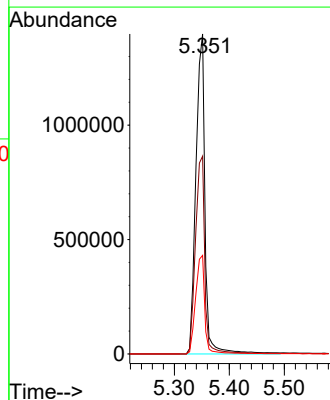
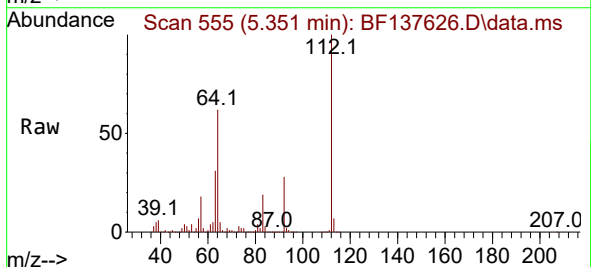




#7
Phenol-d6
Concen: 106.637 ng
RT: 6.369 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF137626.D
Acq: 18 Mar 2024 12:34




Instrument :
BNA_F
ClientSampleId :
PB159633BL


Tgt Ion: 99 Resp: 2166776
Ion Ratio Lower Upper
99 100
42 17.3 14.6 21.8
71 33.0 25.3 37.9

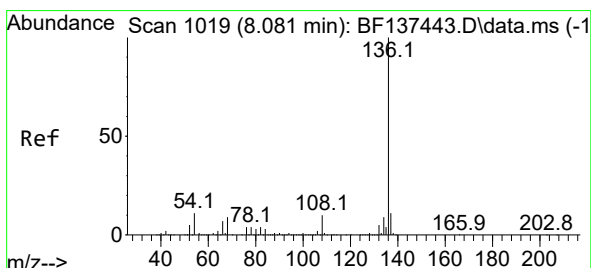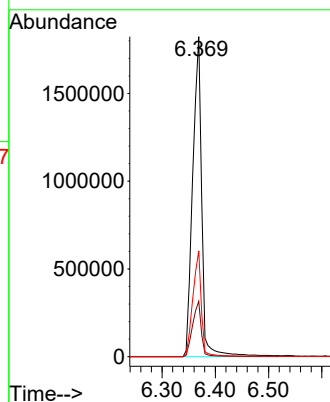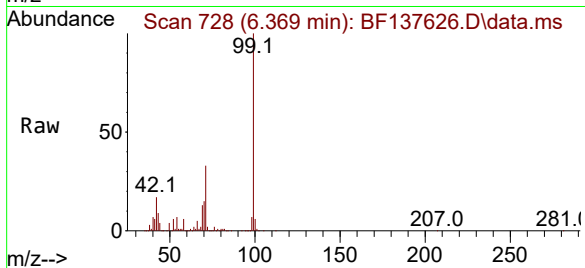

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.004 min Scan# 1006
Delta R.T. -0.006 min
Lab File: BF137626.D
Acq: 18 Mar 2024 12:34

Tgt Ion: 136 Resp: 822536
Ion Ratio Lower Upper
136 100
137 11.1 9.1 13.7
54 10.5 8.5 12.7
68 9.2 7.4 11.2

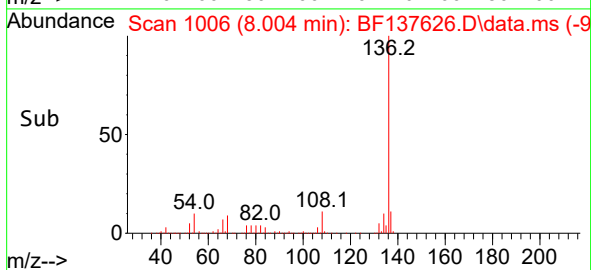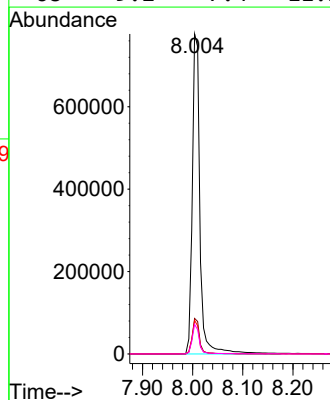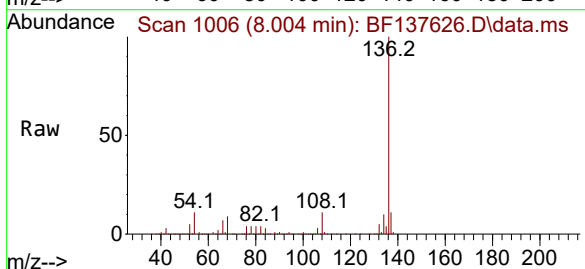



#23

Nitrobenzene-d5

Concen: 76.879 ng

RT: 7.292 min Scan# 81

Delta R.T. -0.006 min

Lab File: BF137626.D

Acq: 18 Mar 2024 12:34

Instrument :

BNA_F

ClientSampleId :

PB159633BL





Tgt Ion: 82 Resp: 1360954

Ion Ratio Lower Upper

82 100

128 40.9 32.5 48.7

54 49.5 41.5 62.3

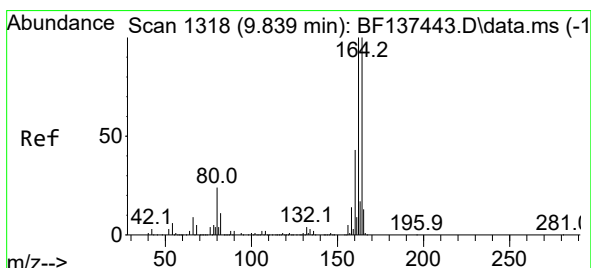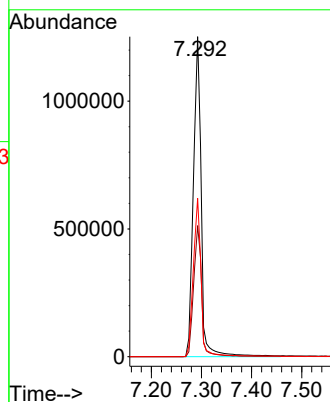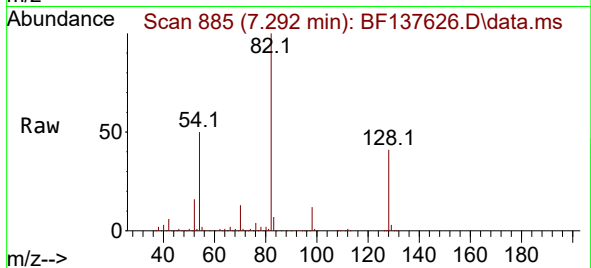

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.757 min Scan# 1304

Delta R.T. -0.006 min

Lab File: BF137626.D

Acq: 18 Mar 2024 12:34




Tgt Ion: 164 Resp: 435299


Ion Ratio Lower Upper

164 100

162 98.3 79.8 119.8

160 43.7 34.4 51.6

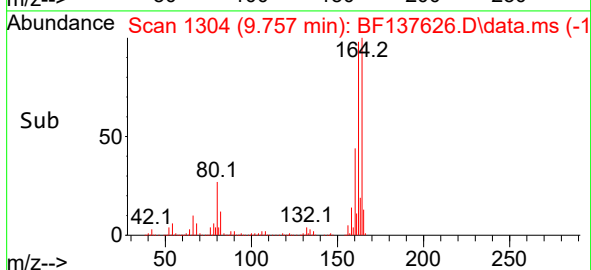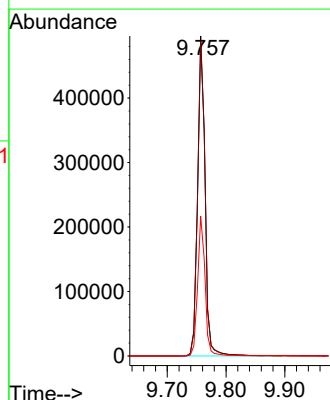



#42

2,4,6-Tribromophenol

Concen: 125.046 ng

RT: 10.551 min Scan# 1453

Delta R.T. -0.000 min

Lab File: BF137626.D

Acq: 18 Mar 2024 12:34

Instrument :

BNA_F

ClientSampleId :

PB159633BL





Tgt Ion:330 Resp: 478011

Ion Ratio Lower Upper

330 100

332 97.3 78.0 117.0

141 29.0 27.3 40.9

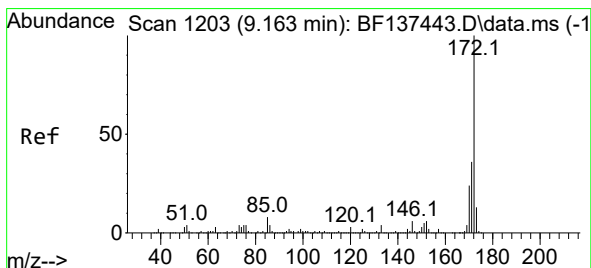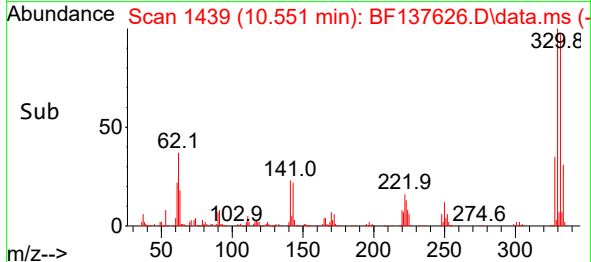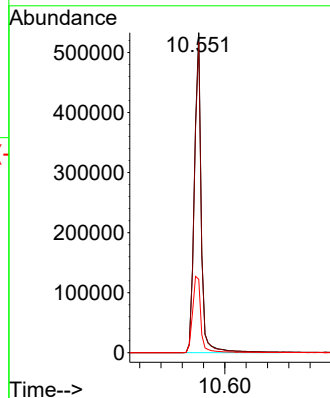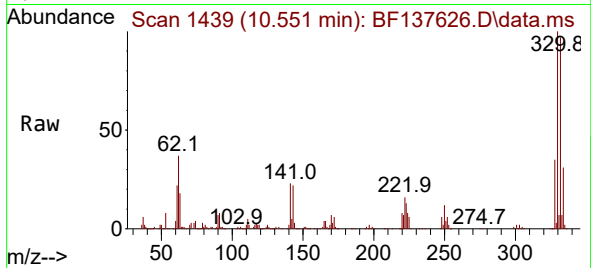

#45

2-Fluorobiphenyl

Concen: 78.249 ng

RT: 9.086 min Scan# 1190

Delta R.T. -0.000 min

Lab File: BF137626.D

Acq: 18 Mar 2024 12:34




Tgt Ion:172 Resp: 2175969


Ion Ratio Lower Upper

172 100

171 35.9 28.5 42.7

170 24.0 19.0 28.6


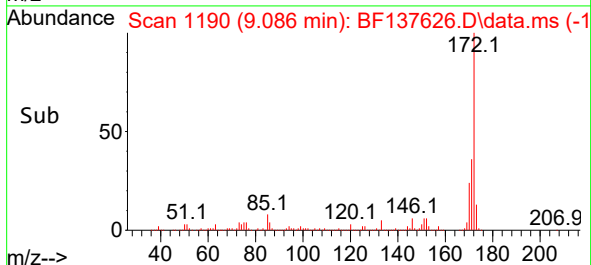
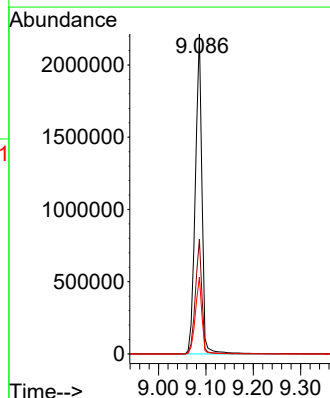
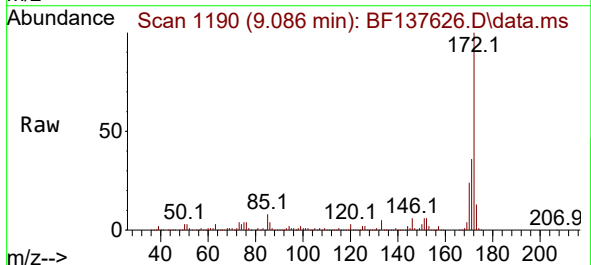




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.239 min Scan# 11
Delta R.T. -0.000 min
Lab File: BF137626.D
Acq: 18 Mar 2024 12:34




Instrument :
BNA_F
ClientSampleId :
PB159633BL


Tgt Ion:188 Resp: 746900
Ion Ratio Lower Upper
188 100
94 13.4 10.6 15.8
80 14.5 11.5 17.3

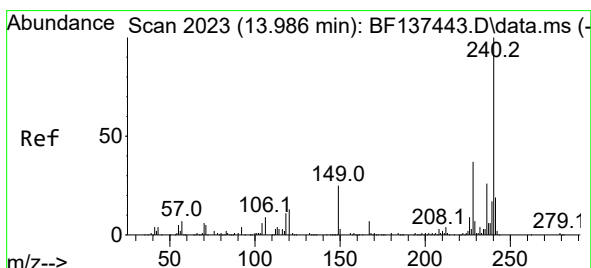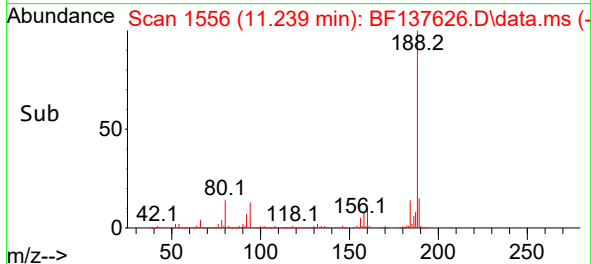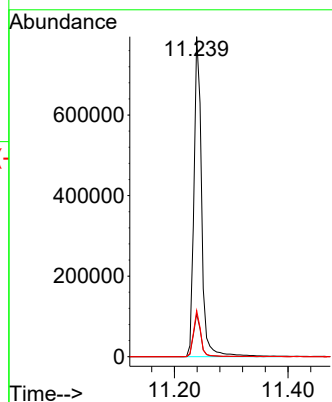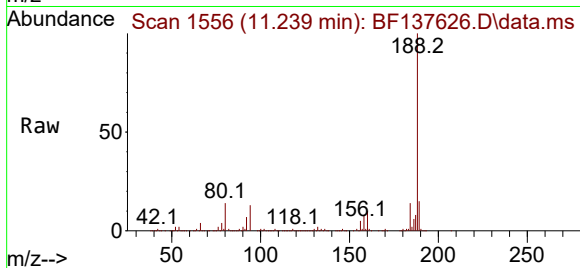

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.874 min Scan# 2004
Delta R.T. -0.000 min
Lab File: BF137626.D
Acq: 18 Mar 2024 12:34


Tgt Ion:240 Resp: 480906
Ion Ratio Lower Upper
240 100
120 13.6 10.4 15.6
236 26.2 20.9 31.3

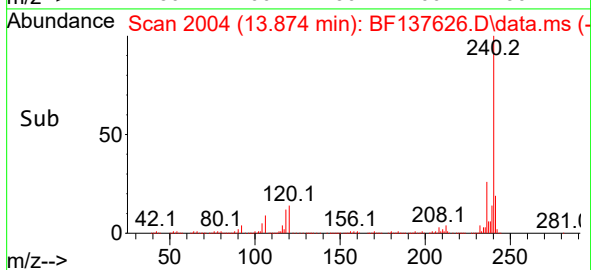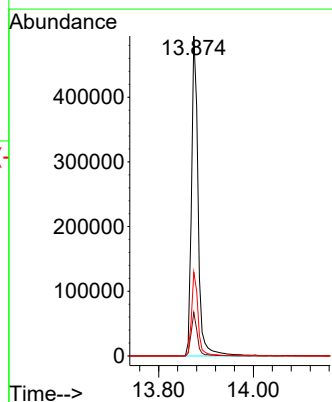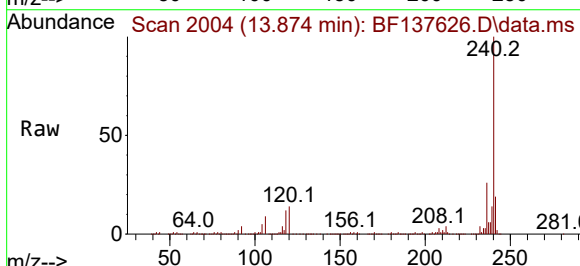






#79
 Terphenyl-d14
 Concen: 69.340 ng
 RT: 12.833 min Scan# 1843
 Delta R.T. 0.006 min
 Lab File: BF137626.D
 Acq: 18 Mar 2024 12:34

Instrument :
 BNA_F
 ClientSampleId :
 PB159633BL

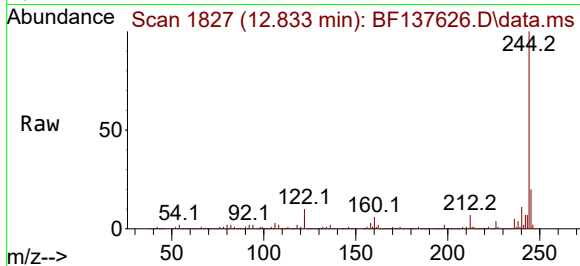

Tgt Ion:244 Resp: 2424967
 Ion Ratio Lower Upper
 244 100
 212 6.7 5.4 8.2
 122 10.1 9.1 13.7

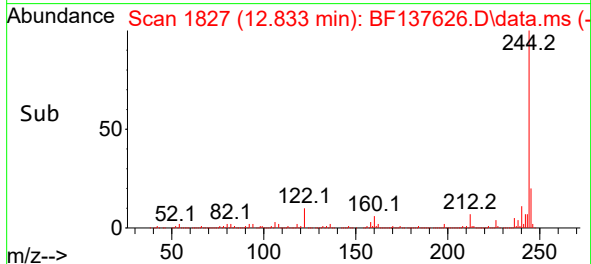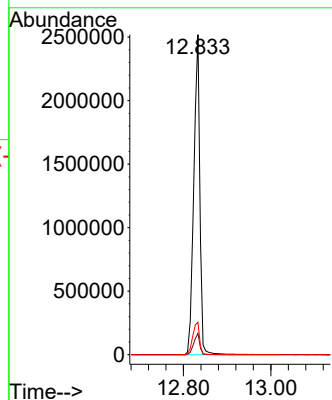

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.298 min Scan# 2246
 Delta R.T. -0.000 min
 Lab File: BF137626.D
 Acq: 18 Mar 2024 12:34

Tgt Ion:264 Resp: 393200
 Ion Ratio Lower Upper
 264 100
 260 23.8 19.3 28.9
 265 21.9 17.4 26.0

