

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031824\
 Data File : BF137631.D
 Acq On : 18 Mar 2024 15:07
 Operator : CG\JU
 Sample : P1326-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137631.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.328	547	551	569	rBV	2376213	2342394	85.05%	12.464%
2	6.357	723	726	744	rBV	2333577	2428907	88.20%	12.924%
3	6.722	785	788	806	rBV	685605	683545	24.82%	3.637%
4	7.287	881	884	898	rBV	1597726	1448408	52.59%	7.707%
5	8.004	1003	1006	1013	rBV	981434	869367	31.57%	4.626%
6	9.081	1186	1189	1201	rBV	3236120	2754000	100.00%	14.654%
7	9.757	1300	1304	1316	rBV	1300352	1076115	39.07%	5.726%
8	10.545	1434	1438	1456	rBV	1641224	1630424	59.20%	8.675%
9	11.239	1553	1556	1569	rBV	1203313	1081955	39.29%	5.757%
10	11.780	1645	1648	1651	rBV2	44215	57326	2.08%	0.305%
11	12.451	1759	1762	1771	rBV	32473	39707	1.44%	0.211%
12	12.680	1794	1801	1803	rBV	41841	39724	1.44%	0.211%
13	12.822	1822	1825	1829	rBV	2814070	2596634	94.29%	13.816%
14	13.733	1976	1980	1990	rBV4	52332	132265	4.80%	0.704%
15	13.874	1999	2004	2016	rBV	793357	792000	28.76%	4.214%
16	14.716	2144	2147	2151	rBV	34293	36563	1.33%	0.195%
17	14.898	2174	2178	2186	rBV	24746	49190	1.79%	0.262%
18	15.298	2241	2246	2259	rBV	527242	735409	26.70%	3.913%




Sum of corrected areas: 18793933

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031824\
Data File : BF137631.D
Acq On : 18 Mar 2024 15:07
Operator : CG\JU
Sample : P1326-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

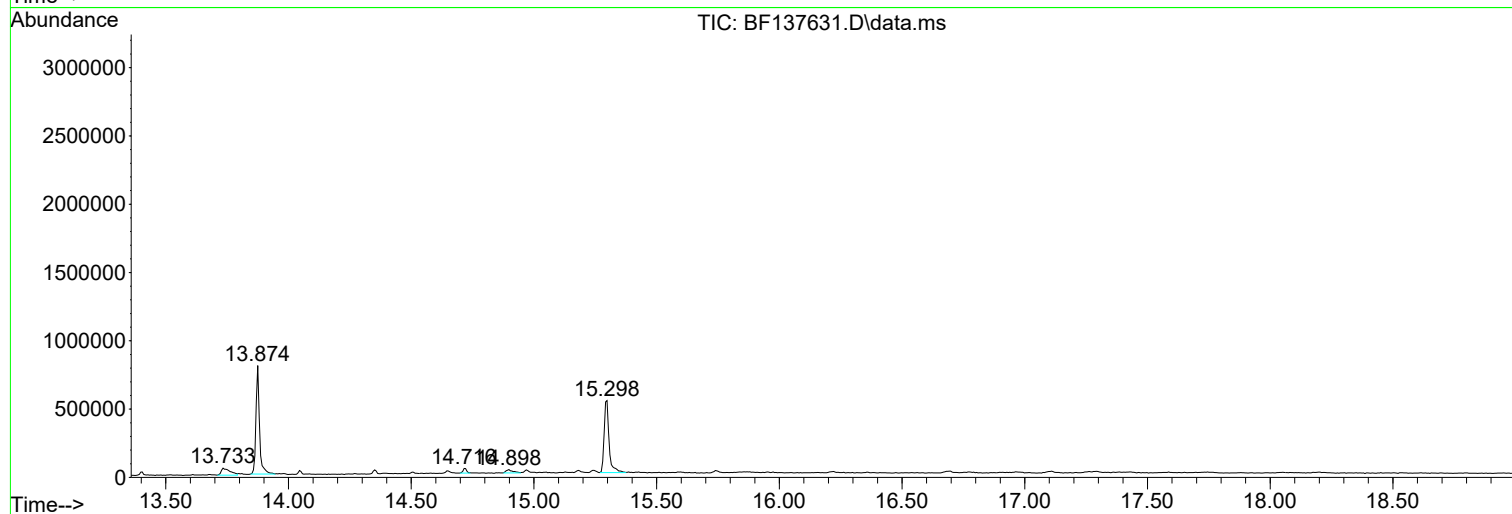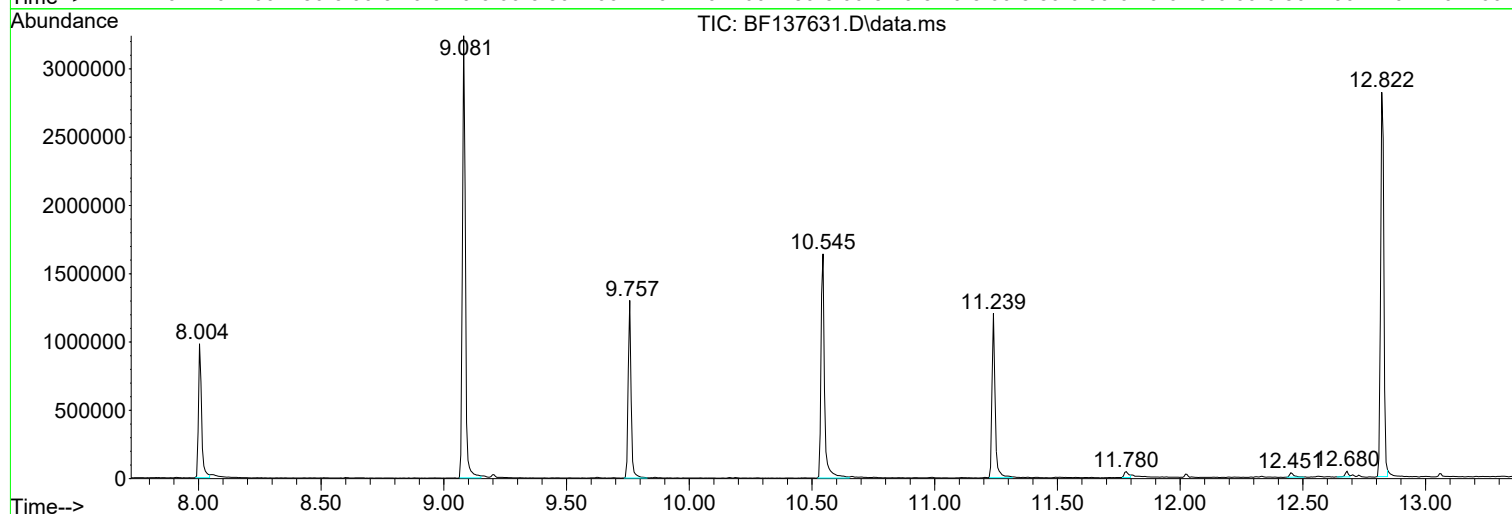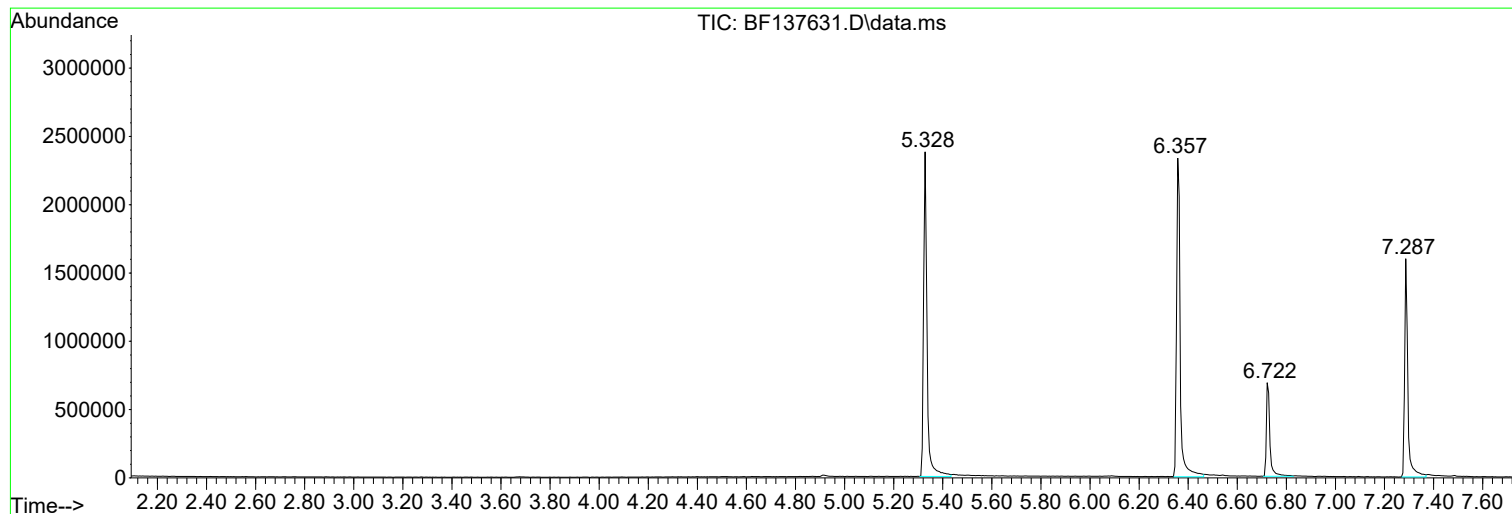

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031824\
Data File : BF137631.D
Acq On : 18 Mar 2024 15:07
Operator : CG\JU
Sample : P1326-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Pentadecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.733	3.34 ng	132265	Chrysene-d12	13.874

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Pentadecane	212	C15H32	000629-62-9	93
2			Carbonic acid, eicosyl vinyl ester	368	C23H44O3	1000382-54-3	87
3			Tritetracontane	605	C43H88	007098-21-7	83
4			Sulfurous acid, 2-propyl tetradec...	320	C17H36O3S	1010309-12-5	83
5			Ethanol, 2-(dodecyloxy)-	230	C14H30O2	004536-30-5	80

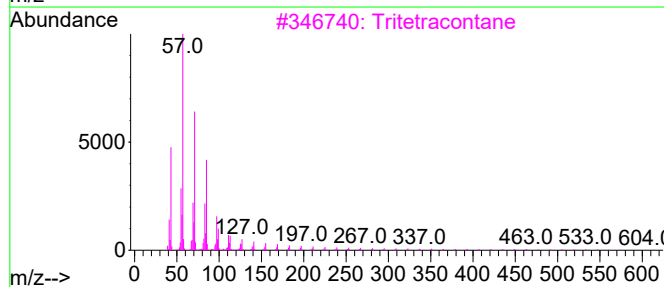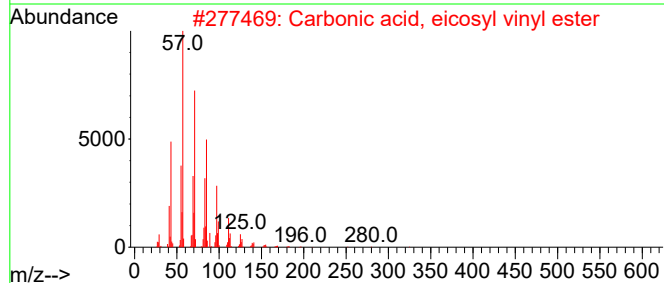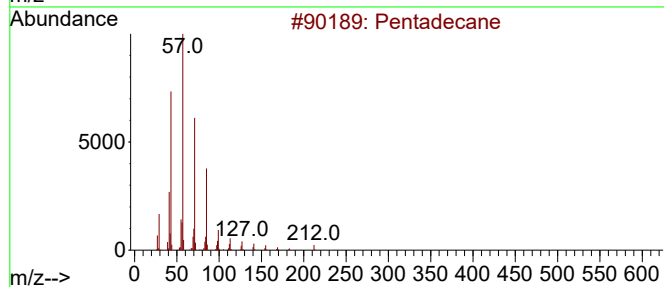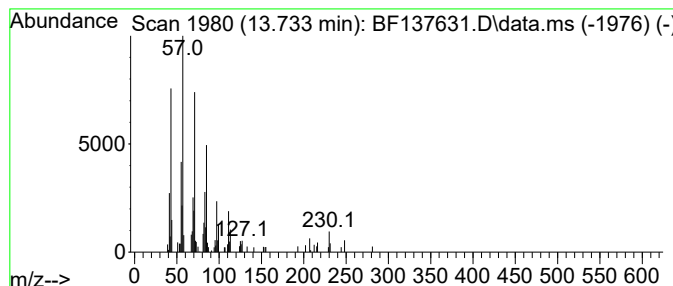

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031824\
Data File : BF137631.D
Acq On : 18 Mar 2024 15:07
Operator : CG\JU
Sample : P1326-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Pentadecane	13.733	3.3	ng	132265	5	13.874	792000	20.0