
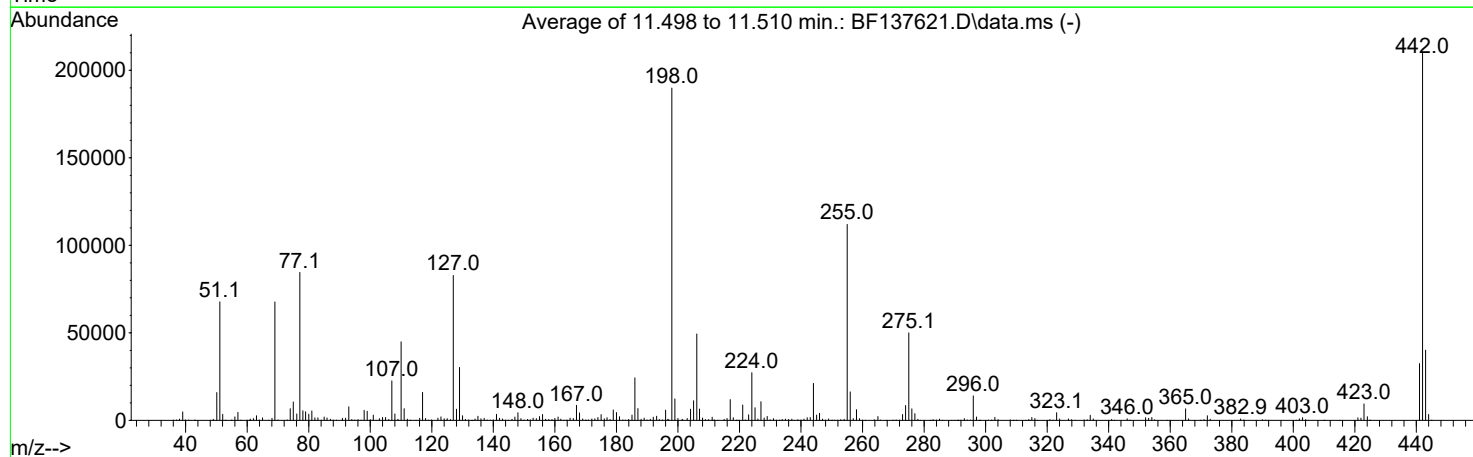


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031824\
Data File : BF137621.D
Acq On : 18 Mar 2024 10:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 14:45:20 2024

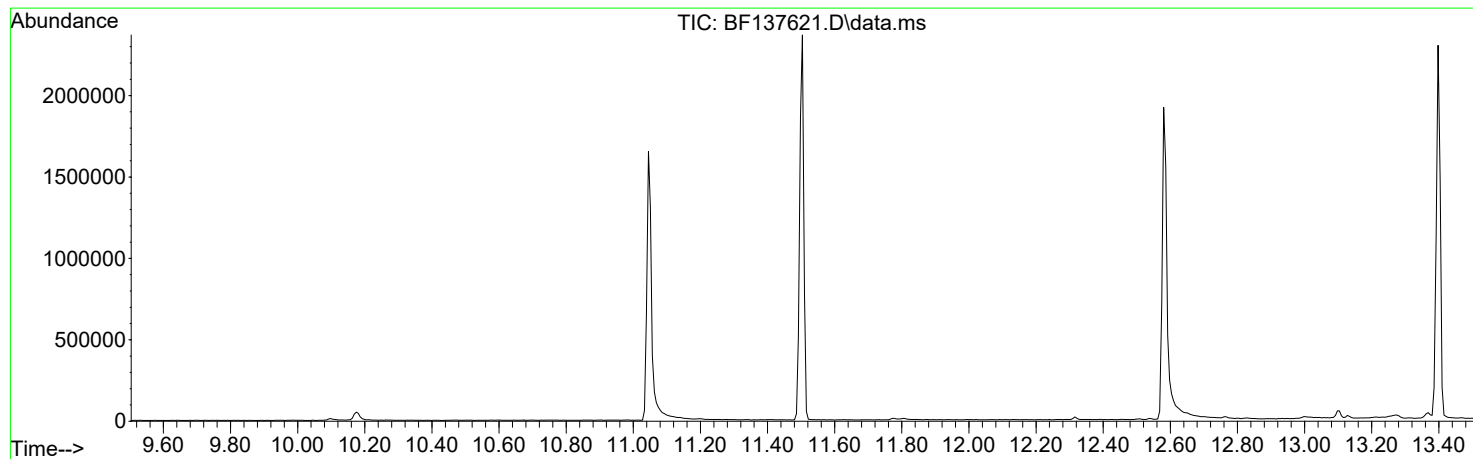

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	67715	PASS
68	69	0.00	2	1.7	1160	PASS
69	198	0.00	100	35.6	67624	PASS
70	69	0.00	2	0.4	298	PASS
127	198	10	80	43.6	82877	PASS
197	198	0.00	2	0.4	669	PASS
198	198	100	100	100.0	189872	PASS
199	198	5	9	6.5	12296	PASS
275	198	10	60	26.4	50043	PASS
365	198	1	100	3.5	6626	PASS
441	198	0.01	100	17.1	32491	PASS
442	442	50	100	100.0	210197	PASS
443	442	15	24	19.1	40112	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/18/2024	BNA_F	<u>BF137621.D</u>
Compound Name	Response	Retention Time
DDT	372016	13.398
DDD	12316	13.104
DDE	1426	12.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13742	385758	3.56

Instrument :
BNA_F
ClientSampleId :
DFTPP

Instrument :
BNA_F
ClientSampleId :
DFTPP

```
lon 265.70 (265.40 to 266.40): BF137621.D\data.ms
lon 268.00 (267.70 to 268.70): BF137621.D\data.ms
lon 264.00 (263.70 to 264.70): BF137621.D\data.ms
```

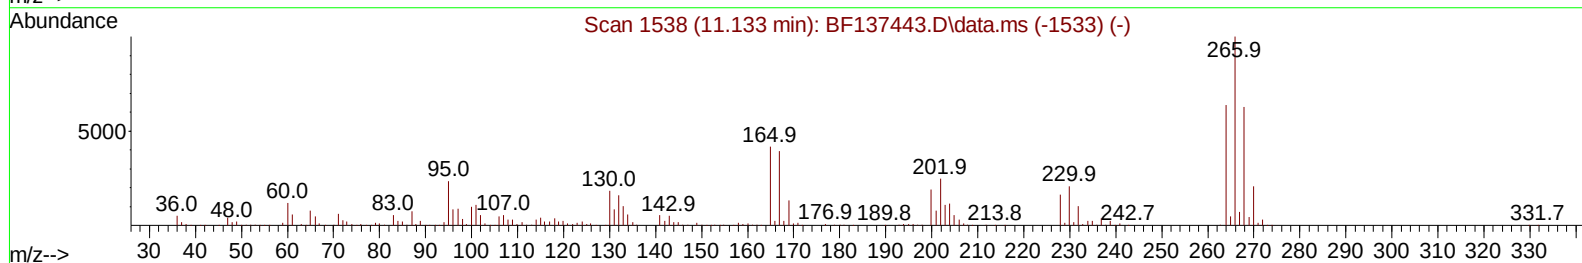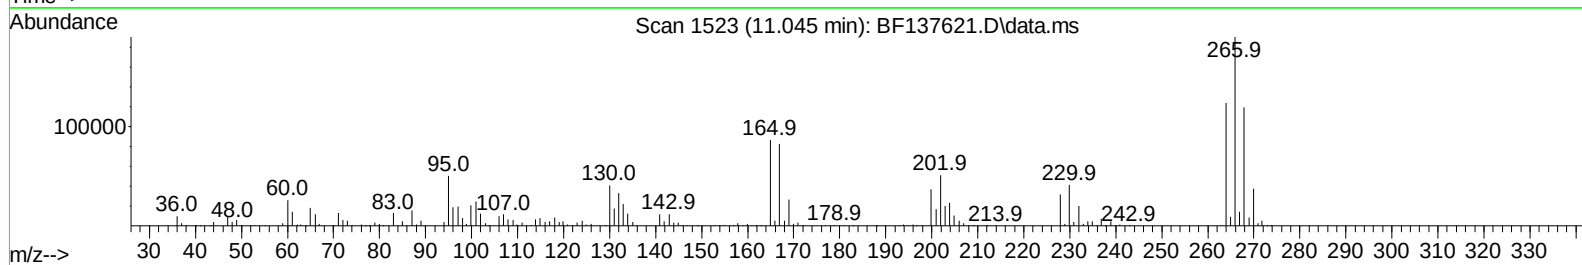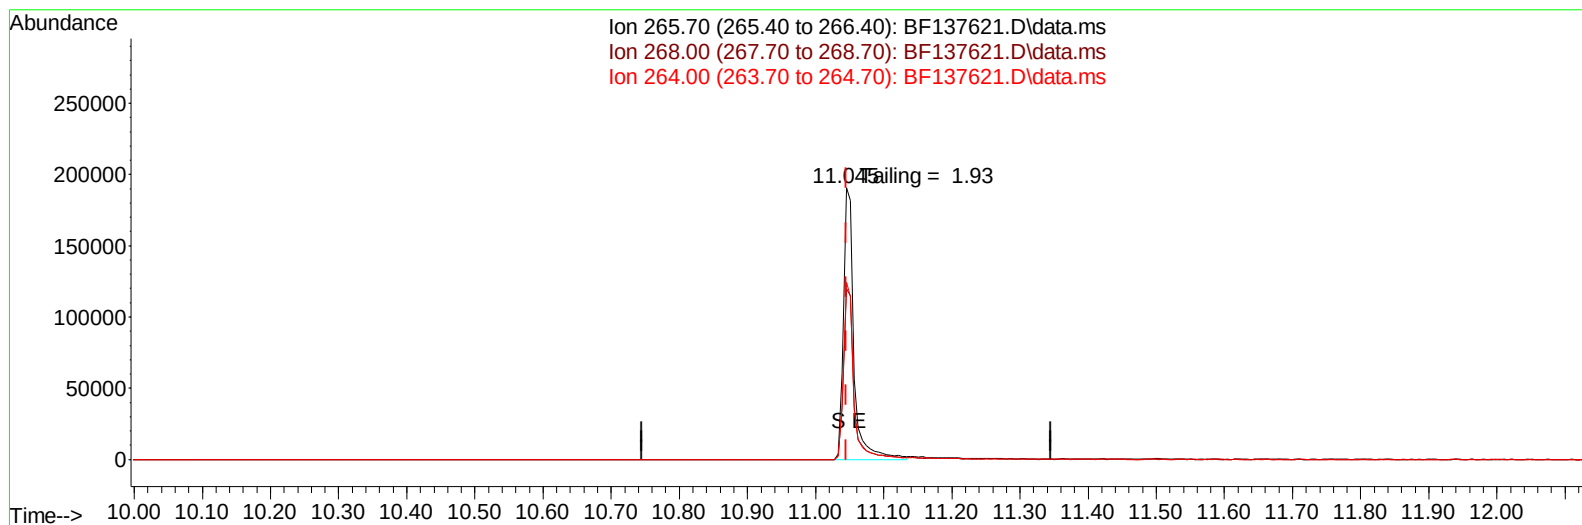




TIC: BF137621.D\data.ms

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.75
264.00	63.60	65.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031824\
Data File : BF137621.D
Acq On : 18 Mar 2024 10:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 18 23:55:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

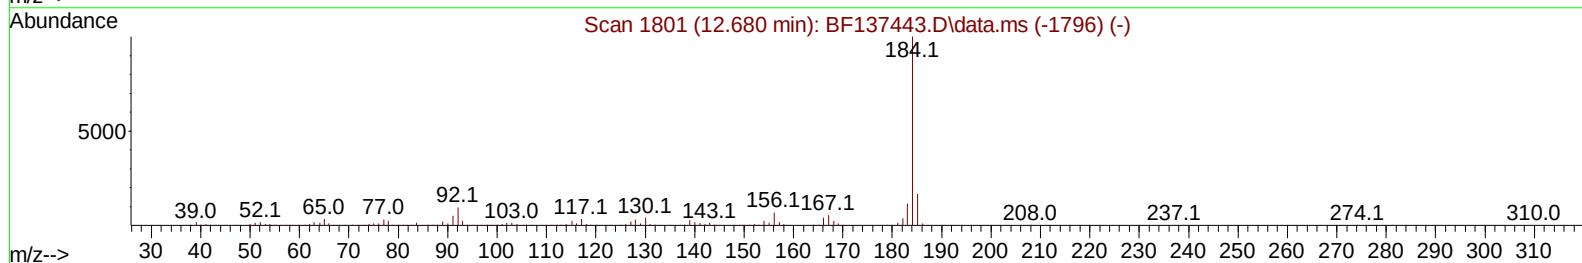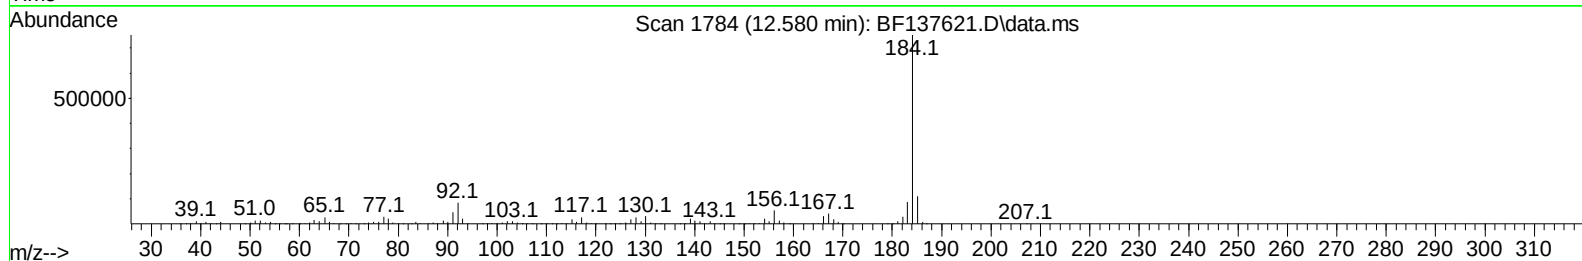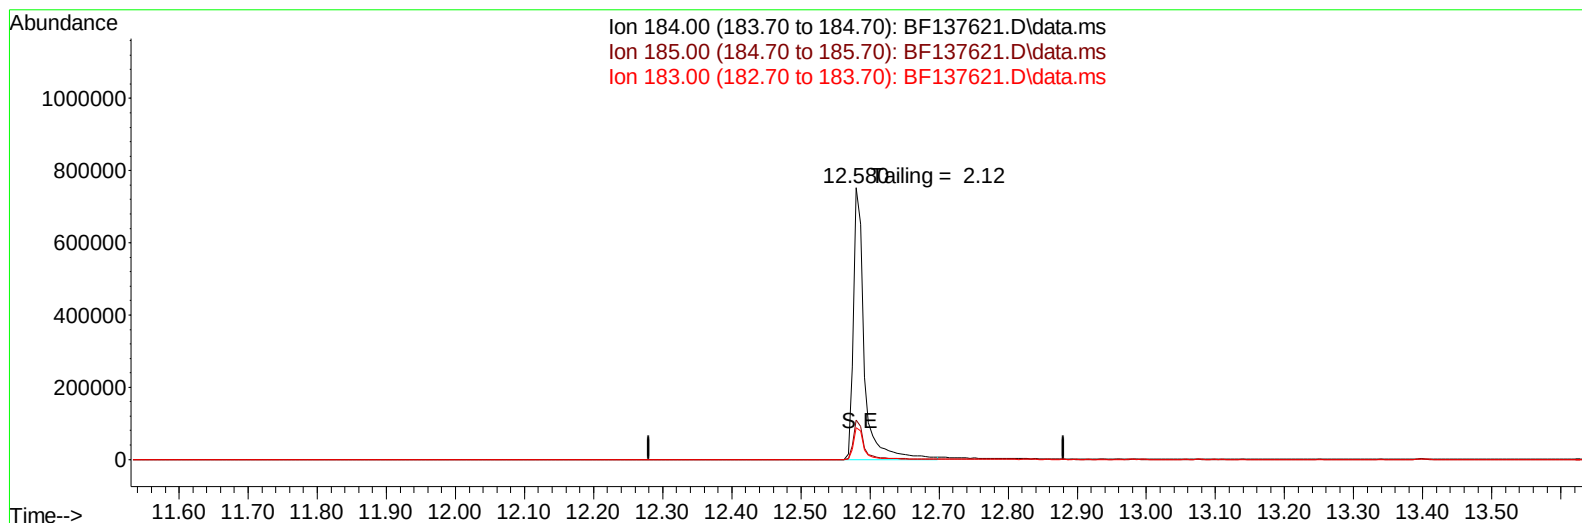

TIC: BF137621.D\data.ms

(77) Benzidine

12.580min (-12.580) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	16.50	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00