

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032019\
 Data File : BF113175.D
 Acq On : 20 Mar 2019 17:07
 Operator : JU/SJ
 Sample : K1688-21 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 JC-02-031919-A

Quant Time: Mar 21 14:48:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 21 12:13:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.72	152	111740	20.00	ng	0.00
21) Naphthalene-d8	8.00	136	445161	20.00	ng	0.00
39) Acenaphthene-d10	9.76	164	206494	20.00	ng	0.00
64) Phenanthrene-d10	11.24	188	376032	20.00	ng	0.00
76) Chrysene-d12	13.87	240	349716	20.00	ng	0.00
87) Perylene-d12	15.28	264	287147	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.34	112	44325	6.17	ng	0.00
7) Phenol-d6	6.37	99	62039	6.88	ng	0.00
23) Nitrobenzene-d5	7.28	82	34262	4.61	ng	-0.01
42) 2,4,6-Tribromophenol	10.55	330	22428	10.23	ng	0.00
45) 2-Fluorobiphenyl	9.08	172	87097	4.23	ng	0.00
79) Terphenyl-d14	12.82	244	118066	6.54	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032019\
Data File : BF113175.D
Acq On : 20 Mar 2019 17:07
Operator : JU/SJ
Sample : K1688-21 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JC-02-031919-A

Quant Time: Mar 21 14:48:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 21 12:13:22 2019
Response via : Initial Calibration

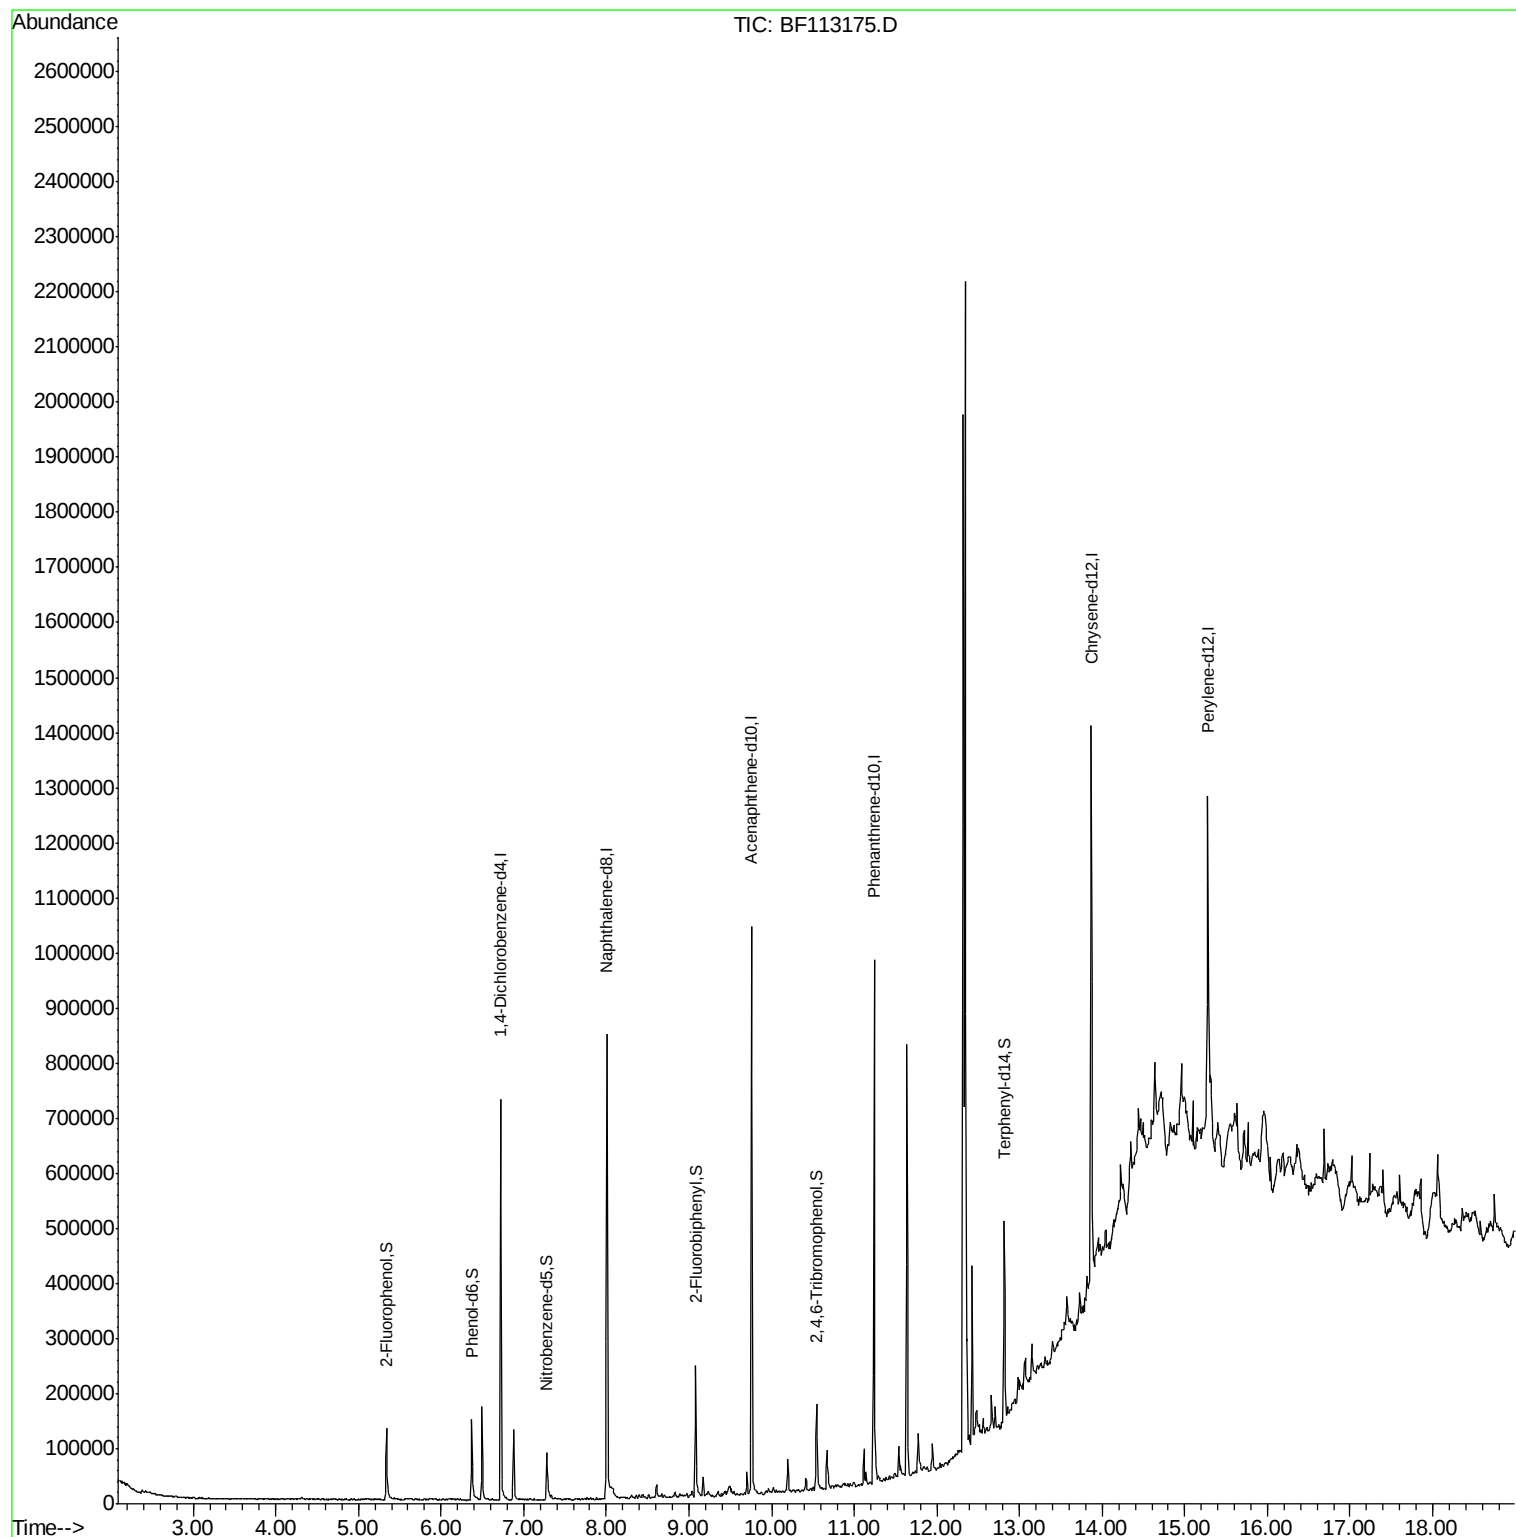

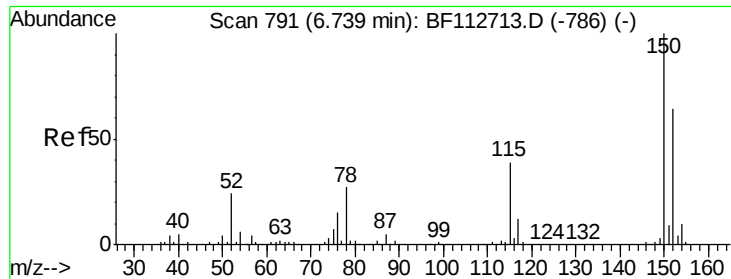


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.72 min Scan# 788
Delta R.T. 0.00 min
Lab File: BF113175.D
Acq: 20 Mar 2019 17:07

Instrument :
BNA_F
ClientSampleId :
JC-02-031919-A

Tgt Ion:152 Resp: 111740
Ion Ratio Lower Upper
152 100
150 156.2 123.0 184.6
115 58.0 45.9 68.9

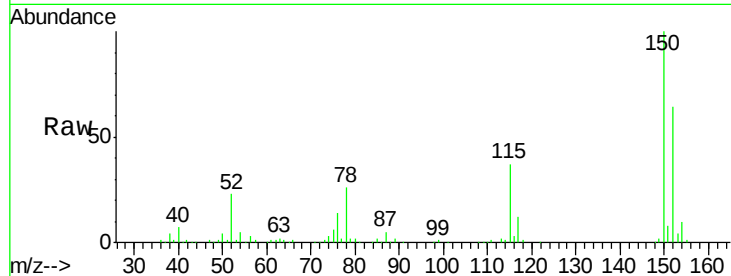


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

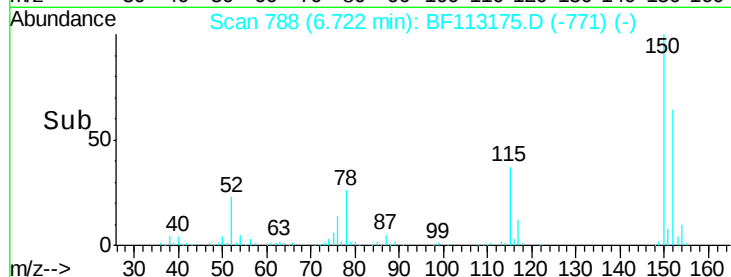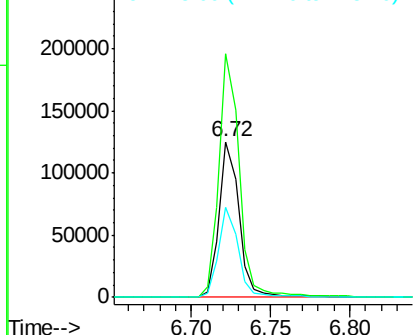



#5


2-Fluorophenol
Concen: 6.171 ng
RT: 5.34 min Scan# 553
Delta R.T. 0.01 min
Lab File: BF113175.D
Acq: 20 Mar 2019 17:07

Tgt Ion:112 Resp: 44325
Ion Ratio Lower Upper
112 100
64 60.3 49.3 73.9
63 31.6 25.4 38.2

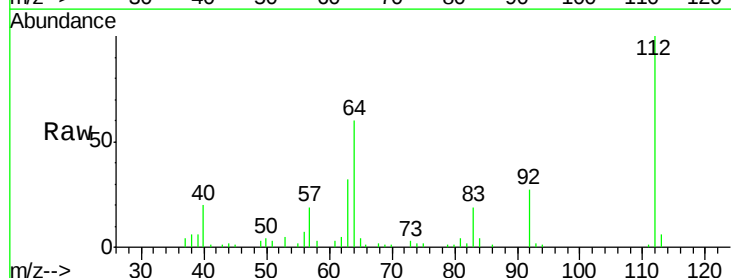

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

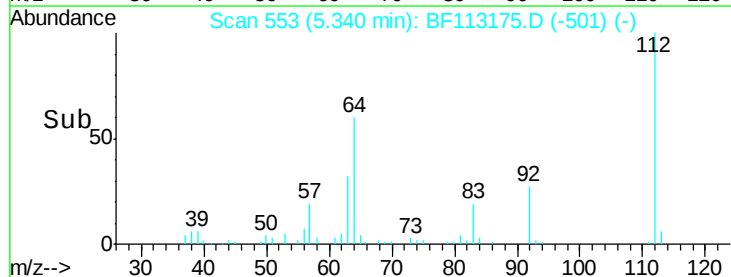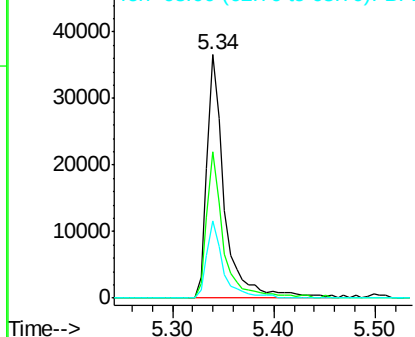

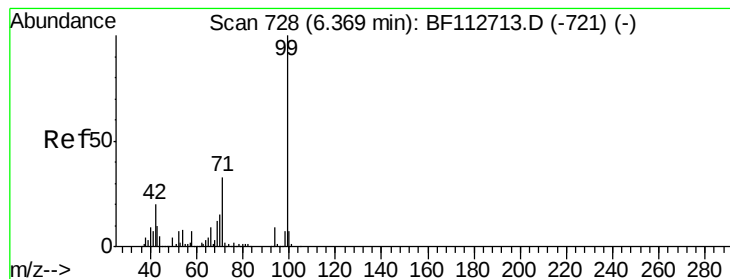

#7

Phenol-d6

Concen: 6.875 ng

RT: 6.37 min Scan# 728

Delta R.T. -0.01 min

Lab File: BF113175.D

Acq: 20 Mar 2019 17:07

Instrument :

BNA_F

ClientSampleId :

JC-02-031919-A


Tgt Ion: 99 Resp: 62039

Ion Ratio Lower Upper

99 100

42 19.2 15.2 22.8




71 33.0 25.7 38.5

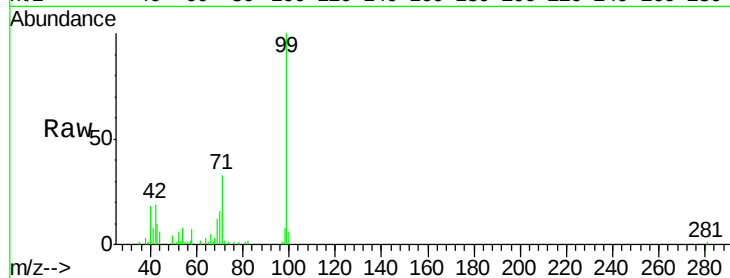

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

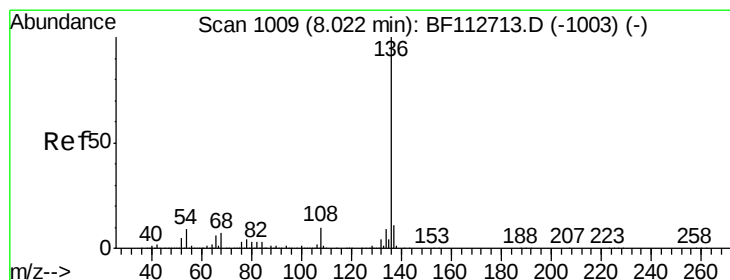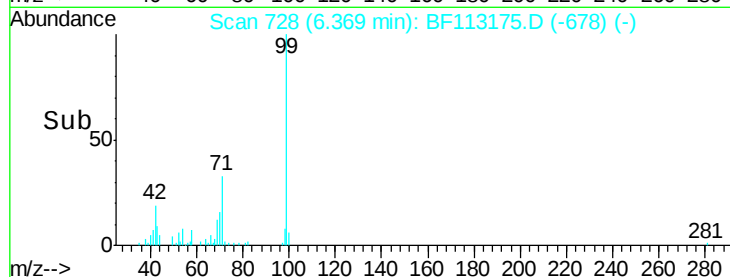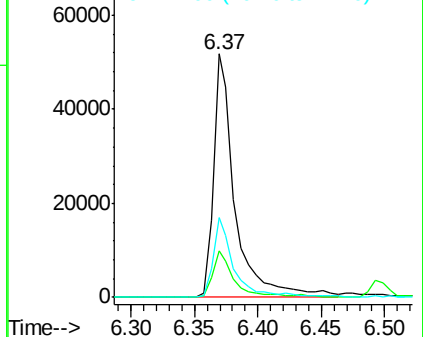

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.00 min Scan# 1006

Delta R.T. -0.00 min

Lab File: BF113175.D

Acq: 20 Mar 2019 17:07

Tgt Ion: 136 Resp: 445161


Ion Ratio Lower Upper

136 100

137 11.3 8.9 13.3

54 8.7 7.0 10.6

68 5.9 5.0 7.4


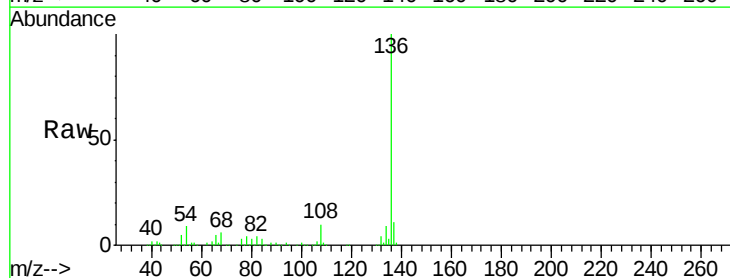


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

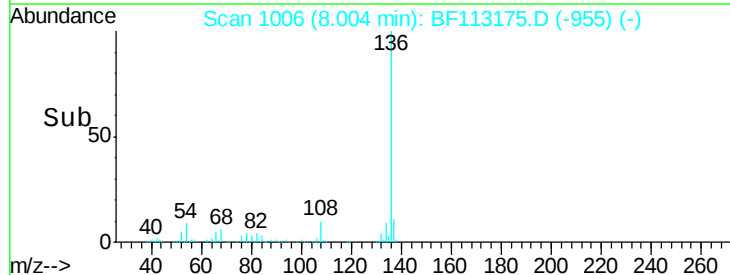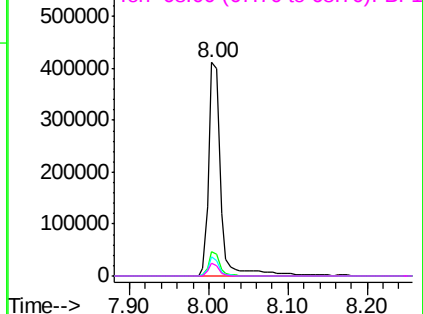






#23
 Nitrobenzene-d5
 Concen: 4.605 ng
 RT: 7.28 min Scan# 883
 Delta R.T. -0.01 min
 Lab File: BF113175.D
 Acq: 20 Mar 2019 17:07

Instrument :
 BNA_F
 ClientSampleId :
 JC-02-031919-A

Tgt Ion: 82 Resp: 34262
 Ion Ratio Lower Upper
 82 100
 128 44.3 37.9 56.9
 54 53.4 41.2 61.8

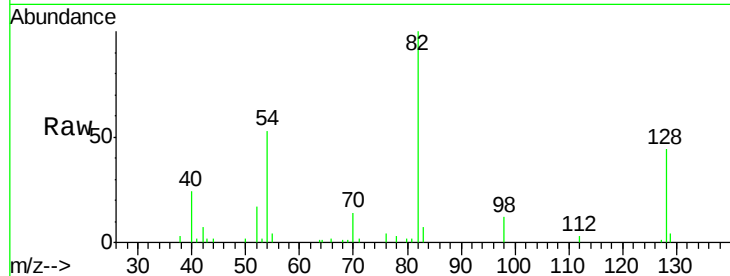


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

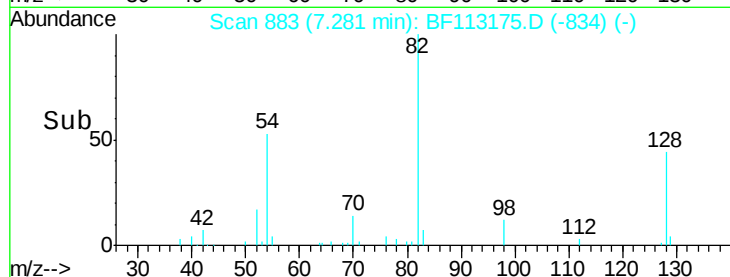
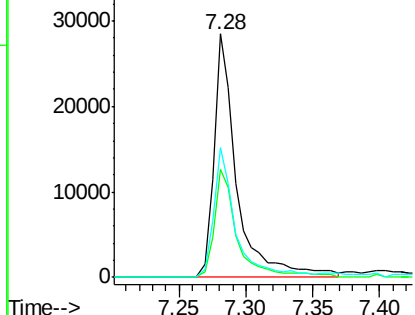



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.76 min Scan# 1304
 Delta R.T. 0.00 min
 Lab File: BF113175.D
 Acq: 20 Mar 2019 17:07

Tgt Ion: 164 Resp: 206494
 Ion Ratio Lower Upper
 164 100
 162 102.1 80.8 121.2
 160 45.2 36.2 54.2

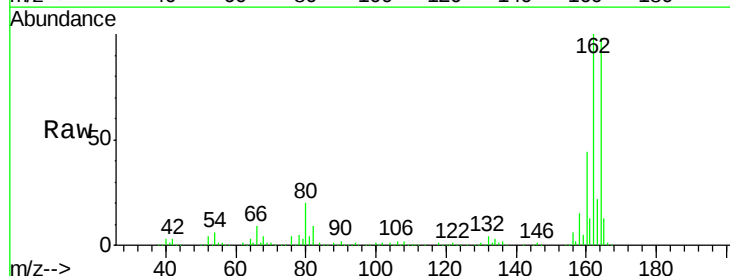

Abundance Ion 164.00 (163.70 to 164.70): BF1
 Ion 162.00 (161.70 to 162.70): BF1
 Ion 160.00 (159.70 to 160.70): BF1

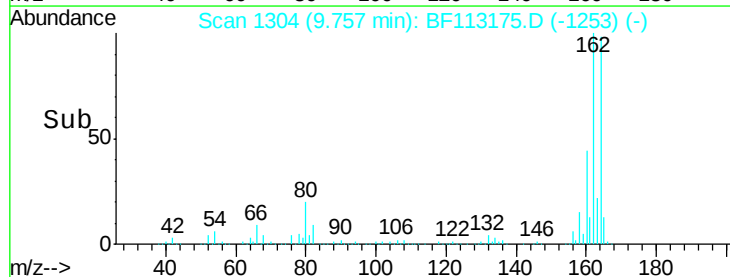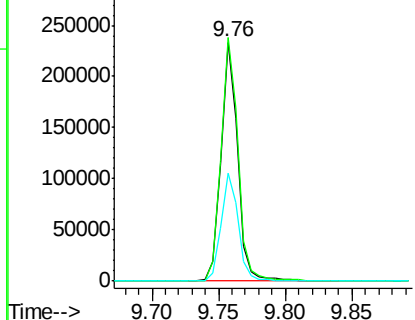


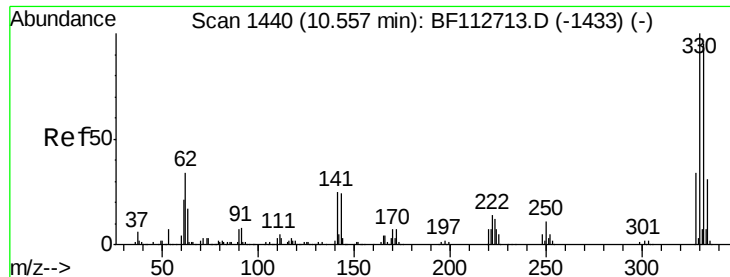




#42
 2,4,6-Tribromophenol
 Concen: 10.231 ng
 RT: 10.55 min Scan# 1438
 Delta R.T. 0.00 min
 Lab File: BF113175.D
 Acq: 20 Mar 2019 17:07

Instrument :
 BNA_F
 ClientSampleId :
 JC-02-031919-A

Tgt Ion:330 Resp: 22428
 Ion Ratio Lower Upper
 330 100
 332 92.8 76.3 114.5
 141 32.3 22.3 33.5

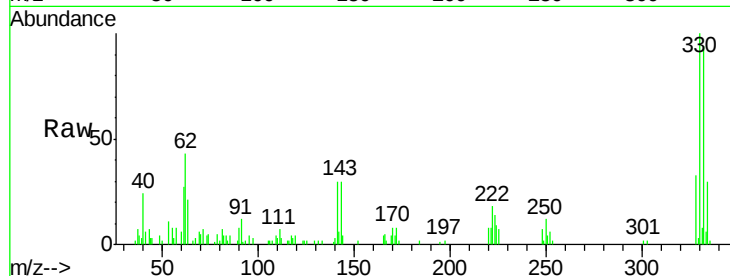


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

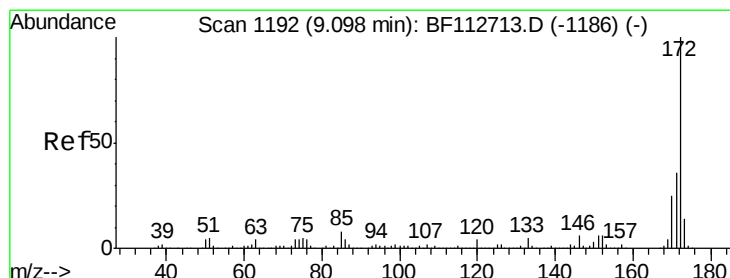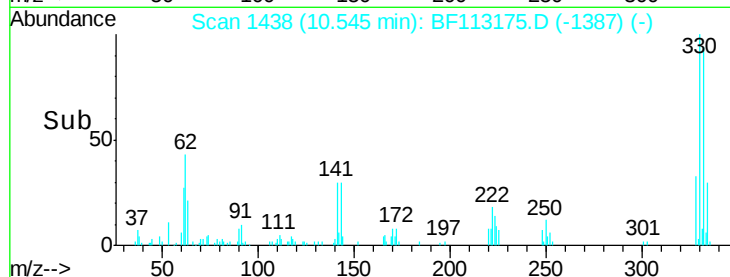
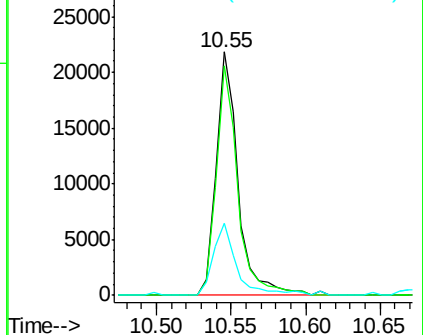


#45
 2-Fluorobiphenyl
 Concen: 4.232 ng
 RT: 9.08 min Scan# 1189
 Delta R.T. -0.01 min
 Lab File: BF113175.D
 Acq: 20 Mar 2019 17:07

Tgt Ion:172 Resp: 87097
 Ion Ratio Lower Upper
 172 100
 171 34.2 29.0 43.4
 170 23.9 20.1 30.1

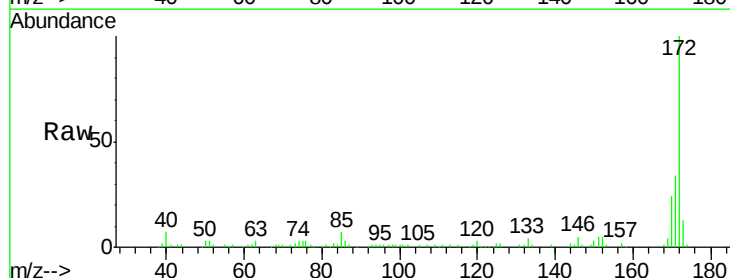

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



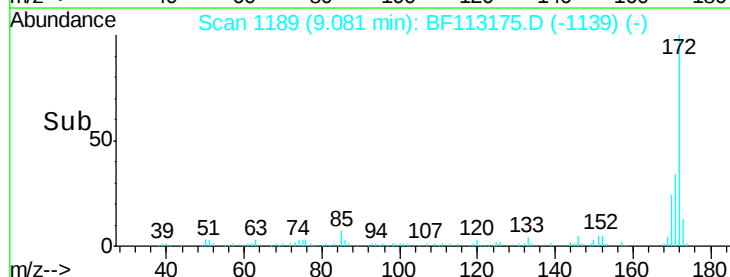
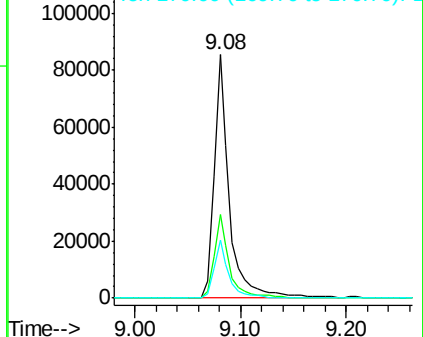




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.24 min Scan# 1556
Delta R.T. 0.01 min
Lab File: BF113175.D
Acq: 20 Mar 2019 17:07




Instrument :
BNA_F
ClientSampleId :
JC-02-031919-A


Tgt Ion:188 Resp: 376032
Ion Ratio Lower Upper
188 100
94 8.2 7.4 11.2
80 8.6 7.9 11.9

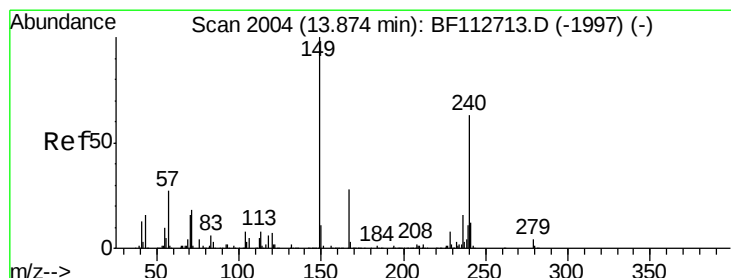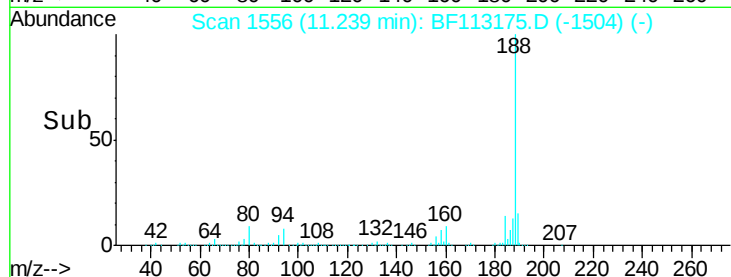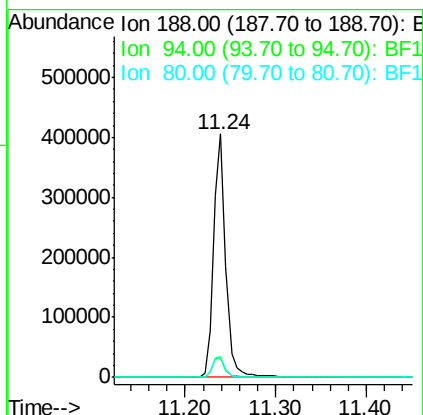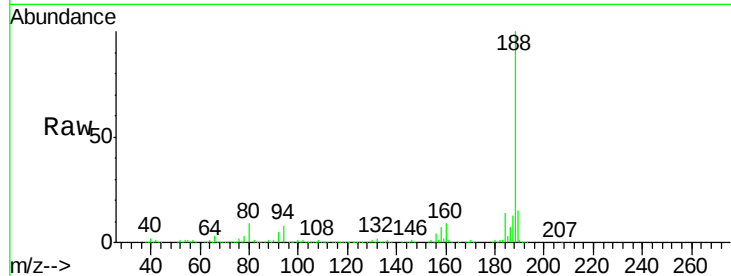

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.87 min Scan# 2003
Delta R.T. -0.00 min
Lab File: BF113175.D
Acq: 20 Mar 2019 17:07

Tgt Ion:240 Resp: 349716
Ion Ratio Lower Upper
240 100
120 10.5 8.6 12.8
236 25.9 21.2 31.8

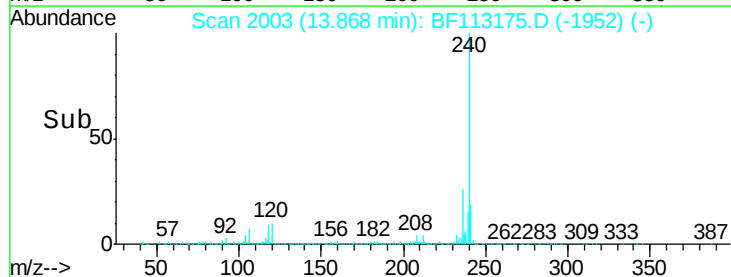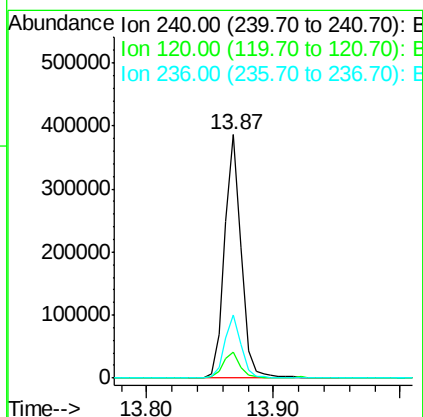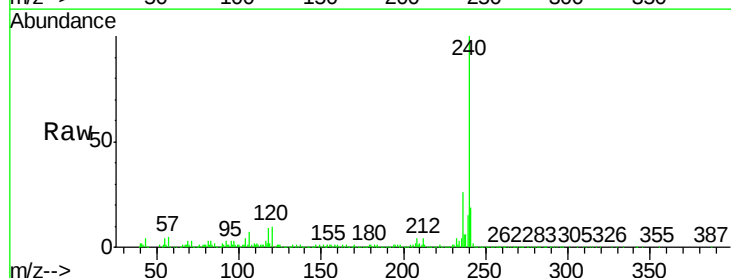

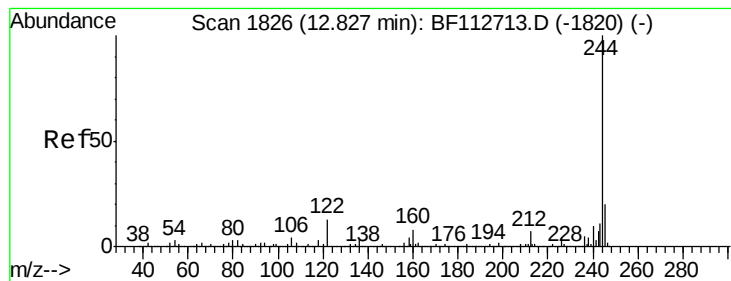

#79

Terphenyl-d14

Concen: 6.544 ng

RT: 12.82 min Scan# 1824

Delta R.T. -0.00 min

Lab File: BF113175.D

Acq: 20 Mar 2019 17:07

Instrument :

BNA_F

ClientSampleId :

JC-02-031919-A


Tgt Ion:244 Resp: 118066

Ion Ratio Lower Upper

244 100

212 6.3 5.7 8.5




122 10.4 9.4 14.2

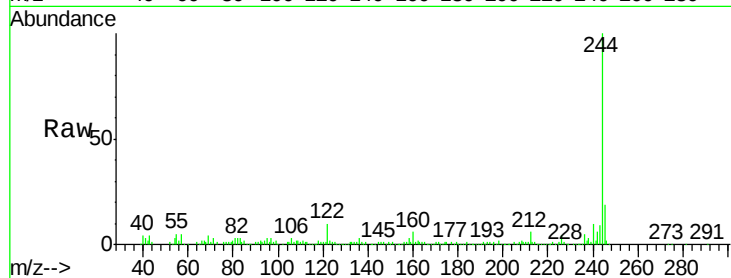

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

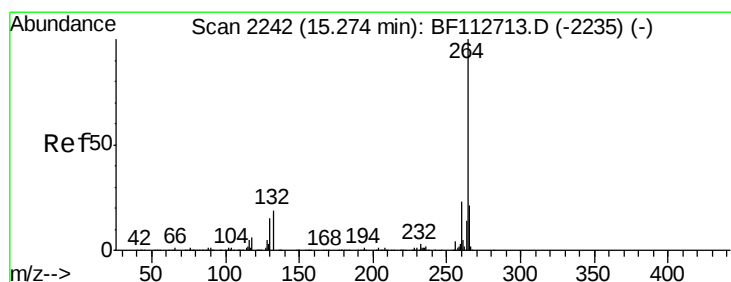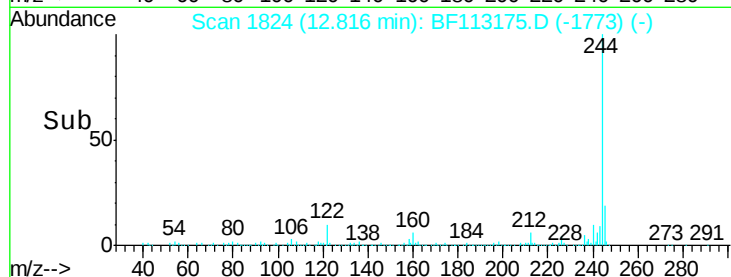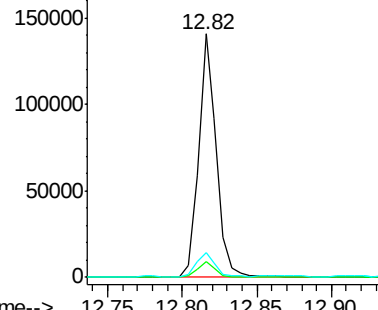

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.28 min Scan# 2243

Delta R.T. 0.01 min

Lab File: BF113175.D

Acq: 20 Mar 2019 17:07


Tgt Ion:264 Resp: 287147

Ion Ratio Lower Upper

264 100

260 24.0 19.2 28.8

265 22.5 17.7 26.5

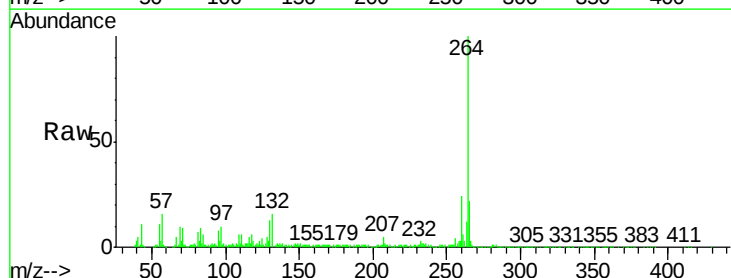

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

