


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032019\
 Data File : BF113162.D
 Acq On : 20 Mar 2019 10:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 13 03:42:55 2019

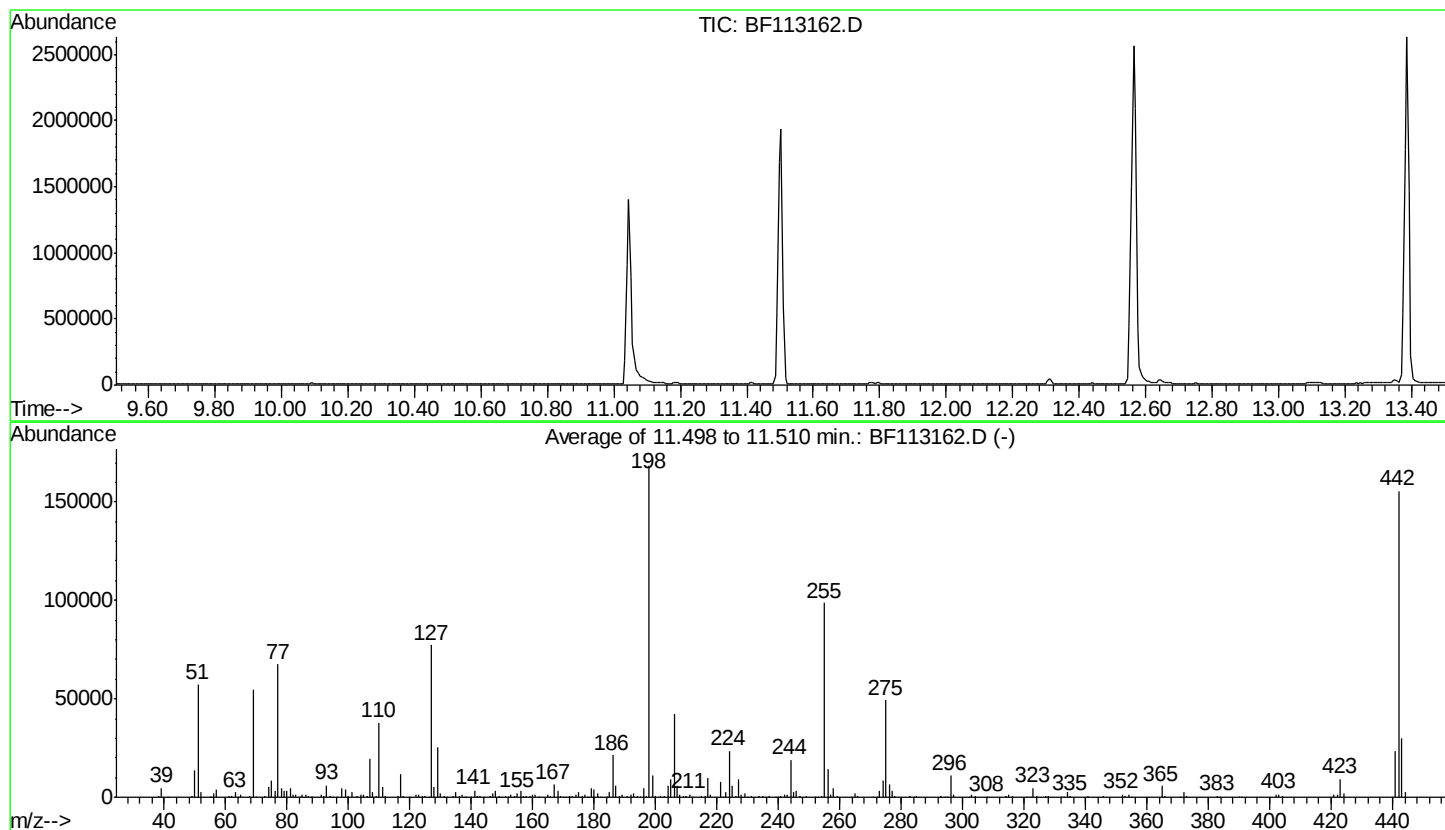

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	57169	PASS
68	69	0.00	2	1.6	844	PASS
69	198	0.00	100	32.3	54417	PASS
70	69	0.00	2	0.4	226	PASS
127	198	10	80	45.8	77128	PASS
197	198	0.00	2	0.3	446	PASS
198	198	100	100	100.0	168429	PASS
199	198	5	9	6.6	11036	PASS
275	198	10	60	29.3	49322	PASS
365	198	1	100	3.4	5789	PASS
441	198	0.01	100	13.9	23336	PASS
442	198	50	100	92.3	155469	PASS
443	442	15	24	19.1	29656	PASS