


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032019\
 Data File : BF113186.D
 Acq On : 20 Mar 2019 23:26
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 13 03:42:55 2019

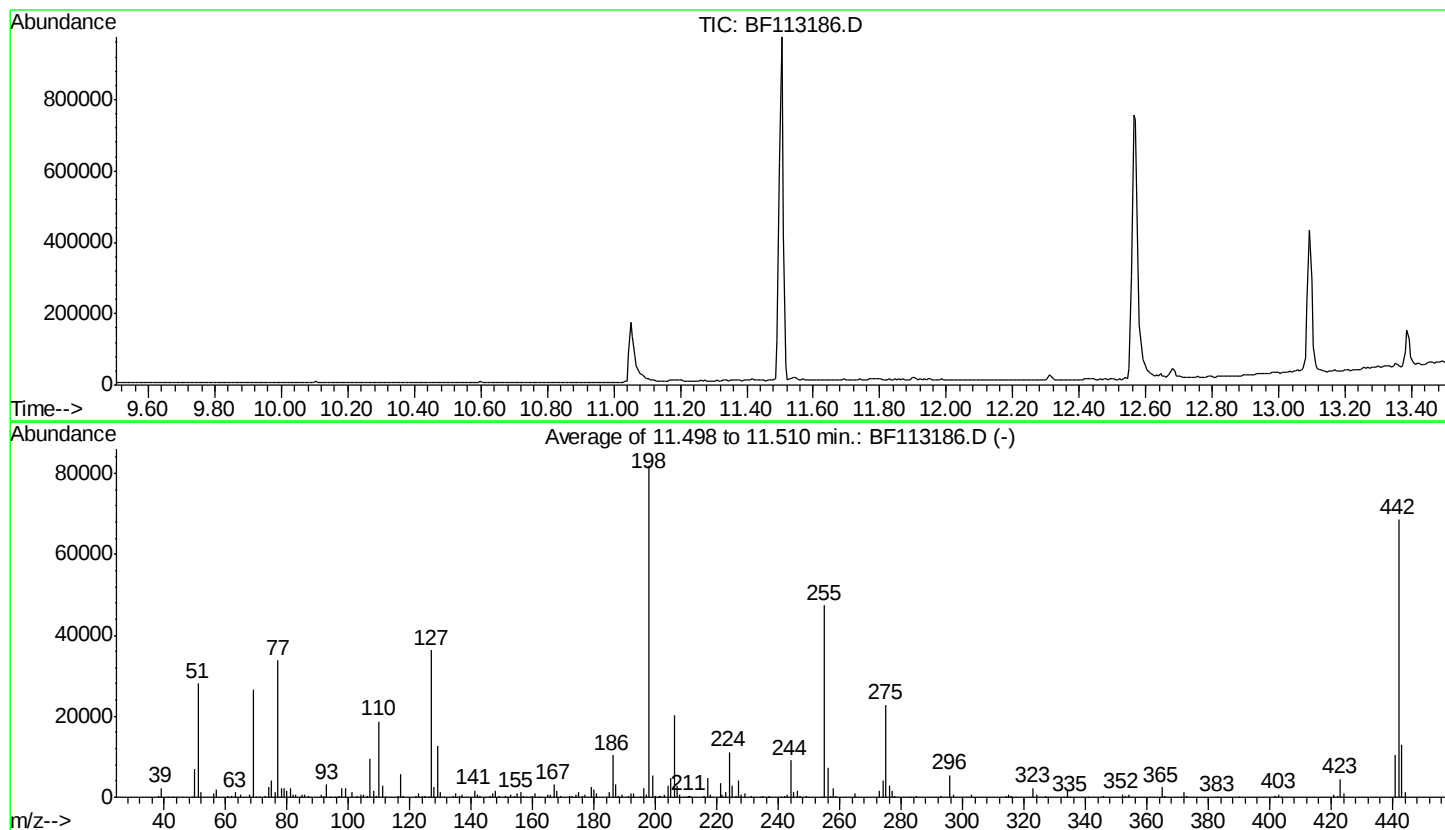

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	28015	PASS
68	69	0.00	2	1.9	496	PASS
69	198	0.00	100	32.3	26449	PASS
70	69	0.00	2	0.4	101	PASS
127	198	10	80	44.3	36253	PASS
197	198	0.00	2	0.6	501	PASS
198	198	100	100	100.0	81898	PASS
199	198	5	9	6.7	5467	PASS
275	198	10	60	28.0	22904	PASS
365	198	1	100	3.1	2515	PASS
441	198	0.01	100	12.9	10528	PASS
442	198	50	100	83.7	68578	PASS
443	442	15	24	18.8	12887	PASS