


Benzaldehyde

Response Ratio

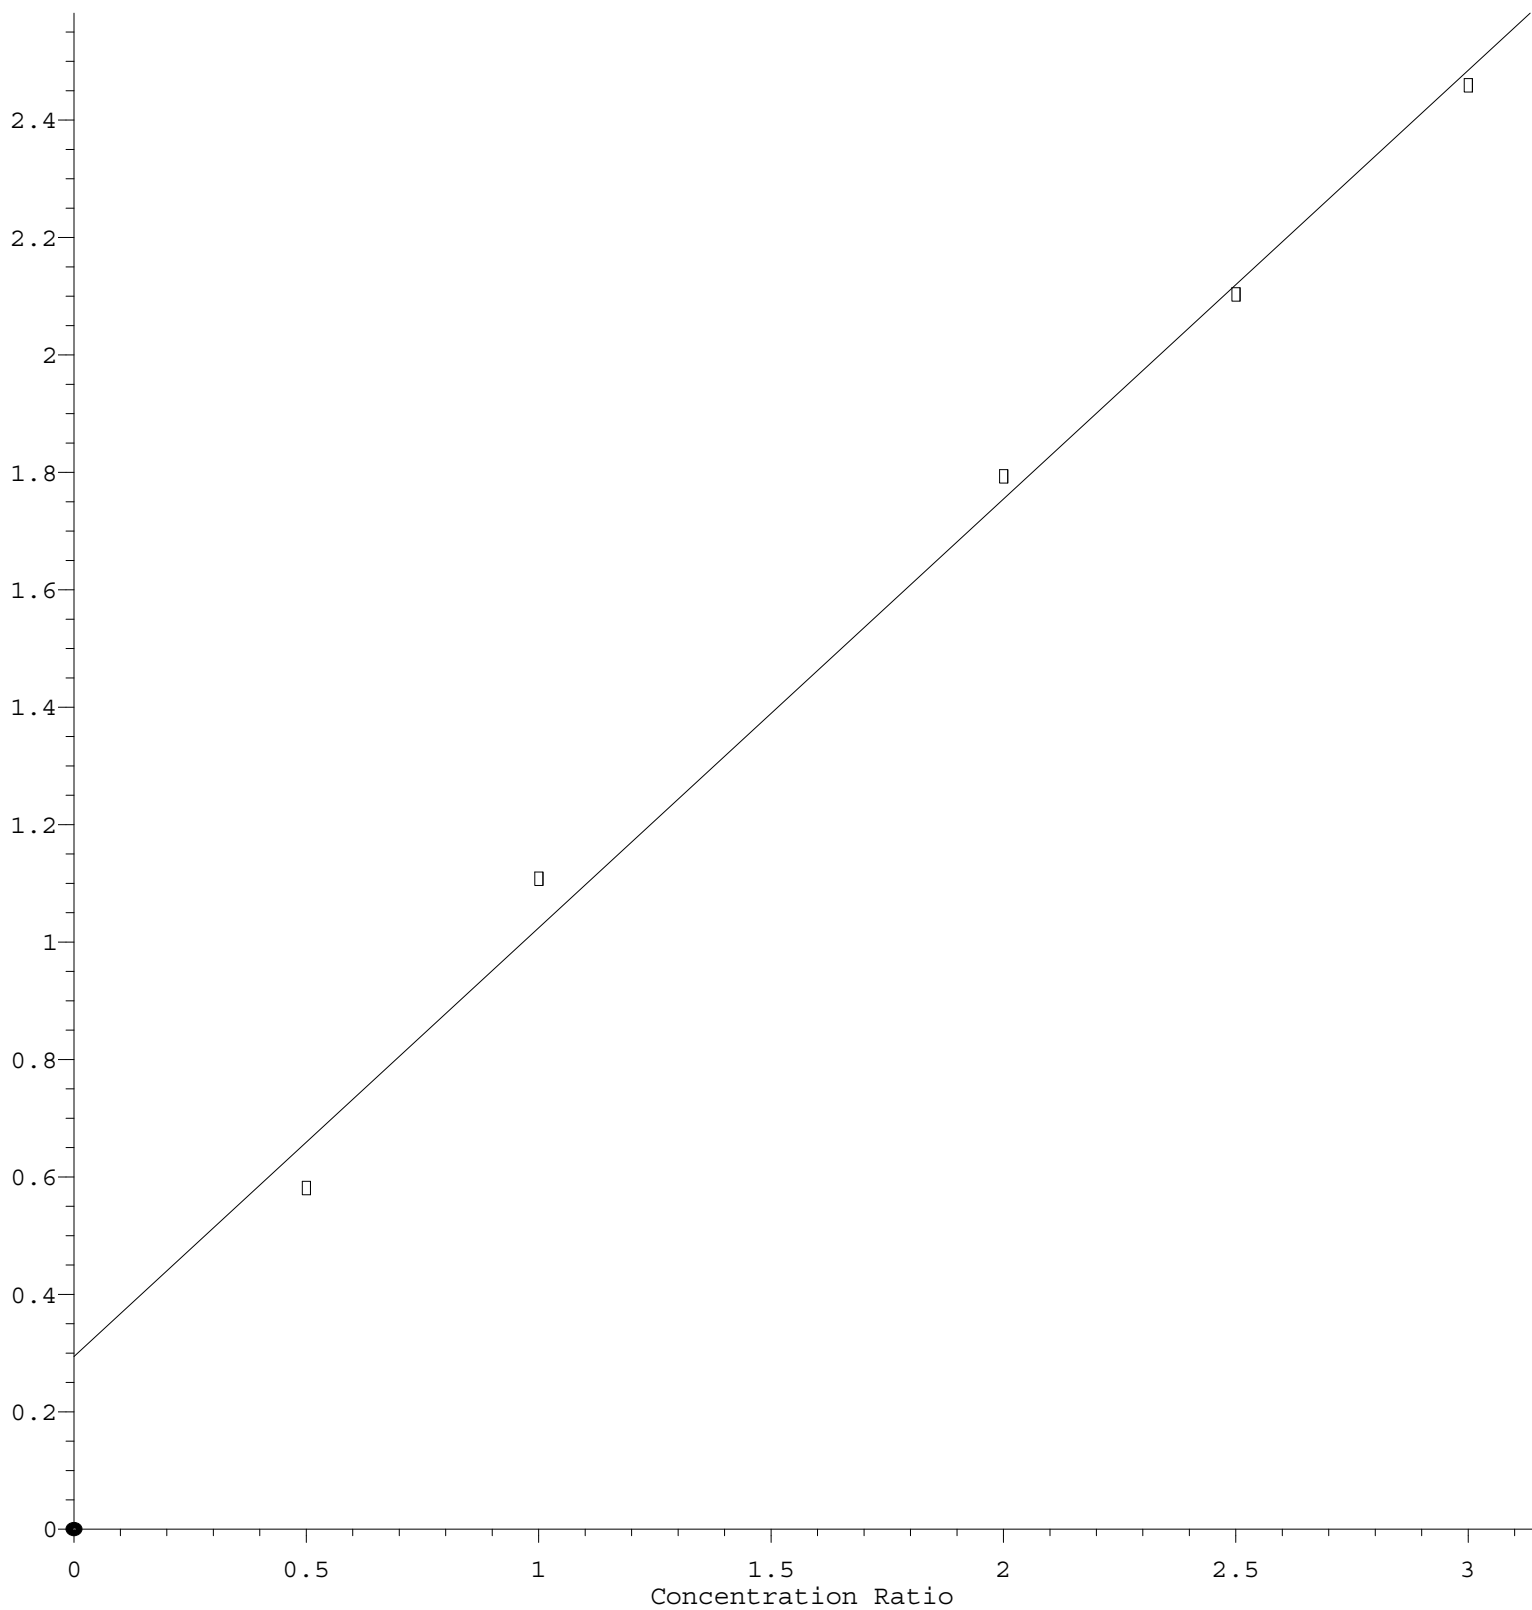


$$\text{Response} = 7.303\text{e-}001 * \text{Amt} + 2.942\text{e-}001$$

Coef of Det (r^2) = 0.993289 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA F\Methods\8270-BF032122.M

Calibration Table Last Updated: Tue Mar 22 02:16:33 2022


Pentachlorophenol

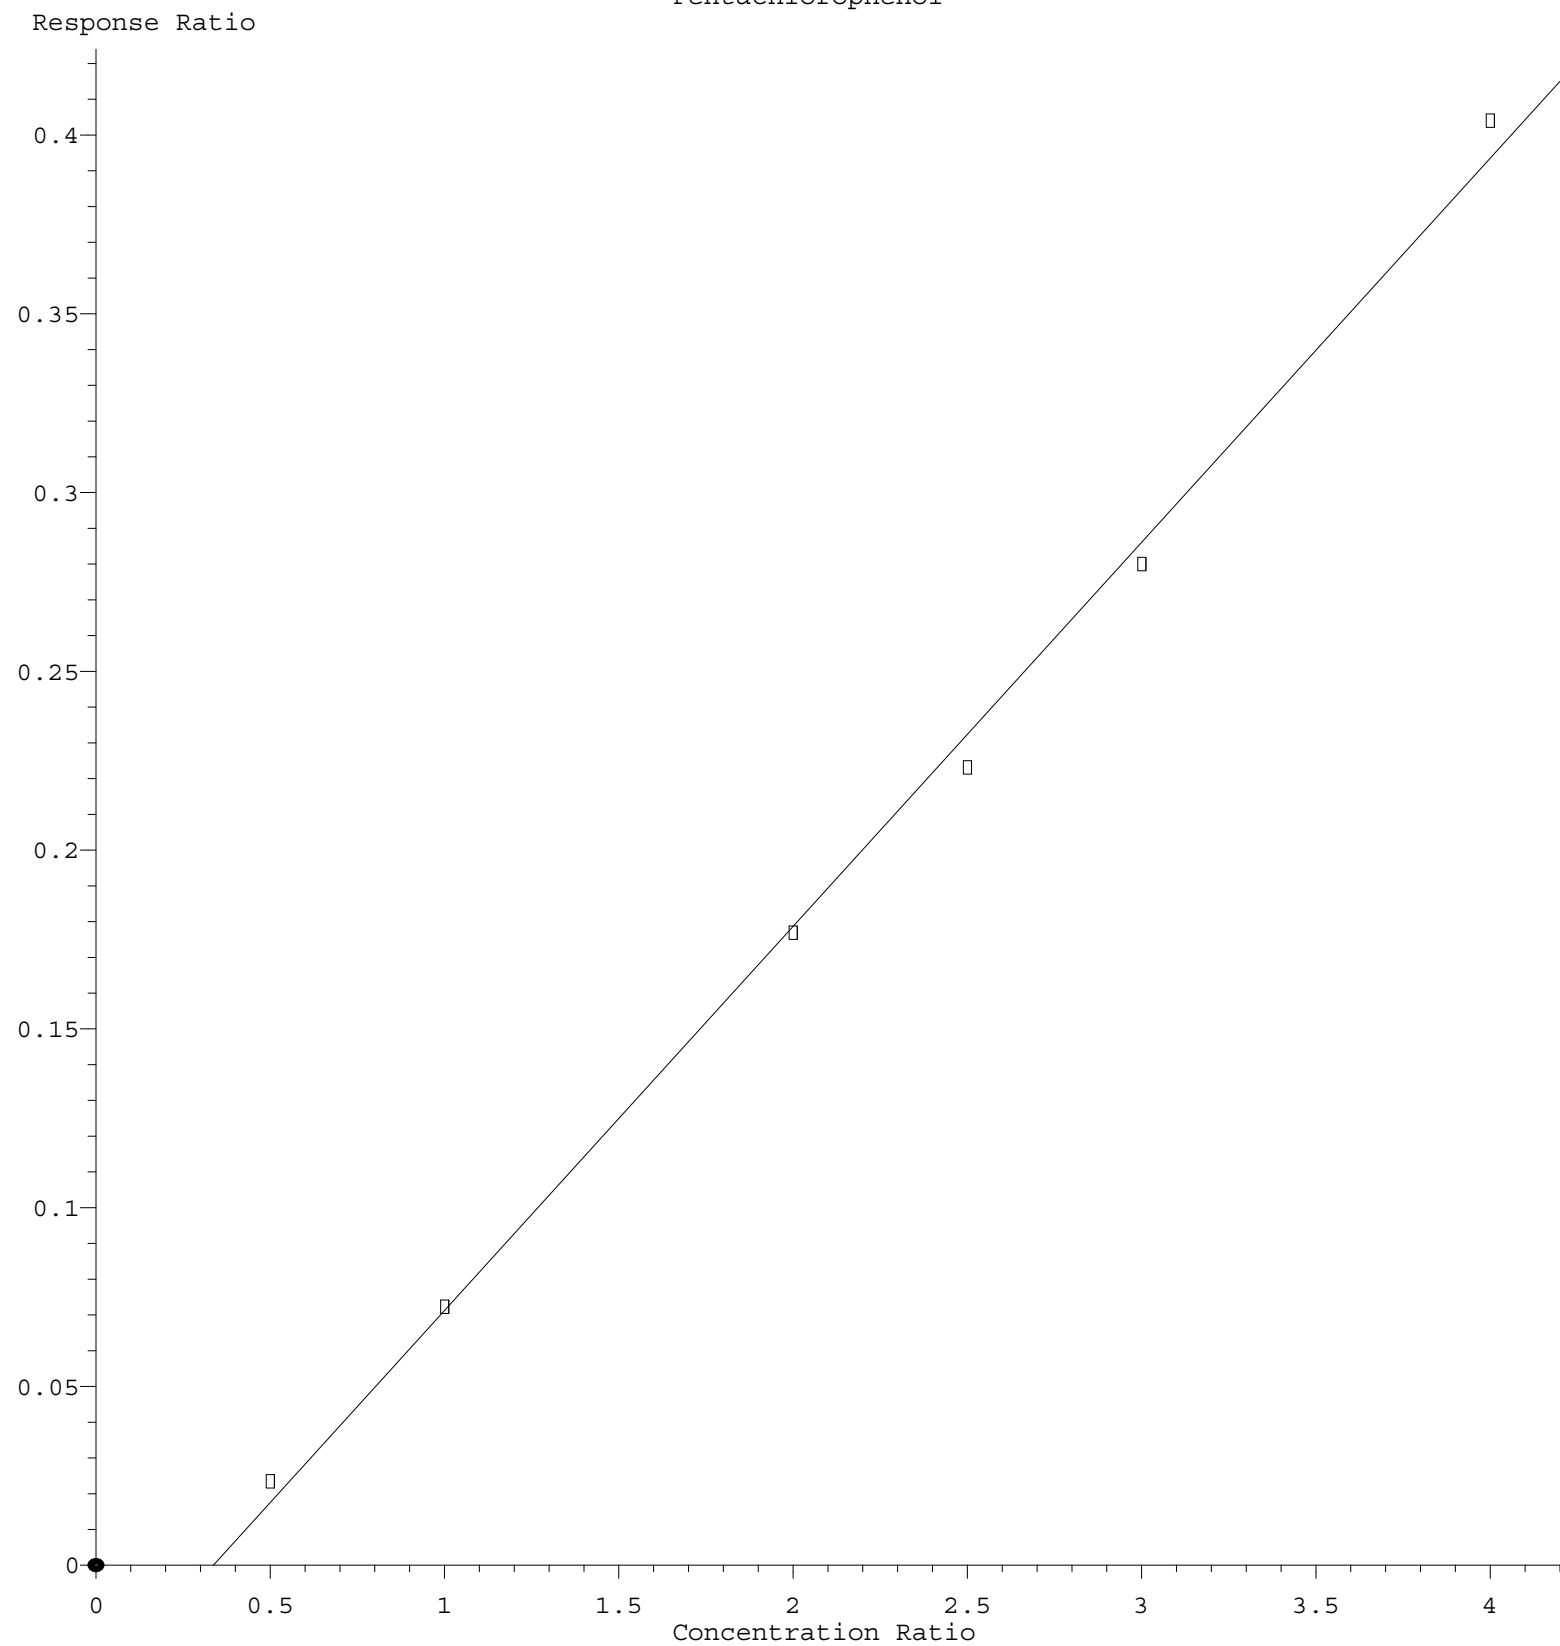

Response = 1.075e-001 * Amt - 3.622e-002
 Coef of Det (r^2) = 0.997178 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA F\Methods\8270-BF032122.M
 Calibration Table Last Updated: Tue Mar 22 02:16:33 2022

Fluorene


Response Ratio

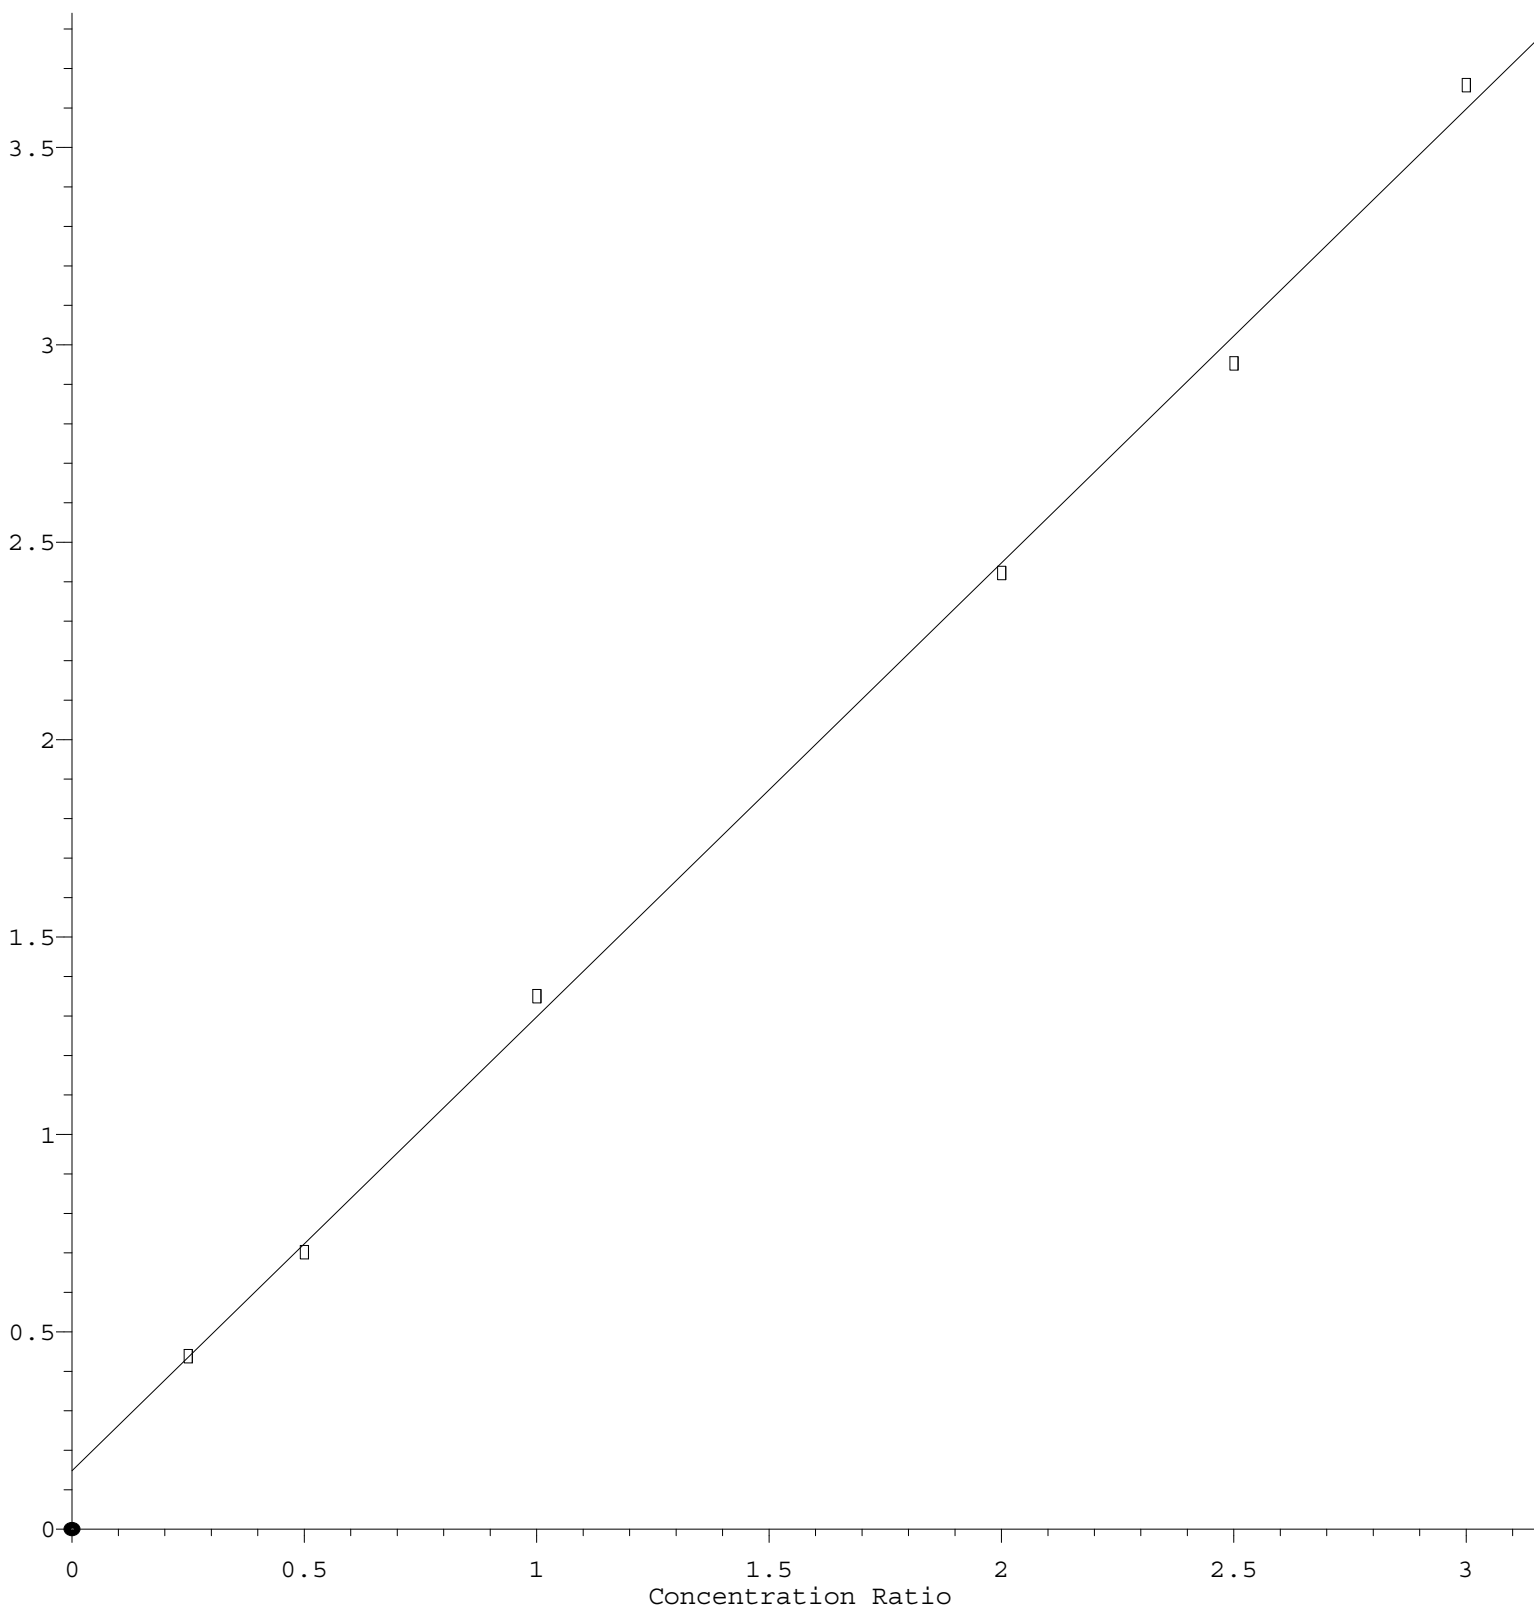

$\text{Response} = 1.150\text{e}+000 * \text{Amt} + 1.477\text{e}-001$
 Coef of Det (r^2) = 0.998523 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA F\Methods\8270-BF032122.M
 Calibration Table Last Updated: Tue Mar 22 02:16:33 2022


Dibenzofuran

Response Ratio

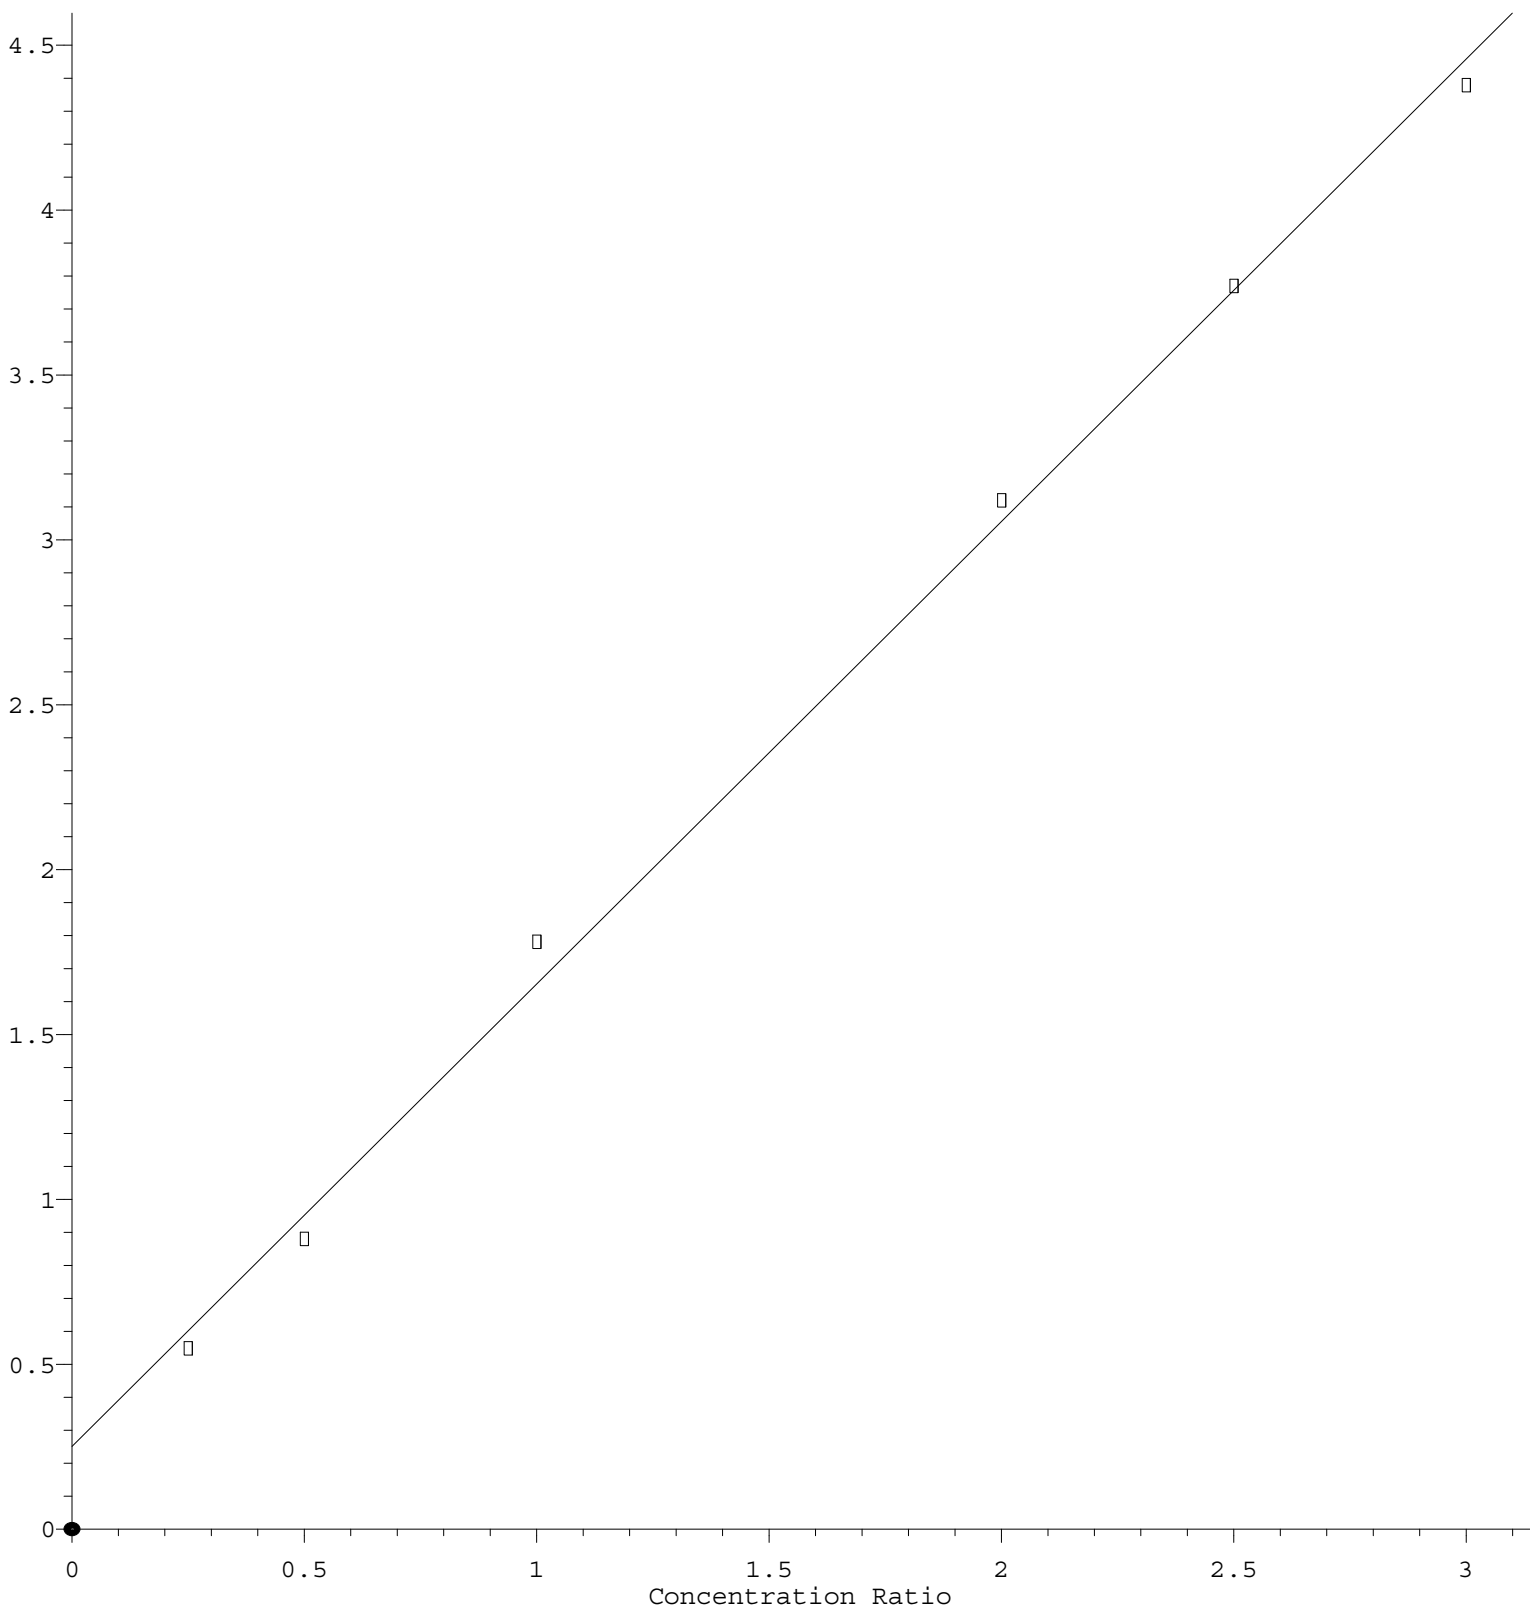

Response = 1.402e+000 * Amt + 2.508e-001
 Coef of Det (r^2) = 0.997181 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA F\Methods\8270-BF032122.M
 Calibration Table Last Updated: Tue Mar 22 02:16:33 2022


2,4-Dinitrophenol

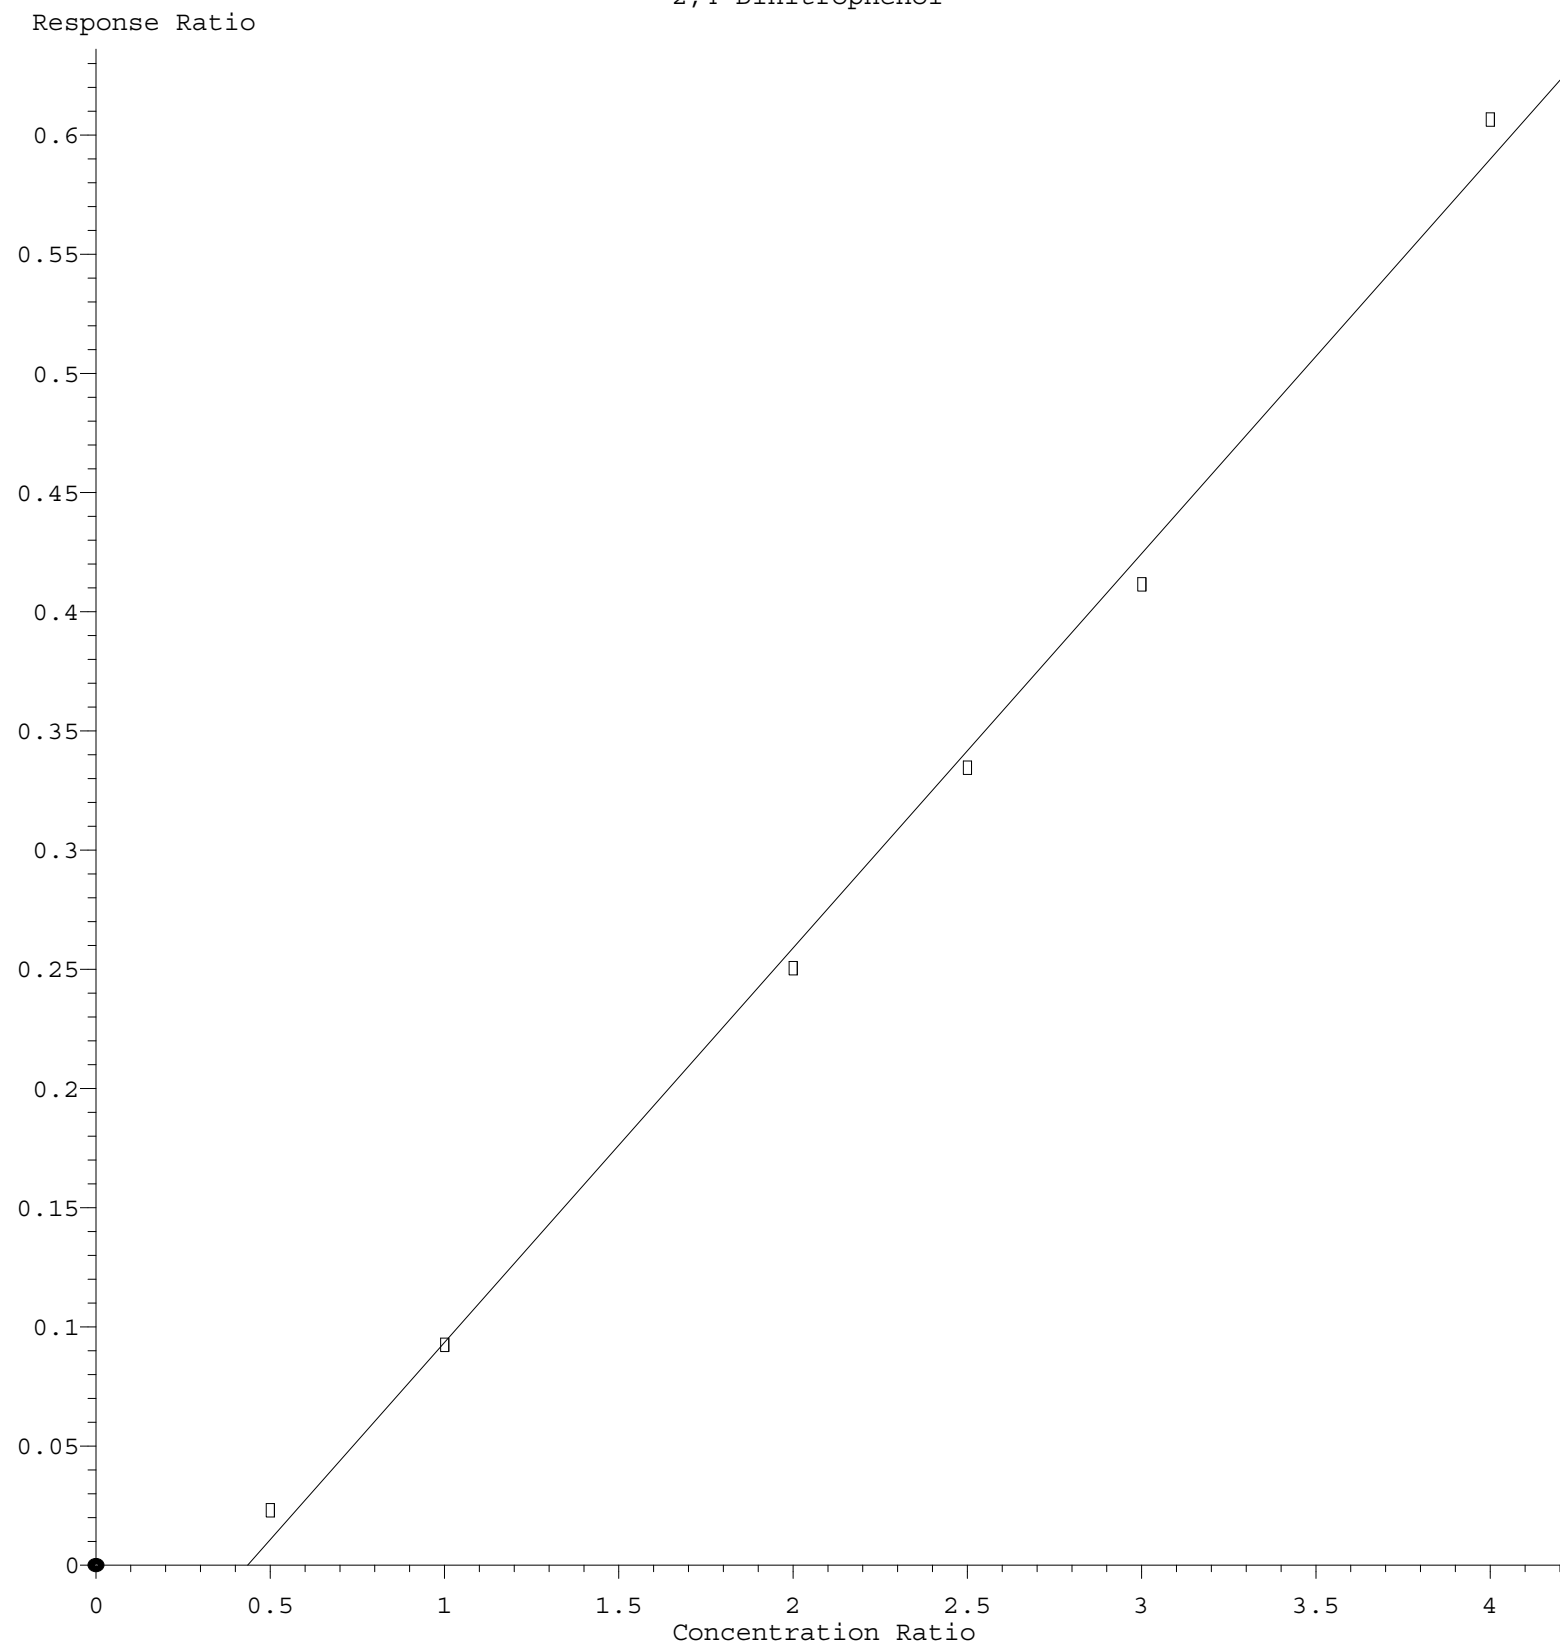

Response = 1.654e-001 * Amt - 7.195e-002
 Coef of Det (r^2) = 0.996865 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA F\Methods\8270-BF032122.M
 Calibration Table Last Updated: Tue Mar 22 02:16:33 2022


Hexachlorocyclopentadiene

Response Ratio

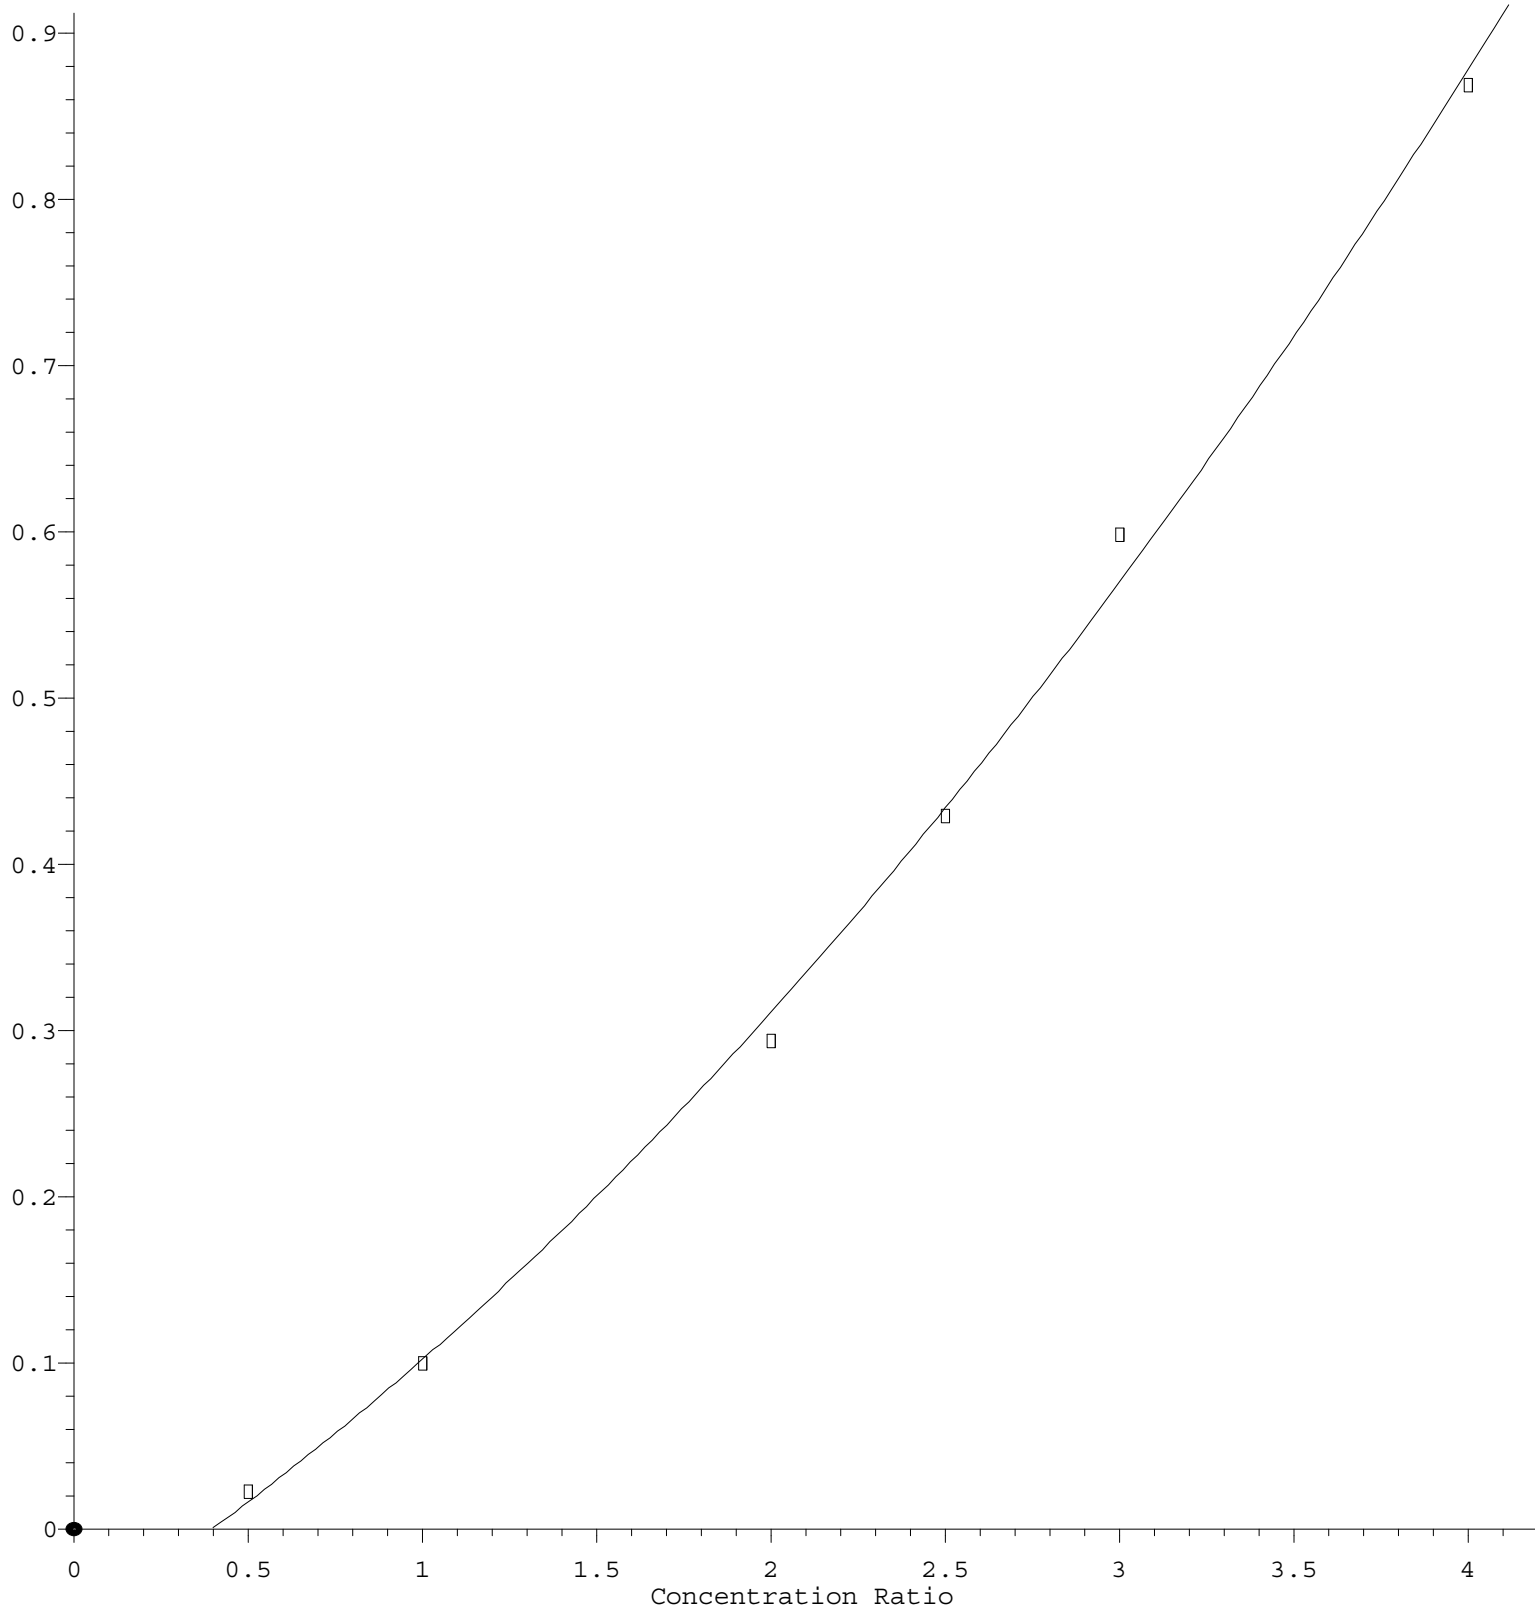

$R = 2.493e-002 A^2 + 1.340e-001 A - 5.678e-002$
Coef of Det (r^2) = 0.997469 Curve Fit: Quadratic
Method Name: Z:\svoasrv\HPCHEM1\BNA F\Methods\8270-BF032122.M
Calibration Table Last Updated: Tue Mar 22 02:16:33 2022

Benzoic acid

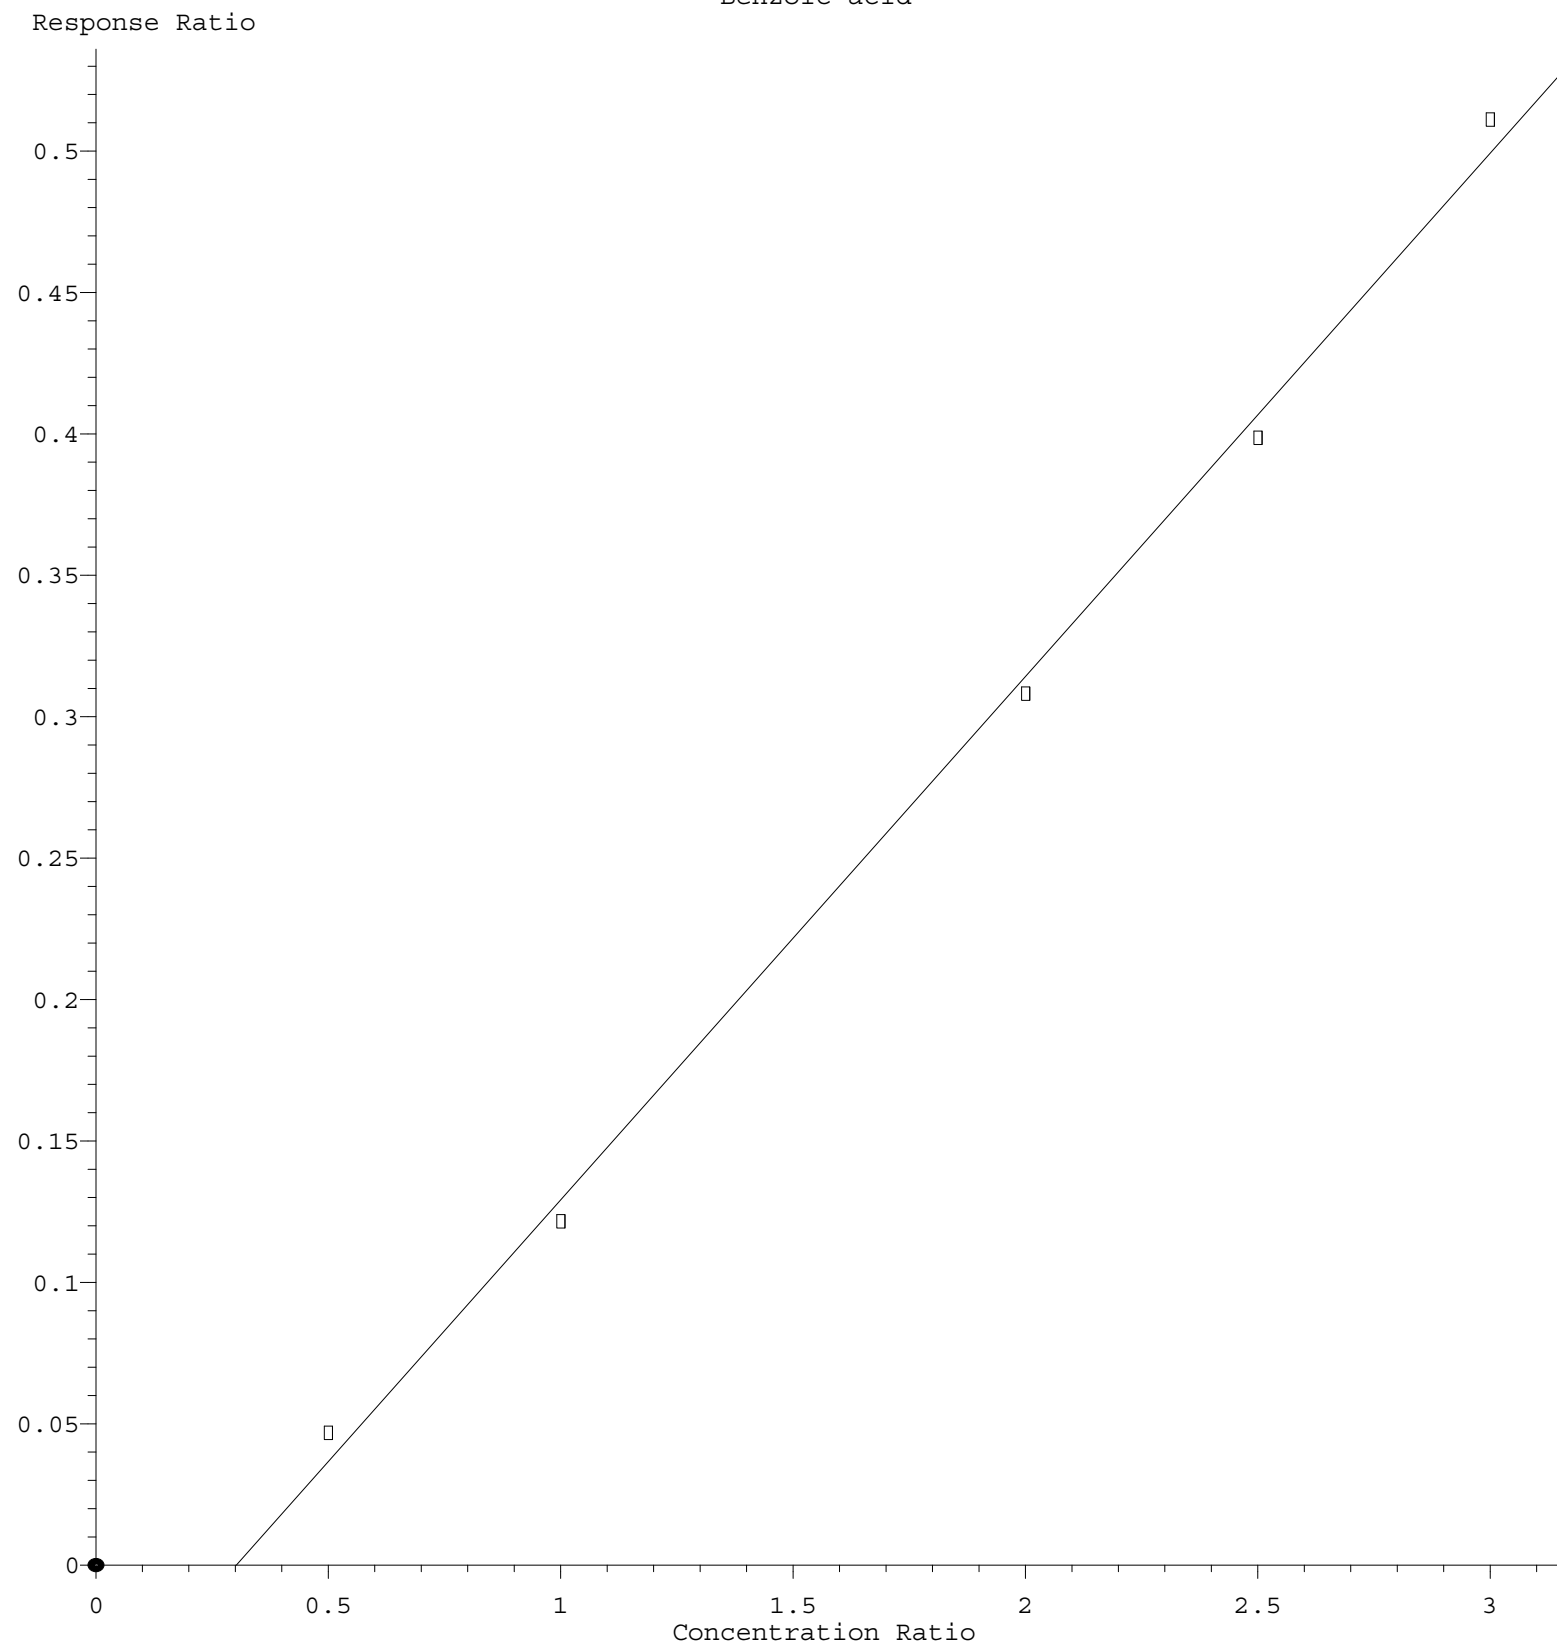

$\text{Response} = 1.851\text{e-}001 * \text{Amt} - 5.592\text{e-}002$
 Coef of Det (r^2) = 0.997264 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA F\Methods\8270-BF032122.M
 Calibration Table Last Updated: Tue Mar 22 02:16:33 2022