
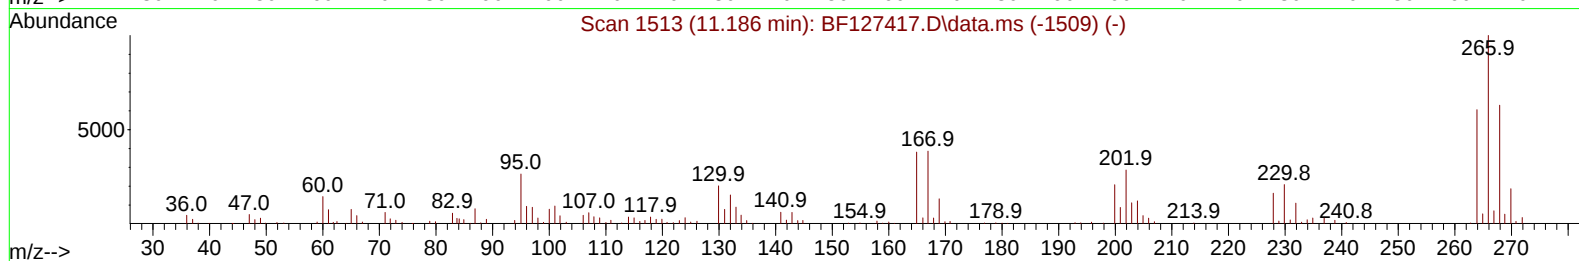
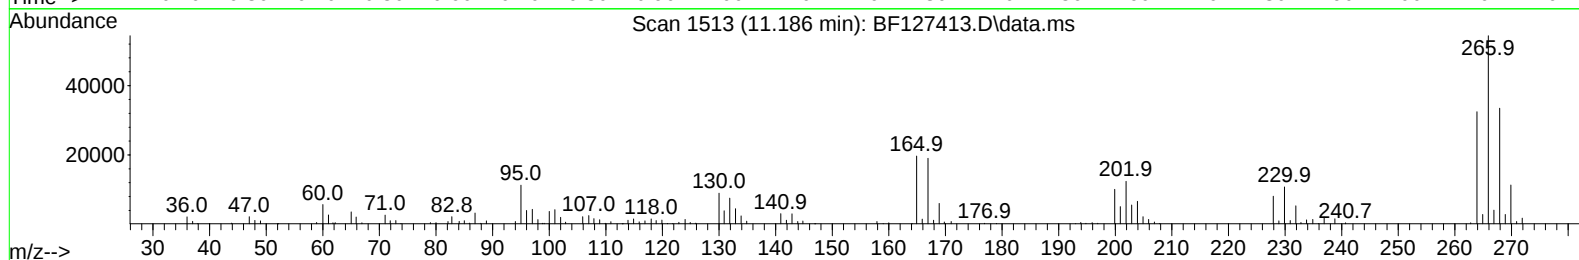


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032122\
Data File : BF127413.D
Acq On : 21 Mar 2022 17:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 03:17:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 22 02:16:33 2022
Response via : Initial Calibration

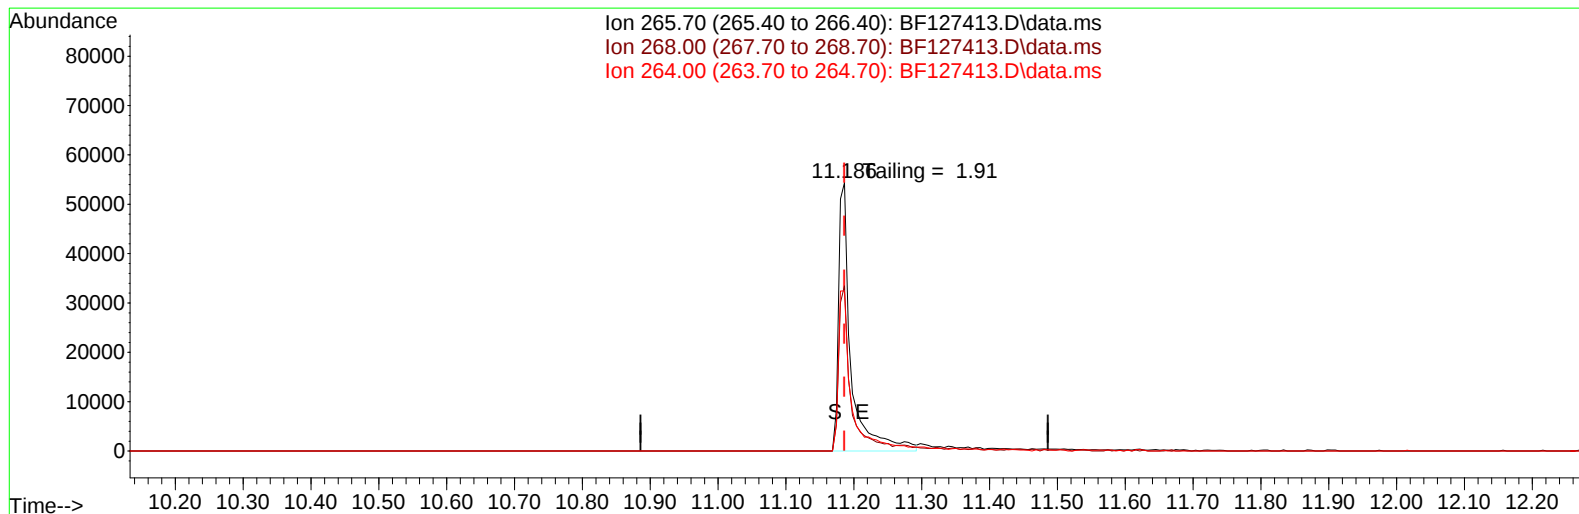

TIC: BF127413.D\data.ms

(70) Pentachlorophenol (C)




11.186min (+ 0.000) 29510.69 ng

response 67535

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	61.53
264.00	60.60	59.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032122\
Data File : BF127413.D
Acq On : 21 Mar 2022 17:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 03:17:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 22 02:16:33 2022
Response via : Initial Calibration

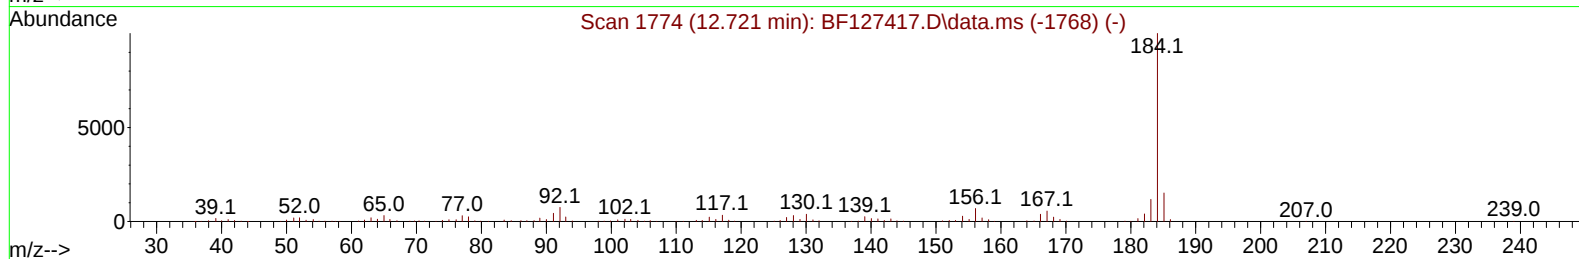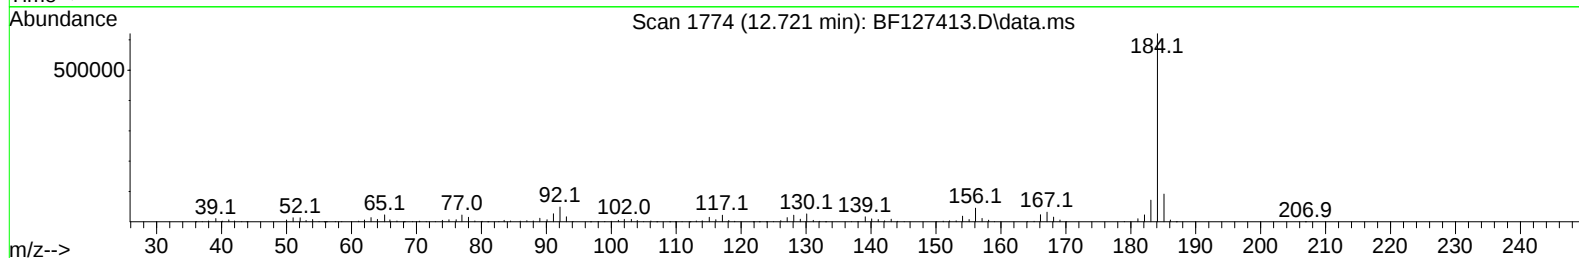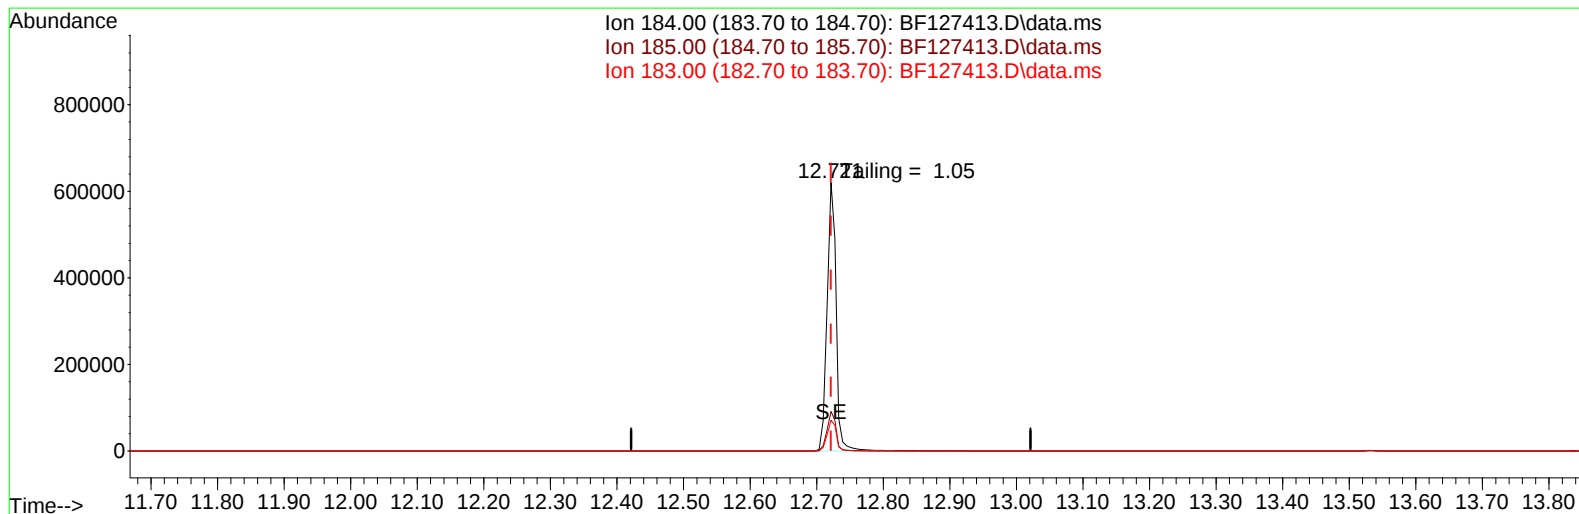

TIC: BF127413.D\data.ms

(77) Benzidine

12.721min (0.000) 0.00 ng

response 586347

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.71
183.00	11.70	11.48
0.00	0.00	0.00