
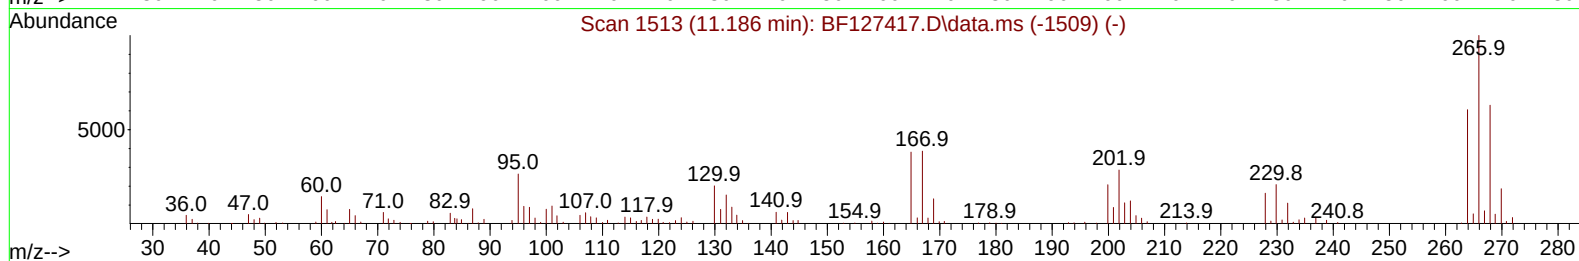
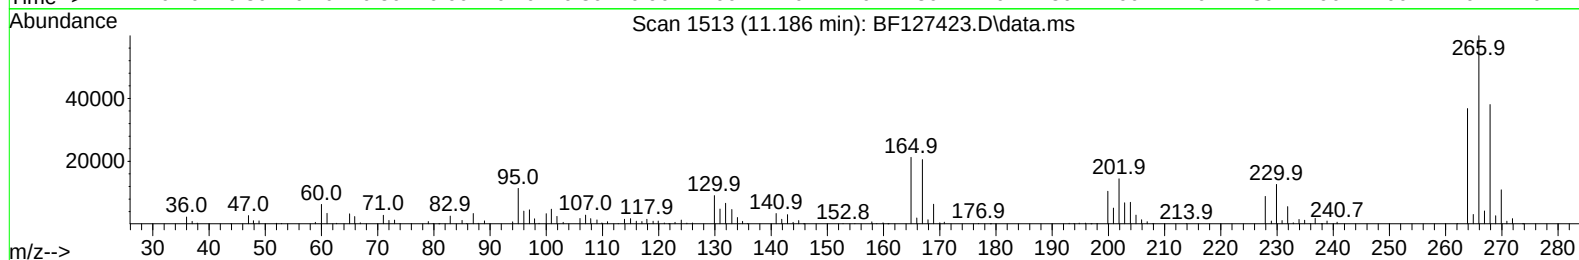


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032122\
Data File : BF127423.D
Acq On : 21 Mar 2022 23:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 06:38:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 22 02:16:33 2022
Response via : Initial Calibration

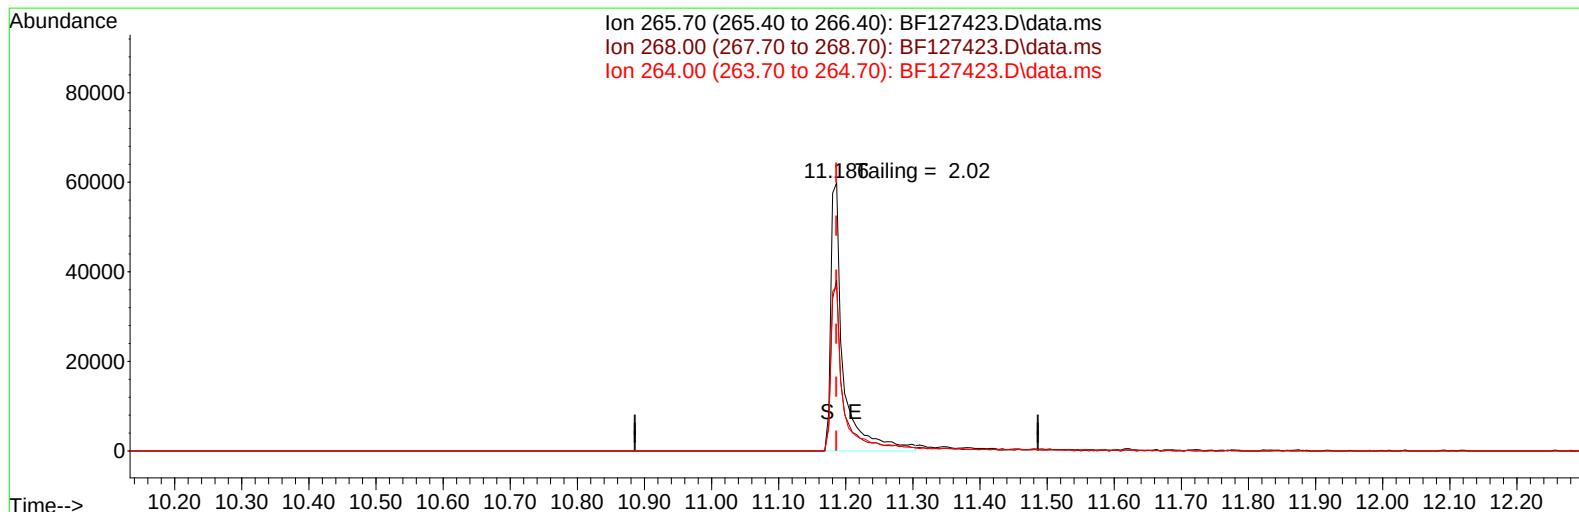

TIC: BF127423.D\data.ms

(70) Pentachlorophenol (C)




11.186min (+ 0.000) 25625.80 ng

response 76538

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.52
264.00	60.60	61.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032122\
Data File : BF127423.D
Acq On : 21 Mar 2022 23:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 06:38:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 22 02:16:33 2022
Response via : Initial Calibration

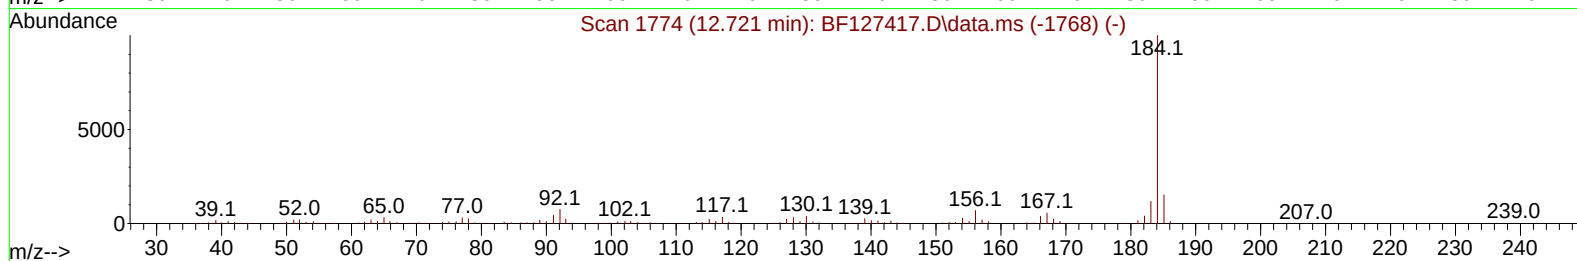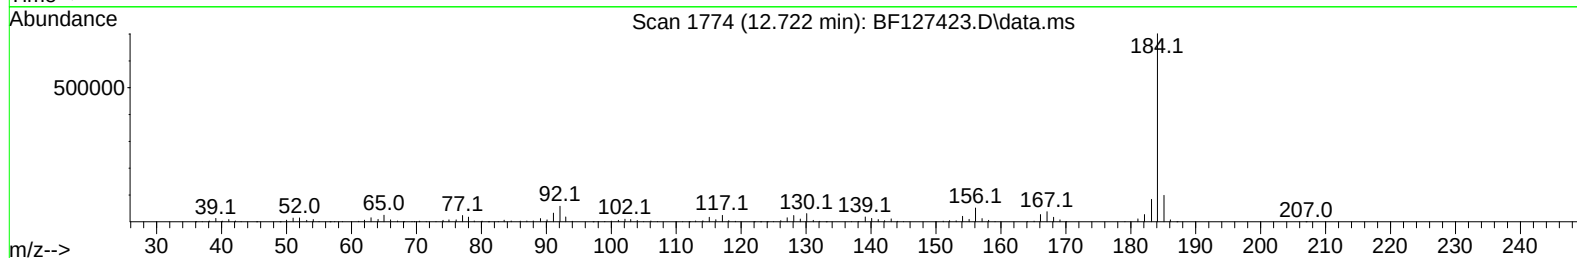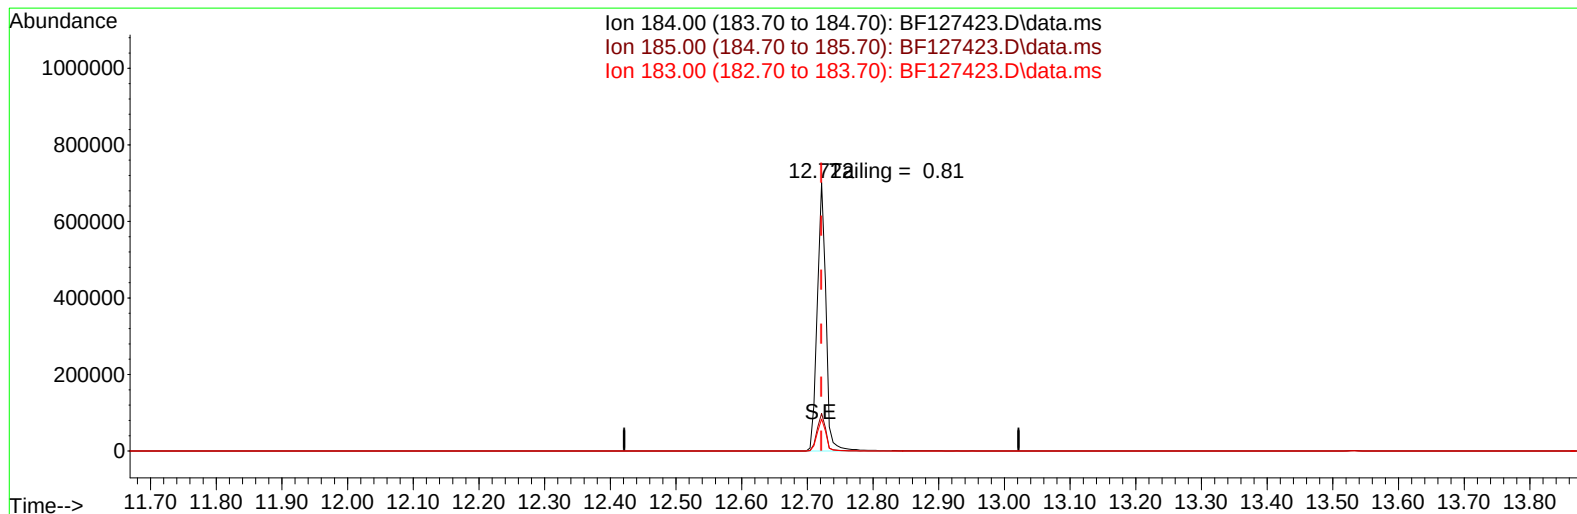

TIC: BF127423.D\data.ms

(77) Benzidine

12.722min (+ 0.000) 0.00 ng

response 648519

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.03
183.00	11.70	11.94
0.00	0.00	0.00