

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032122\
 Data File : BF127425.D
 Acq On : 22 Mar 2022 00:24
 Operator : CG\JU
 Sample : PB143487BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143487BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	539	543	560	rBV	2959658	3169856	79.17%	13.212%
2	6.487	709	714	717	rBV	2825209	3176142	79.33%	13.238%
3	6.845	772	775	784	rBV	830122	682795	17.05%	2.846%
4	7.416	867	872	875	rBV	2104254	2210229	55.20%	9.212%
5	8.128	989	993	1006	rBV	1033773	901458	22.52%	3.757%
6	9.210	1171	1177	1180	rBV	3461945	3632694	90.73%	15.141%
7	9.886	1288	1292	1295	rBV	1234704	1036155	25.88%	4.319%
8	10.680	1423	1427	1430	rBV	2367894	2143213	53.53%	8.933%
9	11.374	1542	1545	1553	rBV	1249890	1109640	27.72%	4.625%
10	12.968	1810	1816	1819	rBV	3910860	4003683	100.00%	16.687%
11	14.021	1991	1995	2005	rBV	1072314	938725	23.45%	3.913%
12	15.498	2240	2246	2260	rVB	516116	722789	18.05%	3.013%
13	15.921	2313	2318	2324	rBV2	32758	50540	1.26%	0.211%
14	16.427	2399	2404	2410	rBV2	27891	48686	1.22%	0.203%
15	17.021	2499	2505	2511	rBV3	18332	42692	1.07%	0.178%
16	17.115	2511	2521	2537	rVB4	27009	123134	3.08%	0.513%




Sum of corrected areas: 23992431

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032122\
Data File : BF127425.D
Acq On : 22 Mar 2022 00:24
Operator : CG\JU
Sample : PB143487BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143487BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

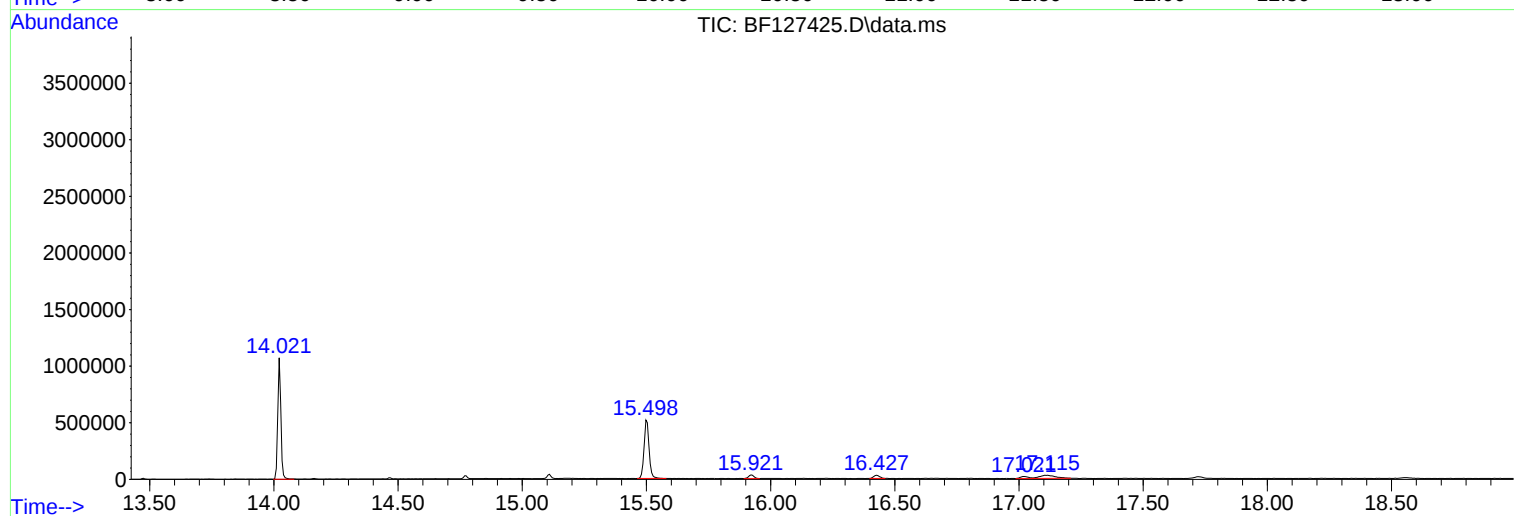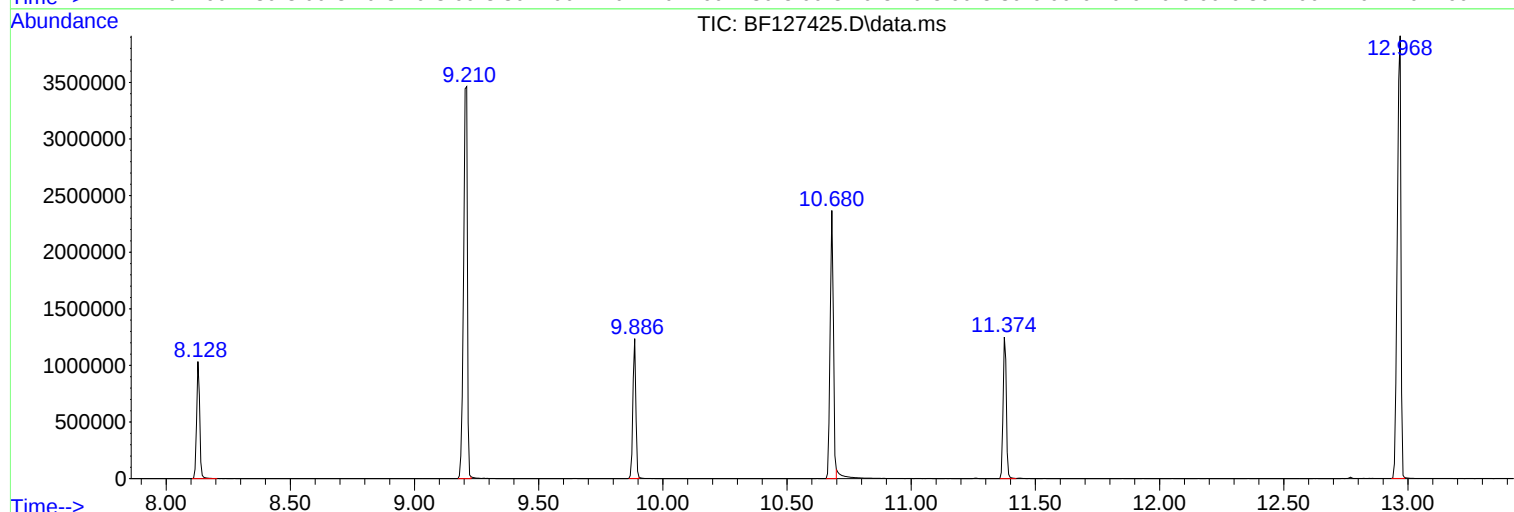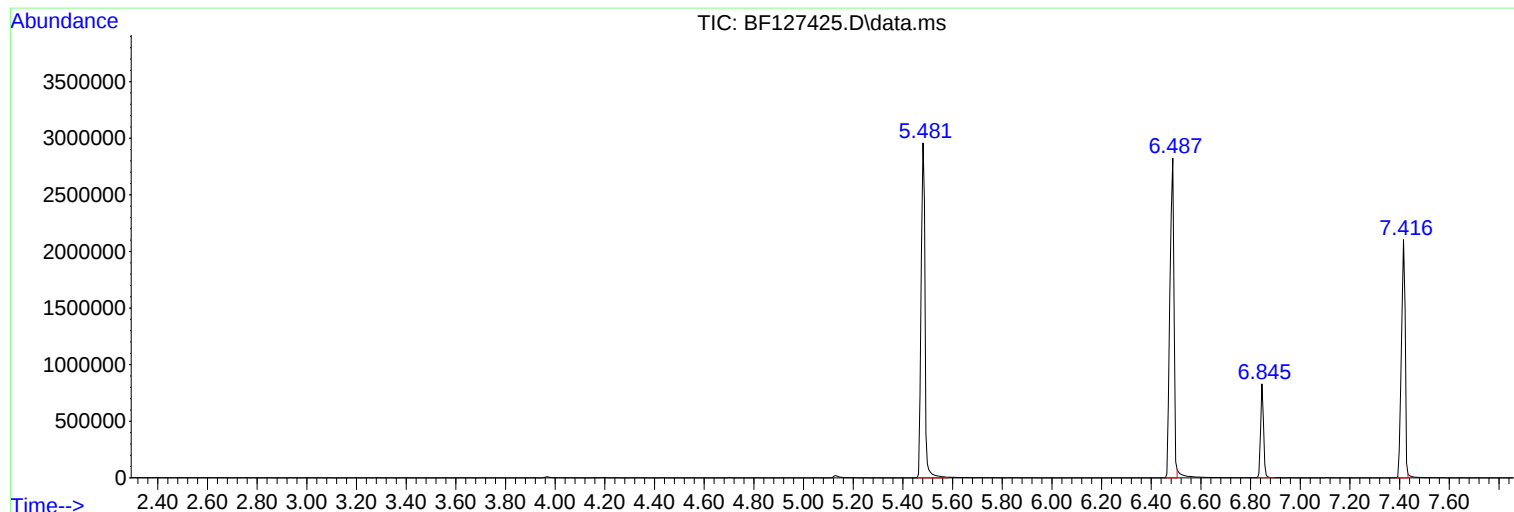

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032122\
Data File : BF127425.D
Acq On : 22 Mar 2022 00:24
Operator : CG\JU
Sample : PB143487BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143487BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (1,1'-Biphenyl)-4,4'-diamin... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.115	3.41 ng	123134	Perylene-d12	15.498

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			(1,1'-Biphenyl)-4,4'-diamine, N,...	360	C26H20N2	006311-48-4	87
2			4-Amino-3-[3-(trifluoromethyl)ph...	360	C14H15F3N2O2SSi	1010500-98-0	58
3			Benzaldehyde, 4-hydroxy-3,5-dime...	360	C18H20N2O6	014414-32-5	53
4			1,3,2-Dioxaborolane, bis(spiro[4...	360	C20H13B06	1000150-23-7	50
5			1H-isindole-1,3(2H)-dione, 2-[5...	360	C21H16N2O4	1000398-48-8	50

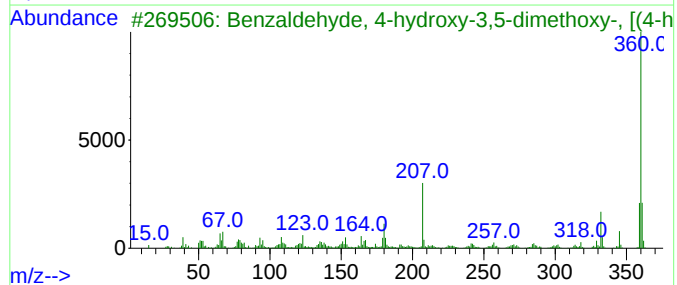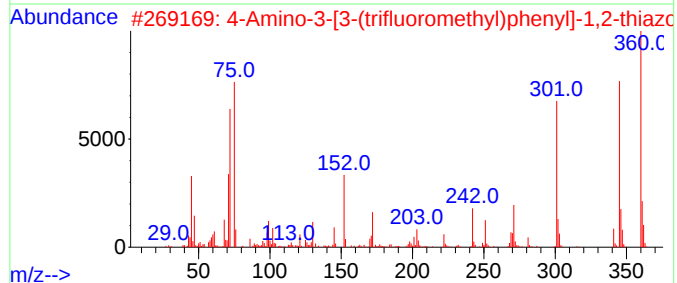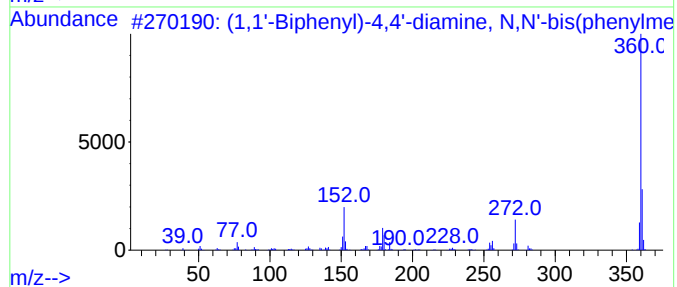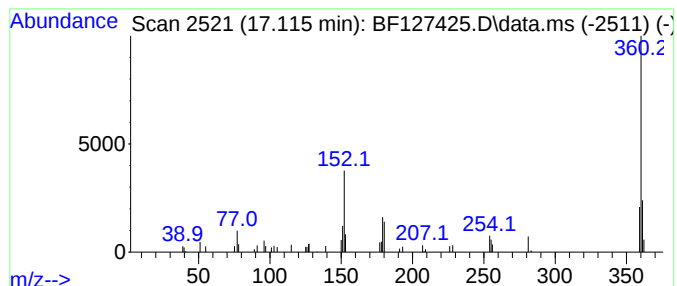

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032122\
Data File : BF127425.D
Acq On : 22 Mar 2022 00:24
Operator : CG\JU
Sample : PB143487BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143487BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(1,1'-Biphenyl)...	17.115	3.4	ng	123134	6	15.498	722789	20.0