
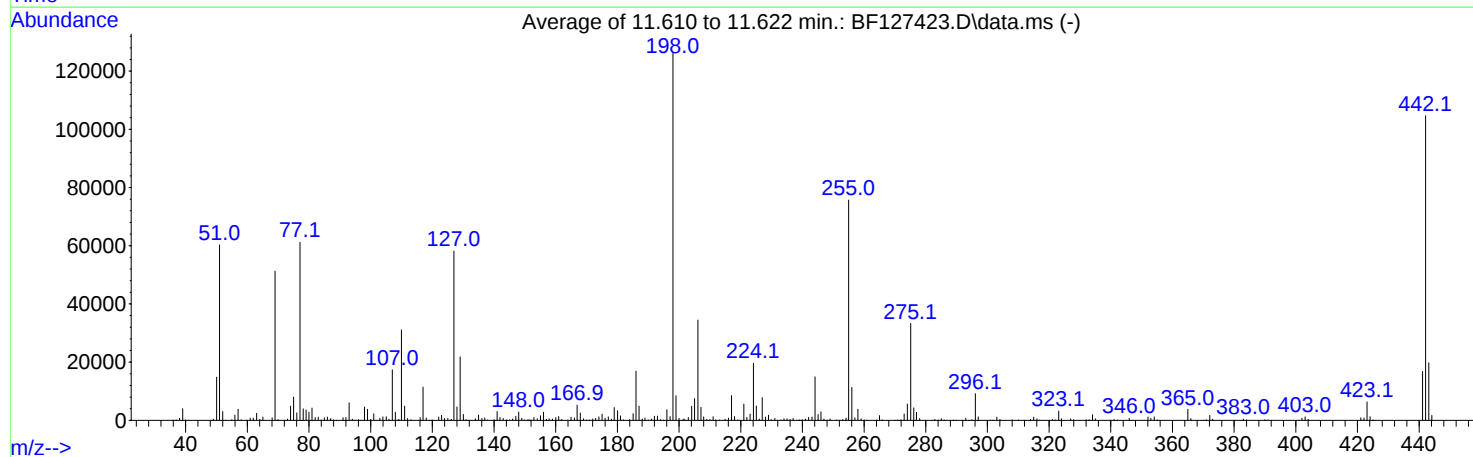


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032122\
 Data File : BF127423.D
 Acq On : 21 Mar 2022 23:27
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 22 02:16:33 2022

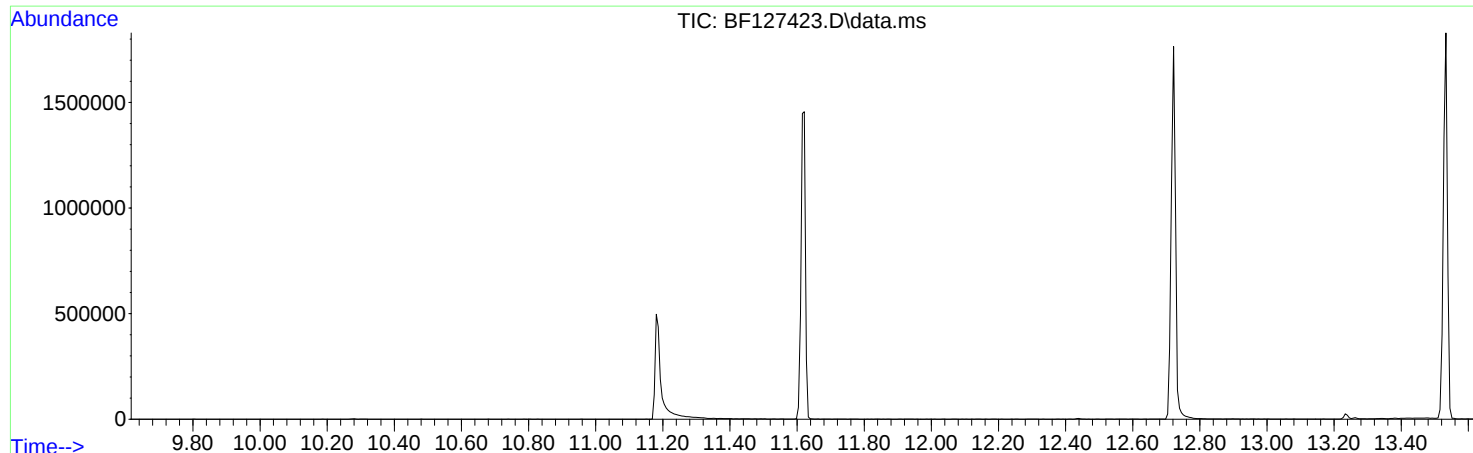




AutoFind: Scans 1585, 1586, 1587; Background Corrected with Scan 1580

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.7	60323	PASS
68	69	0.00	2	1.8	902	PASS
69	198	0.00	100	40.6	51277	PASS
70	69	0.00	2	0.5	274	PASS
127	198	10	80	46.0	58181	PASS
197	198	0.00	2	1.0	1326	PASS
198	198	100	100	100.0	126397	PASS
199	198	5	9	6.7	8475	PASS
275	198	10	60	26.4	33310	PASS
365	198	1	100	3.0	3791	PASS
441	198	0.01	100	13.3	16845	PASS
442	442	50	100	100.0	104656	PASS
443	442	15	24	18.9	19819	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032122\
Data File : BF127423.D
Acq On : 21 Mar 2022 23:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 22 06:38:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 22 02:16:33 2022
Response via : Initial Calibration

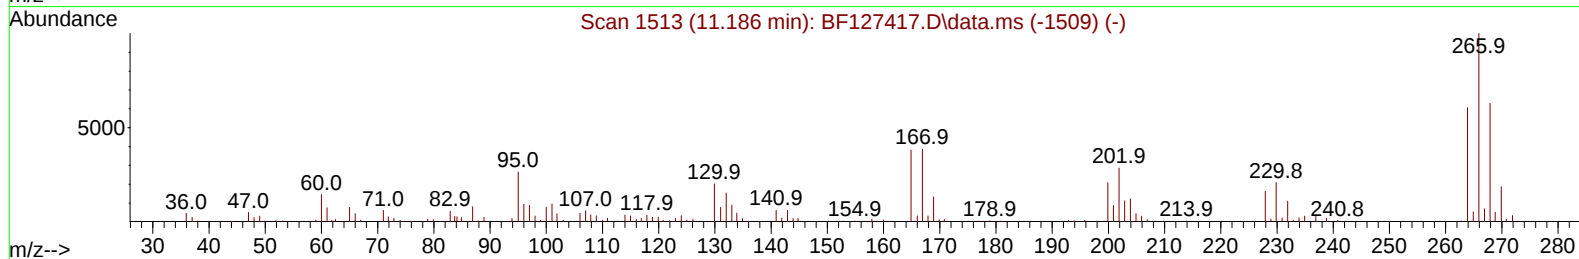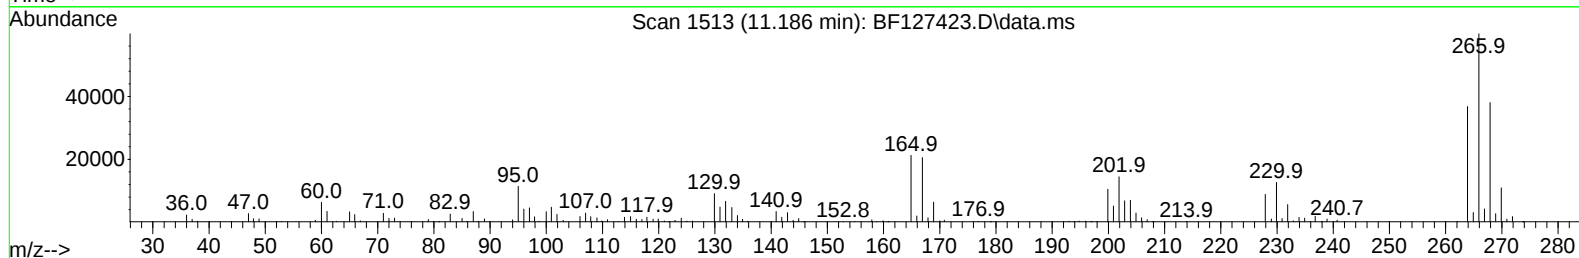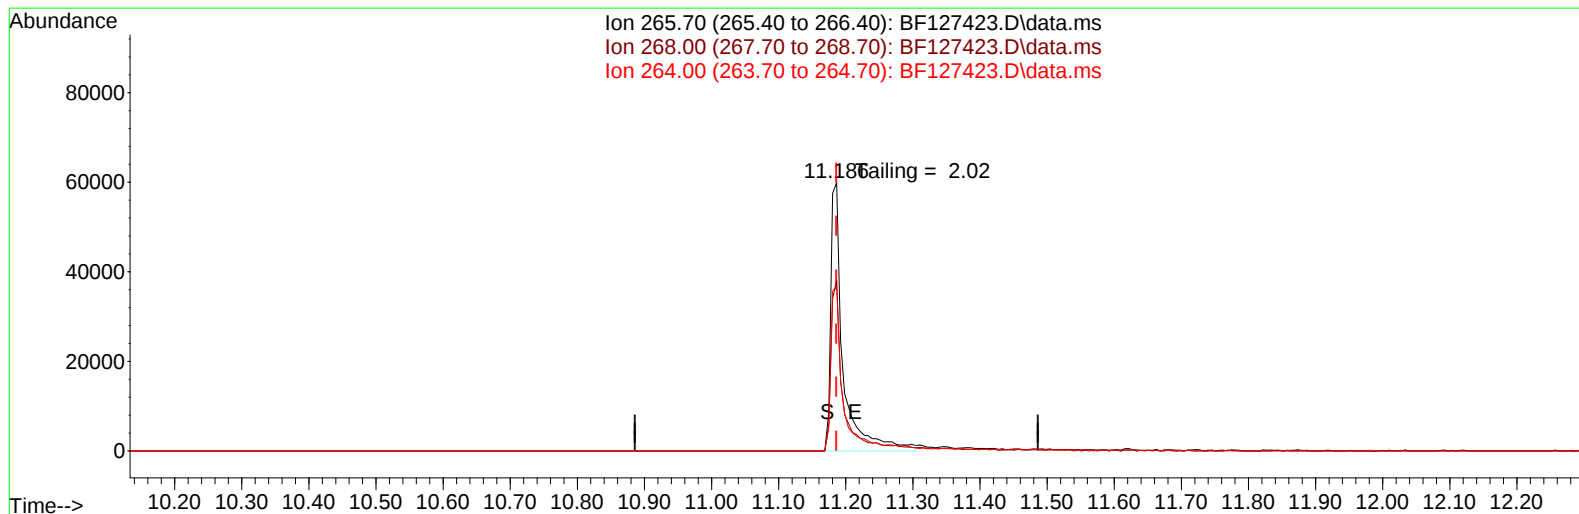

TIC: BF127423.D\data.ms

(70) Pentachlorophenol (C)

11.186min (+ 0.000) 25625.80 ng




response 76538

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.52
264.00	60.60	61.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032122\
 Data File : BF127423.D
 Acq On : 21 Mar 2022 23:27
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 22 06:38:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 22 02:16:33 2022
 Response via : Initial Calibration

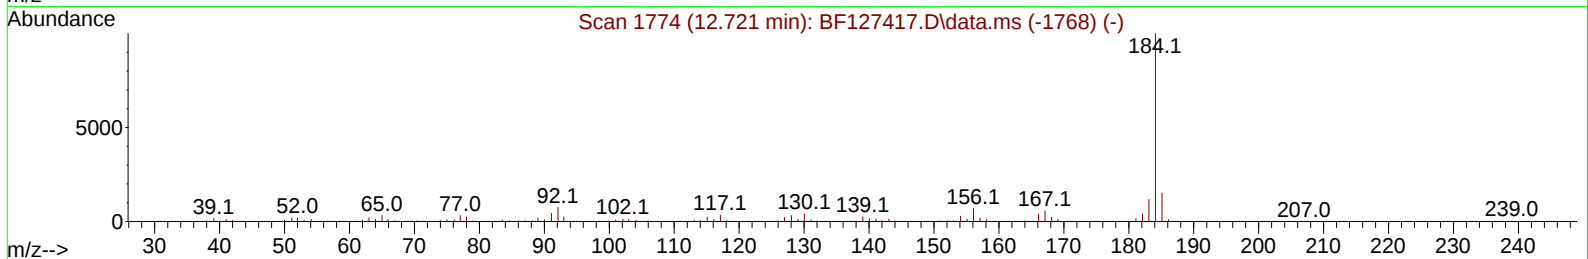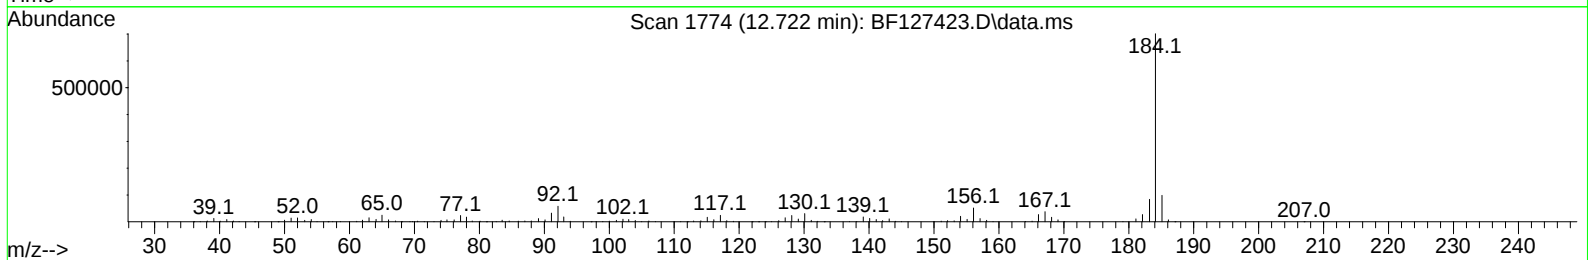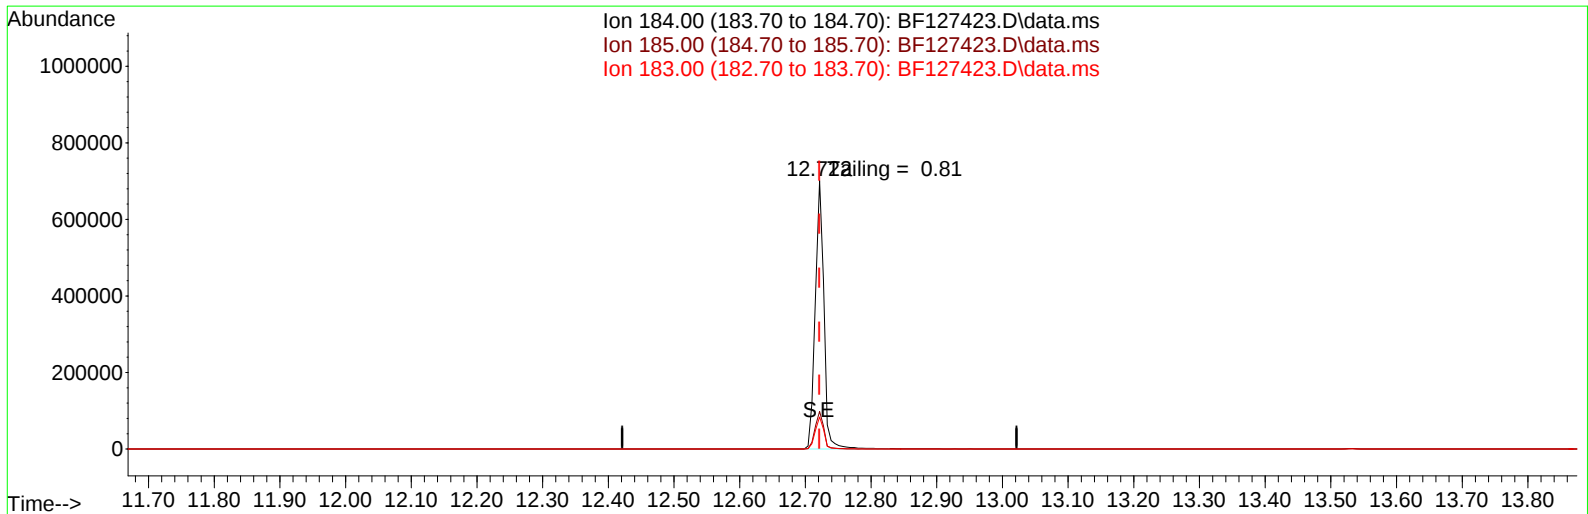

TIC: BF127423.D\data.ms

(77) Benzidine

12.722min (+ 0.000) 0.00 ng

response 648519

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.03
183.00	11.70	11.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/21/2022	BNA_F	<u>BF127423.D</u>
Compound Name	Response	Retention Time
DDT	310333	13.533
DDD	6830	13.233
DDE	417	12.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7247	317580	2.28

Instrument :
BNA_F
ClientSampleId :
DFTPP