


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032219\
 Data File : BF113228.D
 Acq On : 22 Mar 2019 12:08
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 13 03:42:55 2019

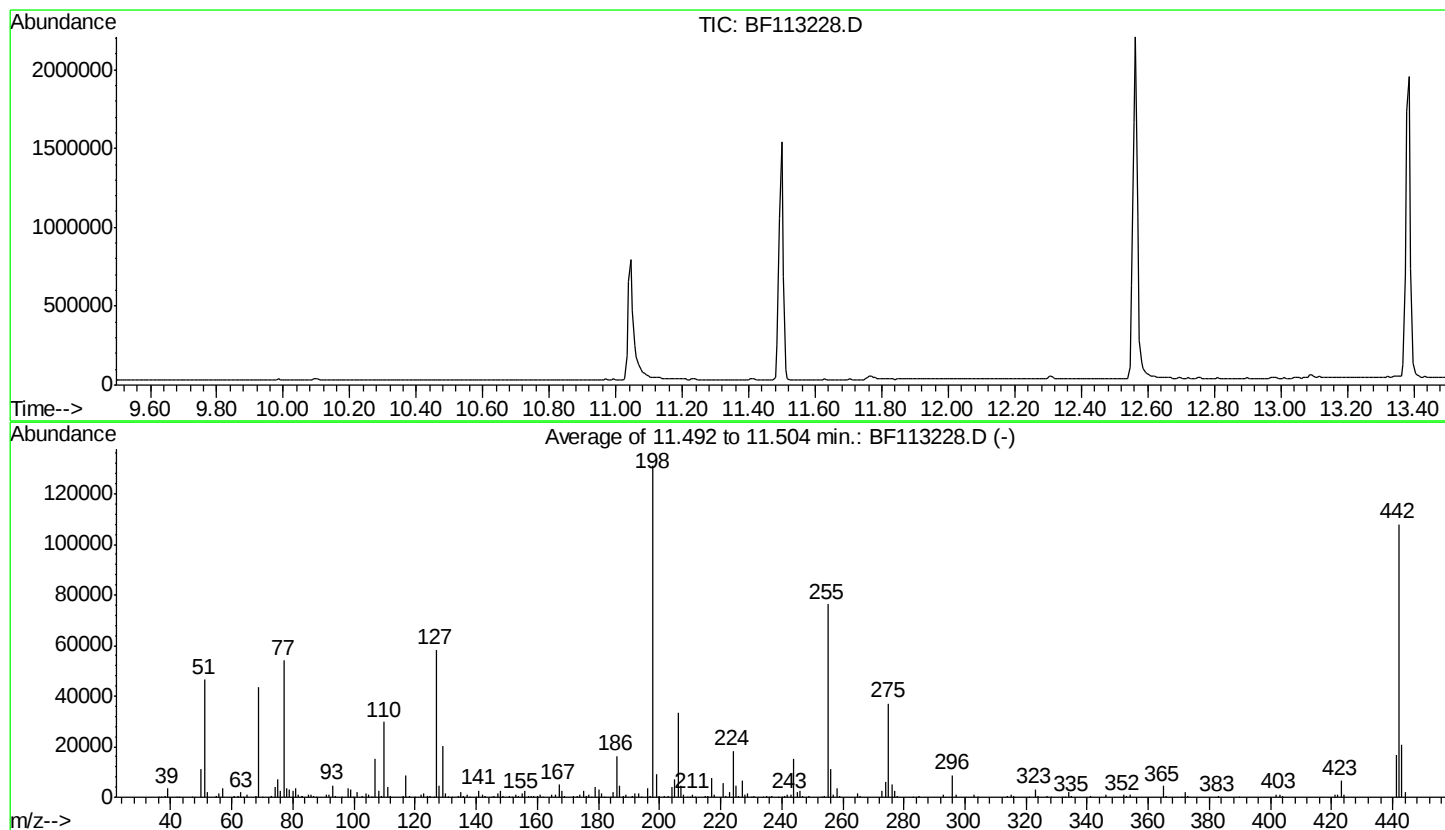

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	46355	PASS
68	69	0.00	2	1.7	722	PASS
69	198	0.00	100	33.1	43357	PASS
70	69	0.00	2	0.3	127	PASS
127	198	10	80	44.5	58341	PASS
197	198	0.00	2	0.2	319	PASS
198	198	100	100	100.0	131152	PASS
199	198	5	9	6.8	8949	PASS
275	198	10	60	28.2	36994	PASS
365	198	1	100	3.3	4360	PASS
441	198	0.01	100	12.7	16671	PASS
442	198	50	100	82.3	107904	PASS
443	442	15	24	19.2	20717	PASS