

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
 Data File : BF127472.D
 Acq On : 23 Mar 2022 11:06
 Operator : CG\JU
 Sample : PB143530BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143530BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.487	540	544	566	rBV	3177108	3294223	86.34%	13.967%
2	6.487	709	714	717	rBV	2915684	3295230	86.37%	13.971%
3	6.845	772	775	787	rBV	815067	659561	17.29%	2.796%
4	7.416	867	872	875	rBV	2141227	2286805	59.94%	9.696%
5	8.128	989	993	1008	rBV	965020	860192	22.55%	3.647%
6	9.204	1170	1176	1179	rBV	3695395	3815240	100.00%	16.176%
7	9.886	1287	1292	1295	rBV	1144124	996045	26.11%	4.223%
8	10.680	1423	1427	1430	rBV	2437166	2174167	56.99%	9.218%
9	11.375	1542	1545	1553	rBV	1175498	1027826	26.94%	4.358%
10	12.963	1810	1815	1818	rBV	3540871	3811293	99.90%	16.159%
11	14.021	1992	1995	2004	rBV	858295	762172	19.98%	3.231%
12	15.504	2240	2247	2262	rVB	403632	552304	14.48%	2.342%
13	17.104	2511	2519	2520	rBV2	30321	50862	1.33%	0.216%




Sum of corrected areas: 23585920

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
Data File : BF127472.D
Acq On : 23 Mar 2022 11:06
Operator : CG\JU
Sample : PB143530BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143530BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

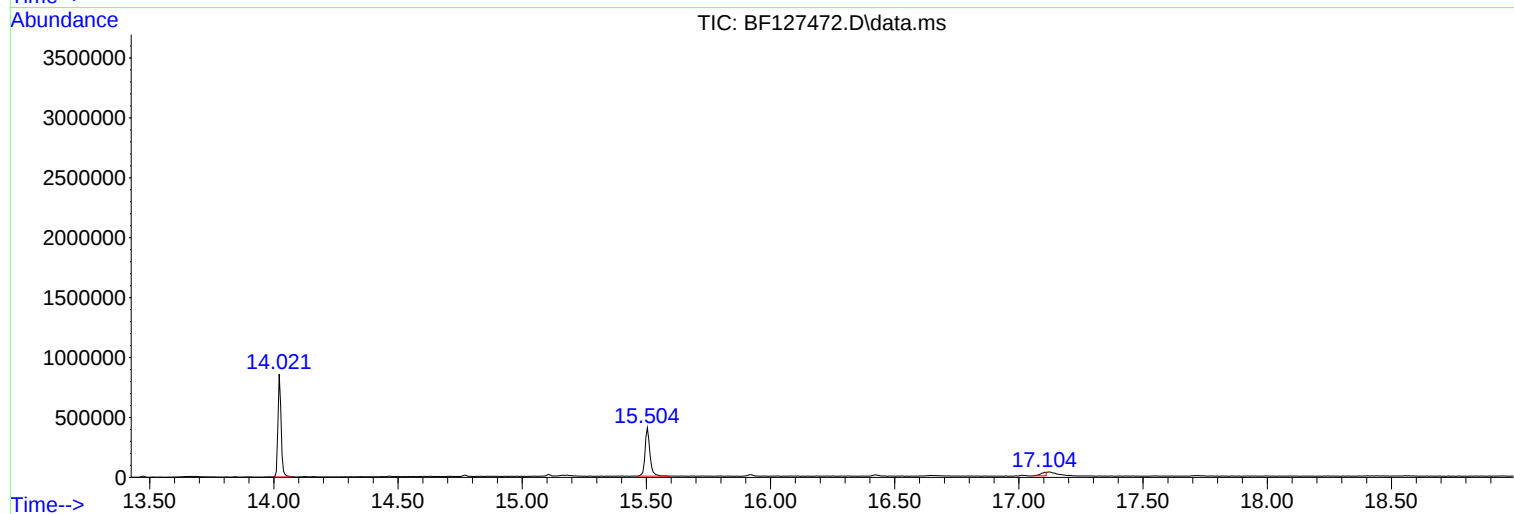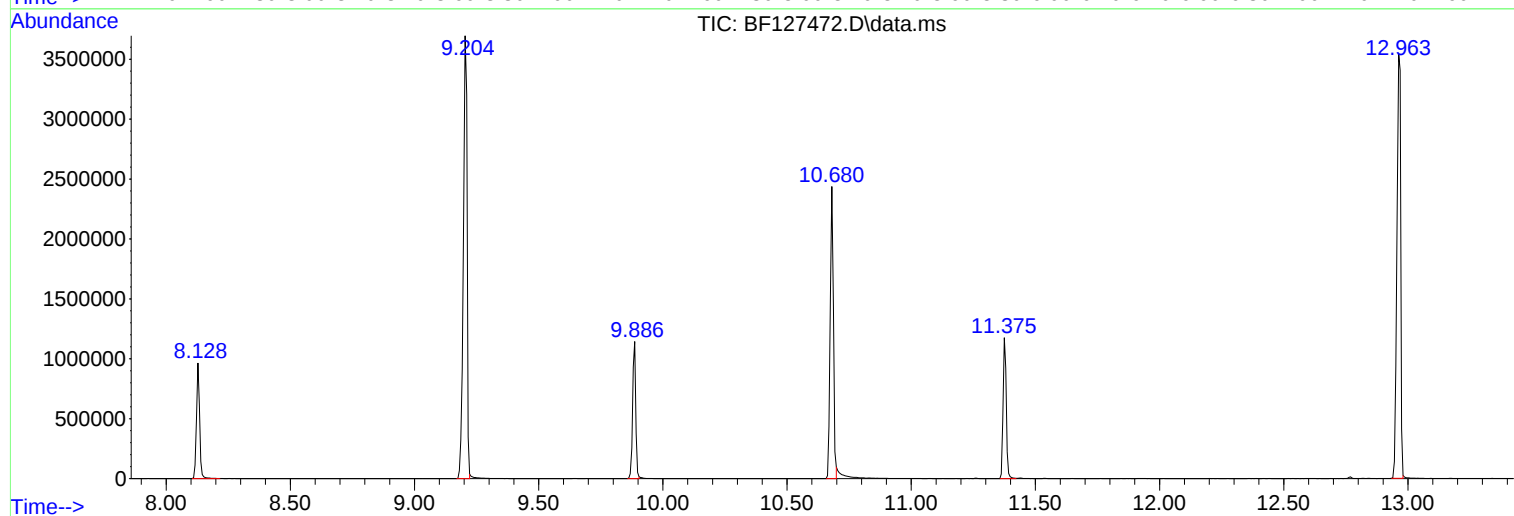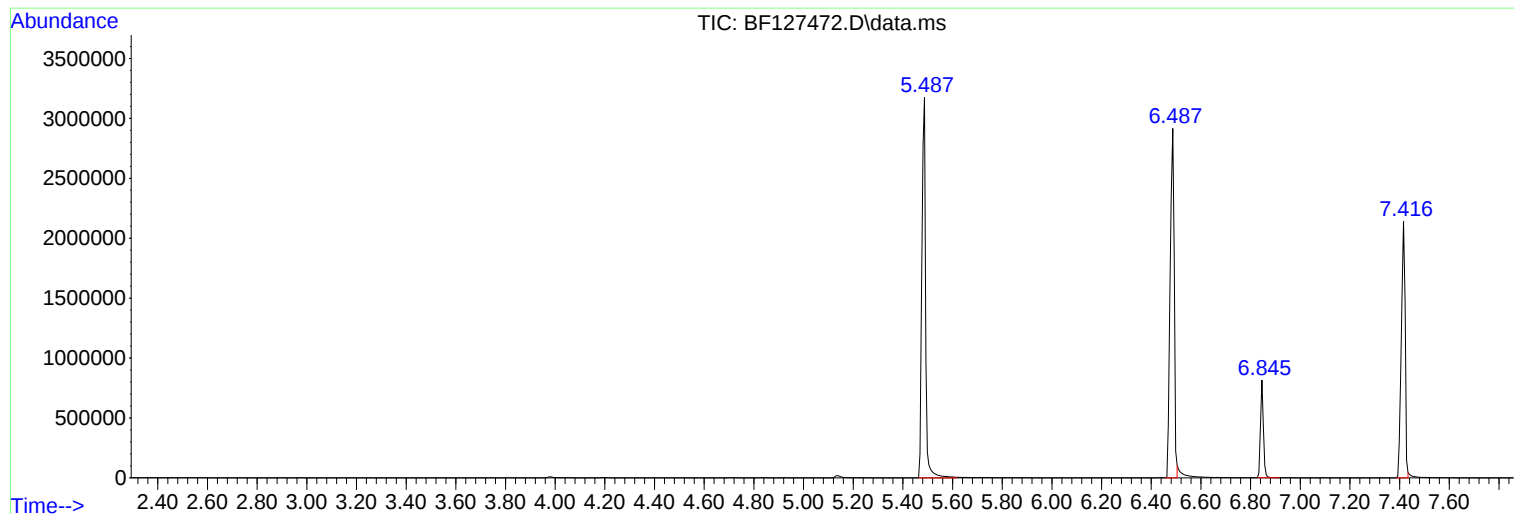

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
Data File : BF127472.D
Acq On : 23 Mar 2022 11:06
Operator : CG\JU
Sample : PB143530BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143530BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
Data File : BF127472.D
Acq On : 23 Mar 2022 11:06
Operator : CG\JU
Sample : PB143530BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143530BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------