

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
 Data File : BF127475.D
 Acq On : 23 Mar 2022 12:39
 Operator : CG\JU
 Sample : N2061-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EB-20220321

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127475.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.934	105	110	118	rBV2	24036	41942	1.31%	0.259%
2	5.075	471	474	483	rBV	30613	41172	1.28%	0.254%
3	5.469	538	541	565	rBV	1318309	1285714	40.03%	7.938%
4	6.481	710	713	731	rBV	739736	801630	24.96%	4.949%
5	6.845	772	775	783	rBV	675950	536885	16.71%	3.315%
6	7.416	867	872	875	rBV	2020401	1924449	59.91%	11.881%
7	8.128	989	993	1002	rBV	833919	687391	21.40%	4.244%
8	9.204	1171	1176	1179	rBV	3641676	3212235	100.00%	19.832%
9	9.886	1288	1292	1295	rBV	880902	783627	24.40%	4.838%
10	10.680	1423	1427	1430	rBV	2205761	1981270	61.68%	12.232%
11	11.375	1542	1545	1553	rBV	954445	788383	24.54%	4.867%
12	11.751	1606	1609	1614	rVB	60352	48406	1.51%	0.299%
13	12.963	1810	1815	1818	rBV	3329676	3013922	93.83%	18.608%
14	14.021	1992	1995	2007	rVB	590684	528129	16.44%	3.261%
15	15.504	2240	2247	2260	rBV	397048	522185	16.26%	3.224%




Sum of corrected areas: 16197340

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
Data File : BF127475.D
Acq On : 23 Mar 2022 12:39
Operator : CG\JU
Sample : N2061-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EB-20220321

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

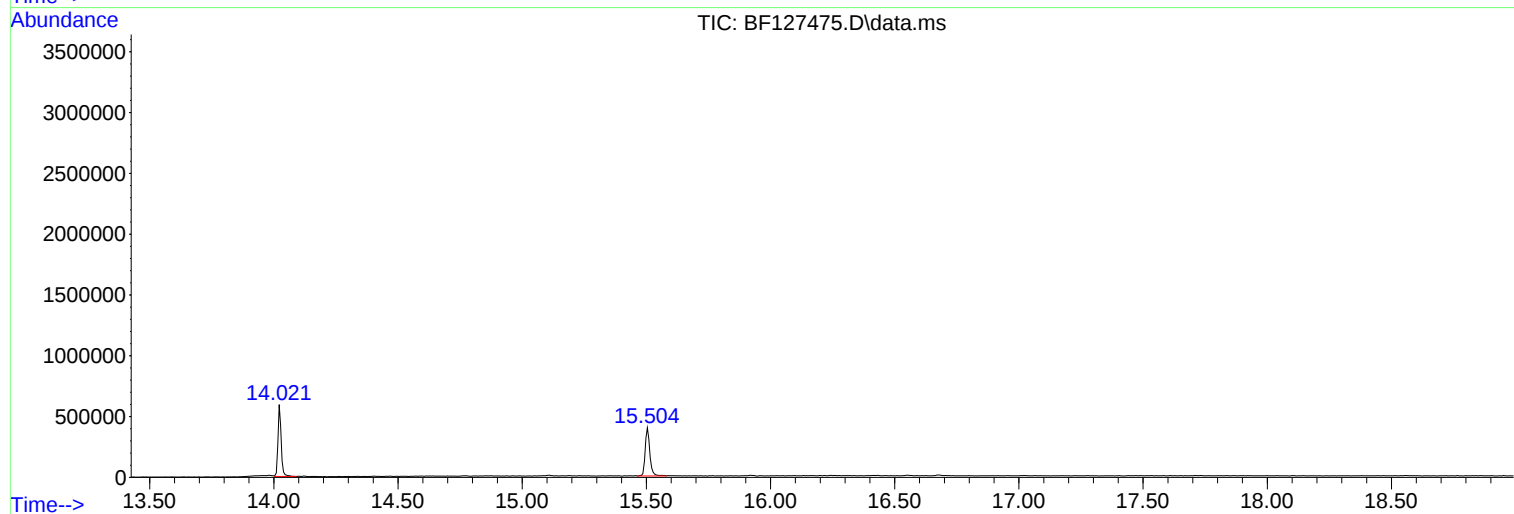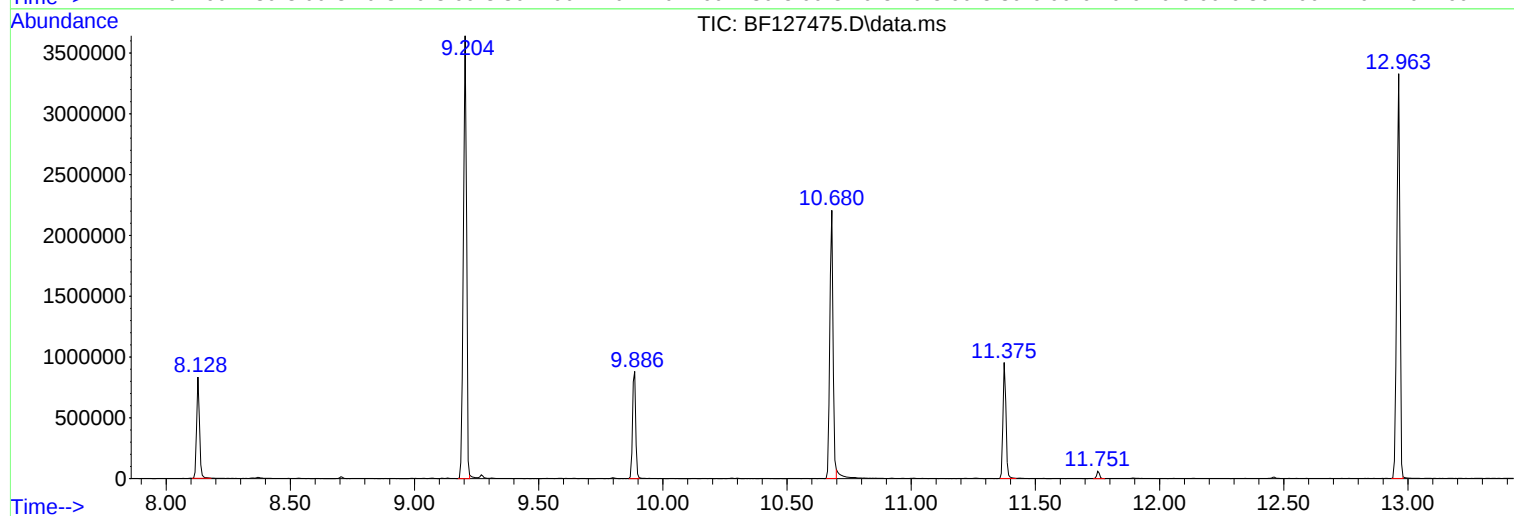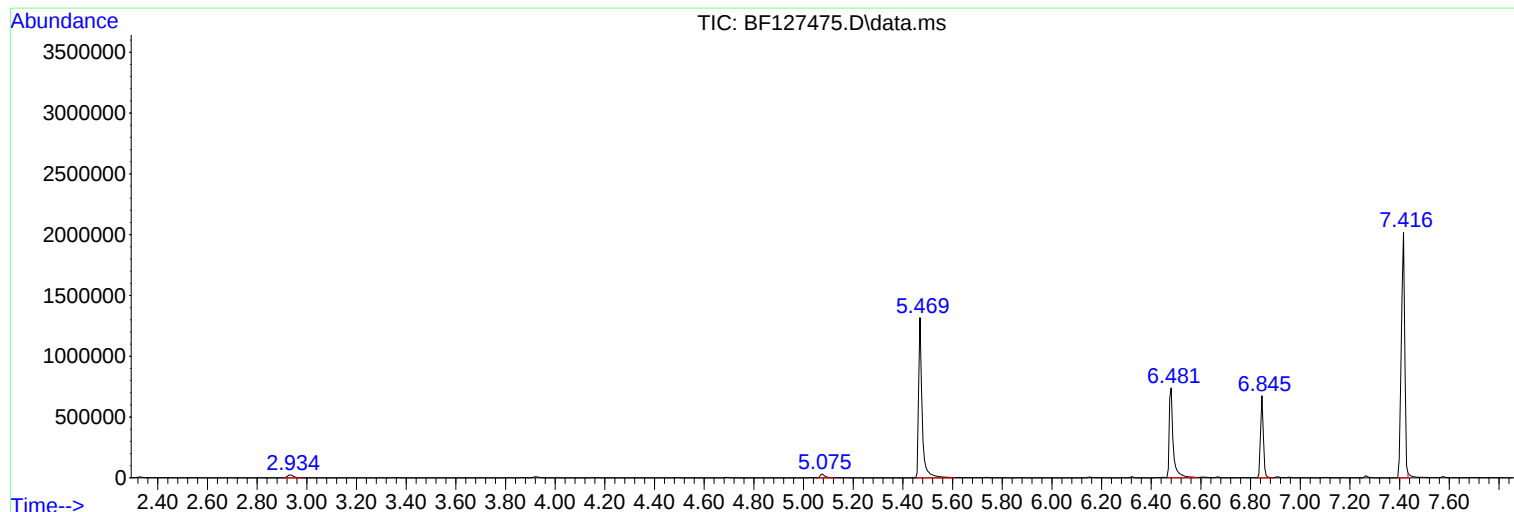

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
Data File : BF127475.D
Acq On : 23 Mar 2022 12:39
Operator : CG\JU
Sample : N2061-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EB-20220321

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
Data File : BF127475.D
Acq On : 23 Mar 2022 12:39
Operator : CG\JU
Sample : N2061-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EB-20220321

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------