

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
 Data File : BF127483.D
 Acq On : 23 Mar 2022 16:28
 Operator : CG\JU
 Sample : N2058-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MHA

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.899	100	104	119	rVB	265181	371068	9.85%	1.549%
2	4.669	401	405	414	rBV	384325	433390	11.51%	1.809%
3	5.098	474	478	499	rVB2	431738	605409	16.07%	2.528%
4	5.493	541	545	575	rBV	2865157	3110677	82.58%	12.987%
5	6.487	710	714	733	rBV	2649685	2996710	79.55%	12.511%
6	6.845	772	775	783	rBV	722067	585847	15.55%	2.446%
7	7.416	867	872	875	rBV	2296822	2295747	60.94%	9.585%
8	8.128	989	993	1009	rBV	903020	798693	21.20%	3.334%
9	9.204	1171	1176	1179	rBV	4015914	3766963	100.00%	15.727%
10	9.604	1241	1244	1250	rBV	51016	51716	1.37%	0.216%
11	9.886	1288	1292	1295	rBV	960371	886548	23.53%	3.701%
12	10.680	1423	1427	1448	rBV	2409521	2447858	64.98%	10.220%
13	11.374	1542	1545	1554	rBV	1097068	916294	24.32%	3.825%
14	12.963	1810	1815	1818	rBV	3716051	3589300	95.28%	14.985%
15	14.021	1992	1995	2007	rBV	597509	557223	14.79%	2.326%
16	15.504	2242	2247	2263	rVB	397430	539050	14.31%	2.250%




Sum of corrected areas: 23952493

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
Data File : BF127483.D
Acq On : 23 Mar 2022 16:28
Operator : CG\JU
Sample : N2058-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MHA

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

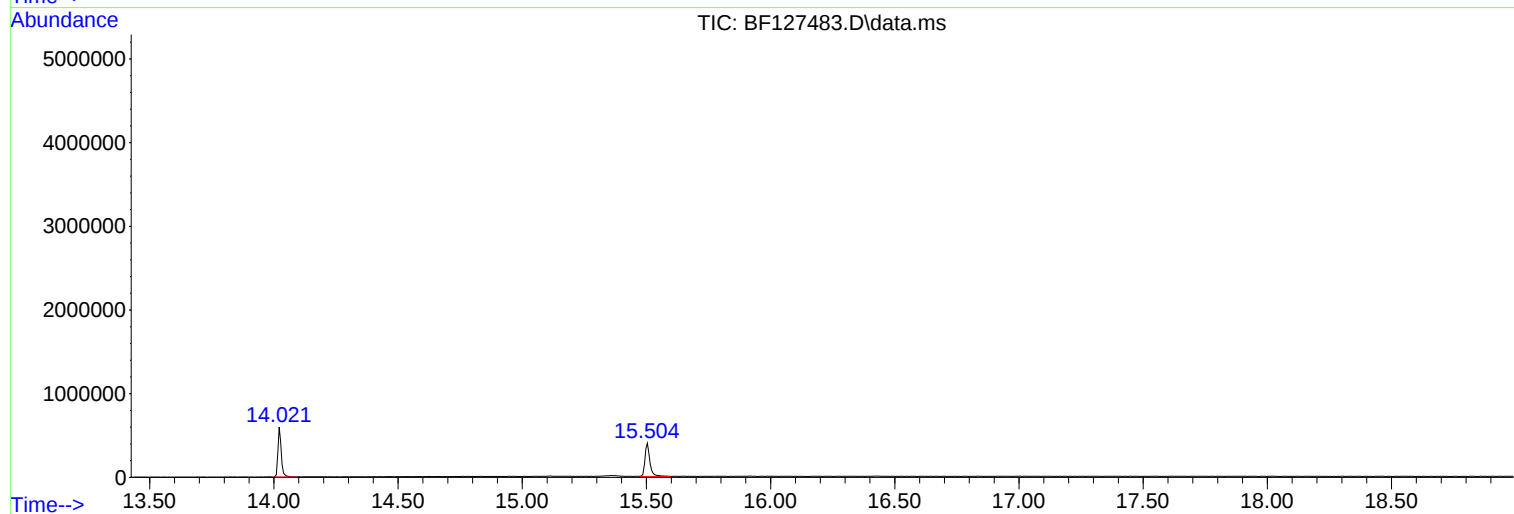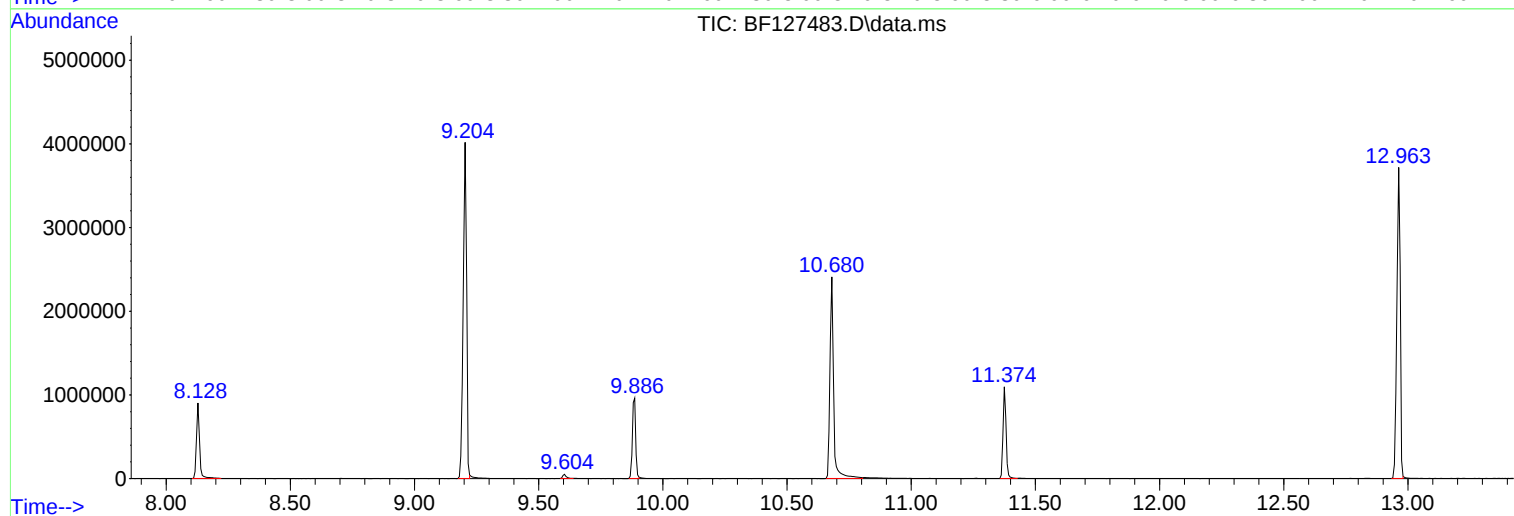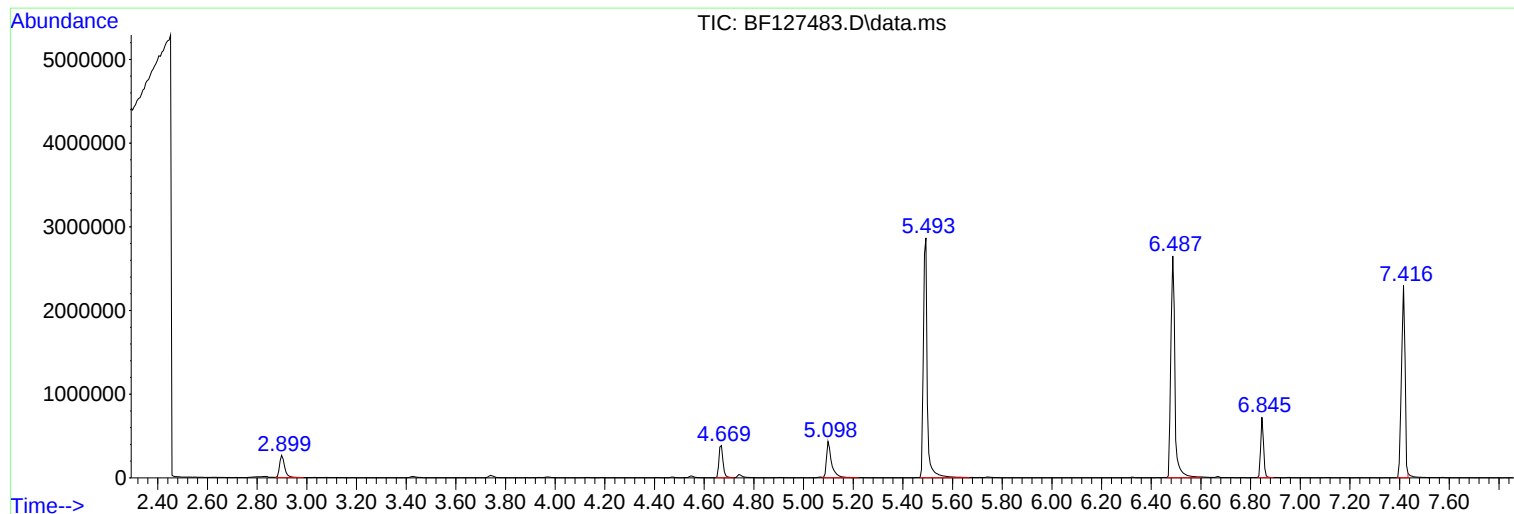

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
Data File : BF127483.D
Acq On : 23 Mar 2022 16:28
Operator : CG\JU
Sample : N2058-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MHA

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
Data File : BF127483.D
Acq On : 23 Mar 2022 16:28
Operator : CG\JU
Sample : N2058-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MHA

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------