

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
 Data File : BF127487.D
 Acq On : 23 Mar 2022 18:22
 Operator : CG\JU
 Sample : N2063-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-9-(10-10.5)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.087	473	476	489	rVB	23379	36217	1.51%	0.231%
2	5.469	538	541	558	rBV	2010393	2003863	83.36%	12.802%
3	6.481	709	713	732	rBV	2185767	2185126	90.90%	13.960%
4	6.845	772	775	785	rBV	668335	560570	23.32%	3.581%
5	7.410	867	871	883	rBV	1433013	1476538	61.42%	9.433%
6	8.127	989	993	1007	rBV	845078	724652	30.14%	4.630%
7	9.204	1171	1176	1179	rBV	2793748	2403977	100.00%	15.358%
8	9.886	1288	1292	1303	rVB	944503	837805	34.85%	5.352%
9	10.680	1423	1427	1439	rBV	1435112	1484464	61.75%	9.484%
10	11.374	1542	1545	1554	rBV	971239	845466	35.17%	5.401%
11	12.962	1810	1815	1818	rBV	2149098	1998238	83.12%	12.766%
12	13.927	1968	1979	1980	rBV7	15194	39961	1.66%	0.255%
13	14.021	1992	1995	2006	rVB	534307	519165	21.60%	3.317%
14	15.503	2243	2247	2259	rVB	391272	502557	20.91%	3.211%
15	17.280	2543	2549	2554	rVB6	17164	34055	1.42%	0.218%




Sum of corrected areas: 15652654

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
Data File : BF127487.D
Acq On : 23 Mar 2022 18:22
Operator : CG\JU
Sample : N2063-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-9-(10-10.5)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

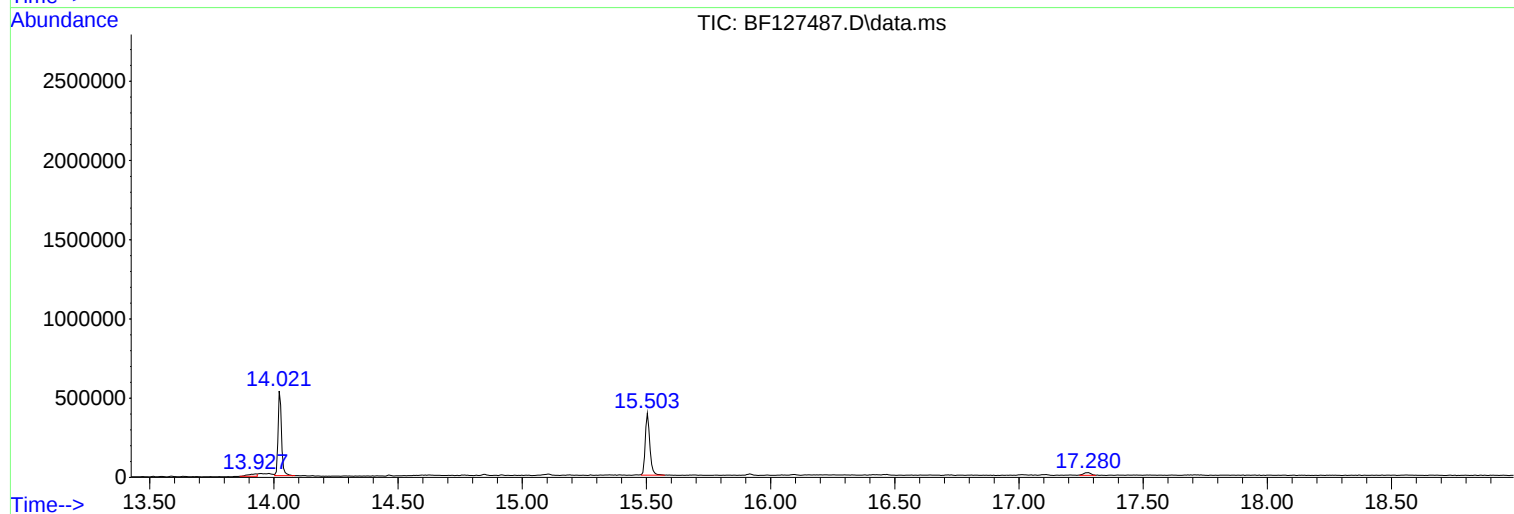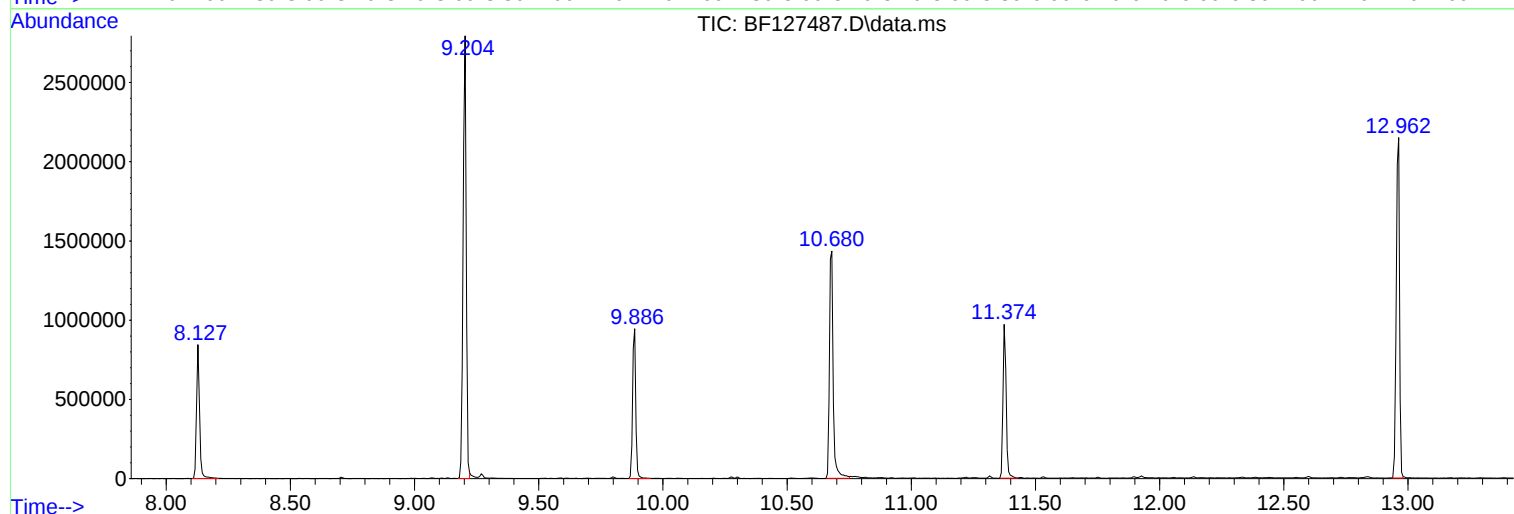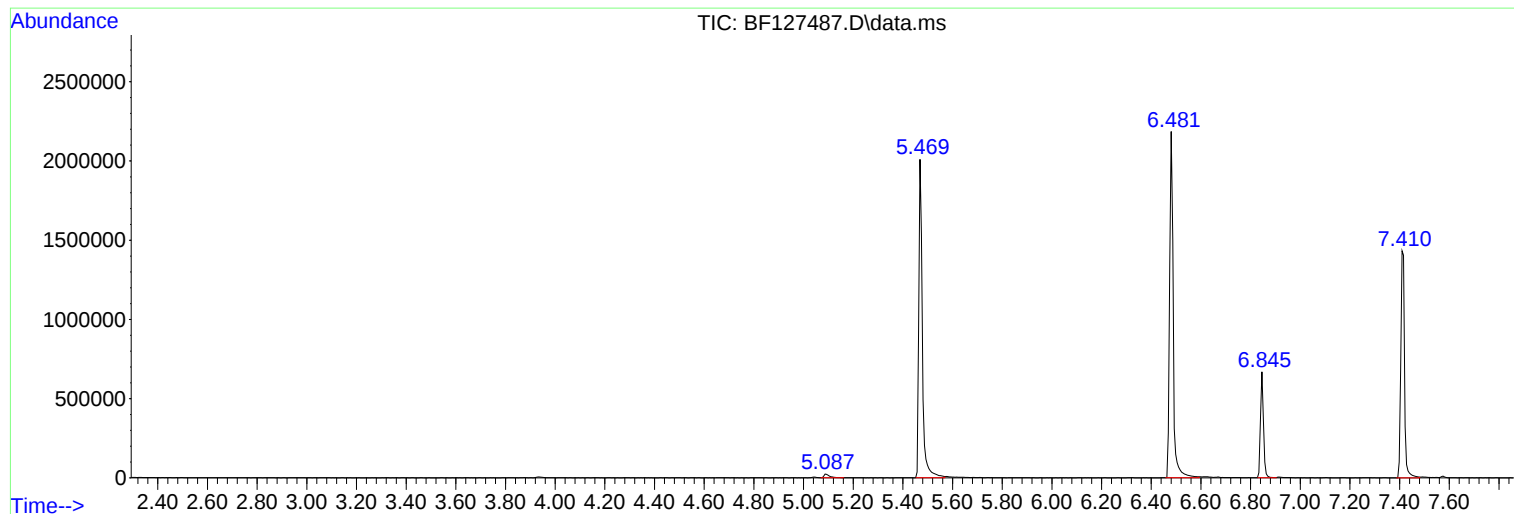

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
Data File : BF127487.D
Acq On : 23 Mar 2022 18:22
Operator : CG\JU
Sample : N2063-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-9-(10-10.5)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
Data File : BF127487.D
Acq On : 23 Mar 2022 18:22
Operator : CG\JU
Sample : N2063-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-9-(10-10.5)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------