

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
 Data File : BF127489.D
 Acq On : 23 Mar 2022 19:19
 Operator : CG\JU
 Sample : N2063-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-4-2-(10-10.5)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127489.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.098	475	478	489	rBV2	17394	25700	1.12%	0.165%
2	5.475	538	542	569	rBV	2213757	2155833	93.62%	13.843%
3	6.481	709	713	732	rBV	2252254	2261791	98.23%	14.524%
4	6.845	772	775	784	rBV	660272	544176	23.63%	3.494%
5	7.410	867	871	884	rBV	1482772	1481934	64.36%	9.516%
6	8.128	989	993	1012	rVB	846966	714369	31.02%	4.587%
7	9.204	1171	1176	1179	rBV	2660527	2302644	100.00%	14.786%
8	9.269	1184	1187	1192	rVB	43263	38728	1.68%	0.249%
9	9.886	1288	1292	1304	rVB	877942	817683	35.51%	5.251%
10	10.675	1423	1426	1439	rBV	1427498	1441348	62.60%	9.255%
11	11.375	1542	1545	1549	rBV	963855	816749	35.47%	5.245%
12	12.598	1749	1753	1757	rVB	45367	45465	1.97%	0.292%
13	12.827	1787	1792	1798	rVB	39470	55011	2.39%	0.353%
14	12.957	1810	1814	1818	rBV	2086222	1857767	80.68%	11.929%
15	14.021	1991	1995	2006	rVB	536618	514674	22.35%	3.305%
16	15.504	2242	2247	2259	rVB	390473	499440	21.69%	3.207%




Sum of corrected areas: 15573312

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
Data File : BF127489.D
Acq On : 23 Mar 2022 19:19
Operator : CG\JU
Sample : N2063-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-4-2-(10-10.5)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

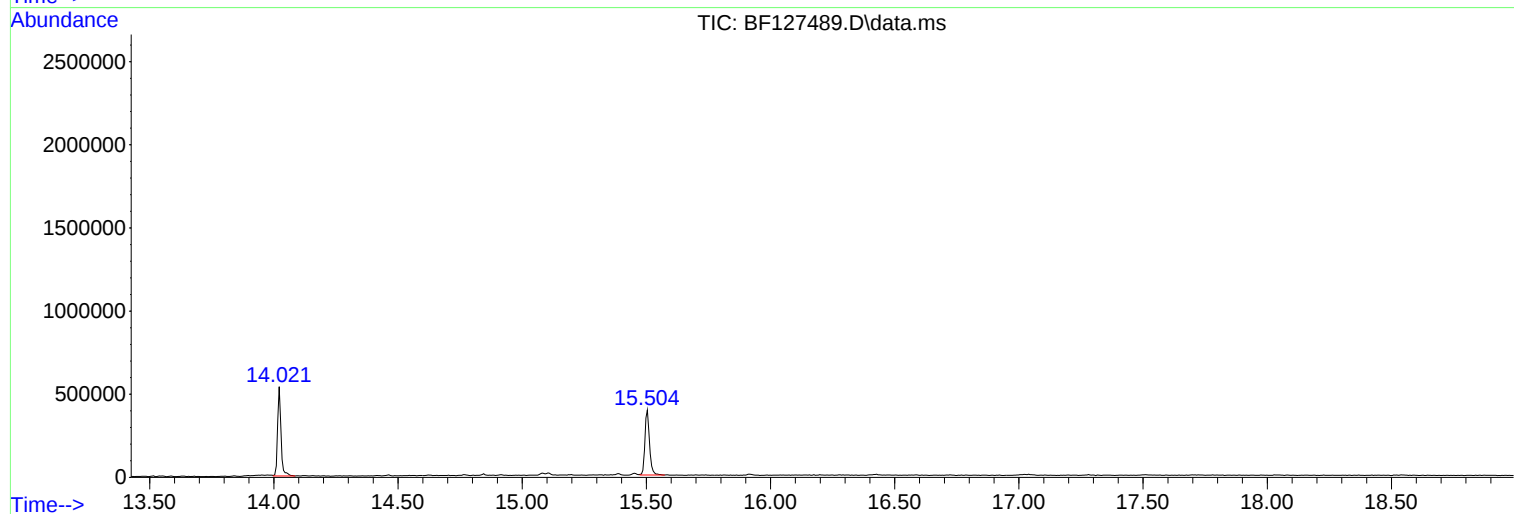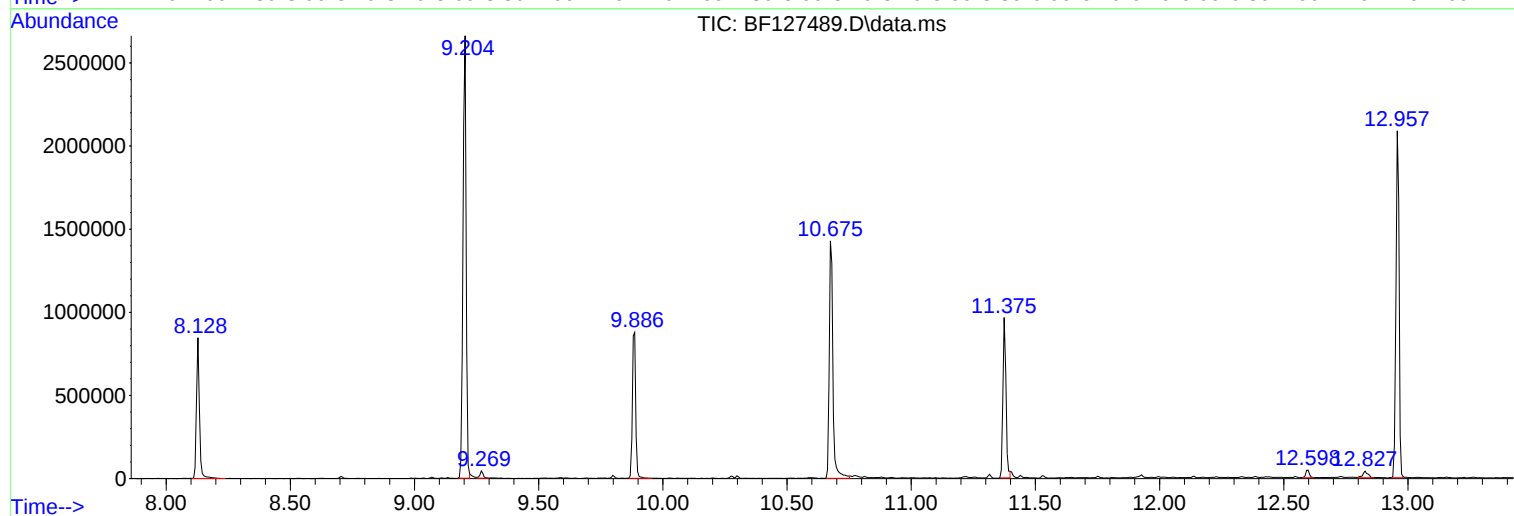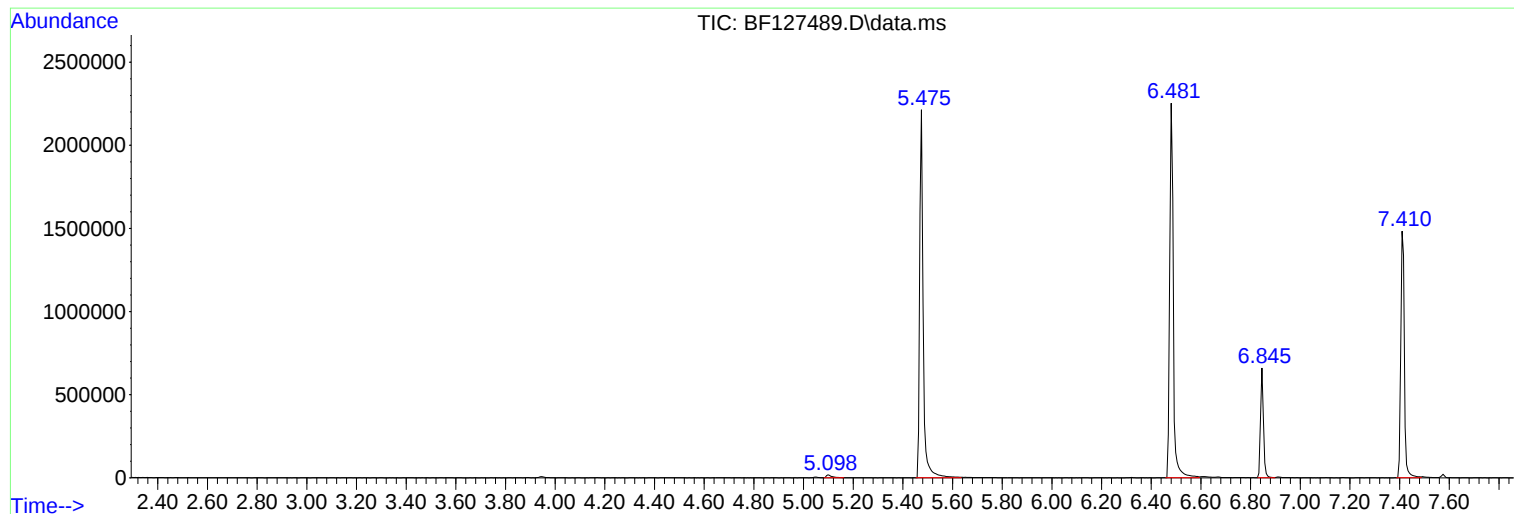

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
Data File : BF127489.D
Acq On : 23 Mar 2022 19:19
Operator : CG\JU
Sample : N2063-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-4-2-(10-10.5)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032322\
Data File : BF127489.D
Acq On : 23 Mar 2022 19:19
Operator : CG\JU
Sample : N2063-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-4-2-(10-10.5)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------