
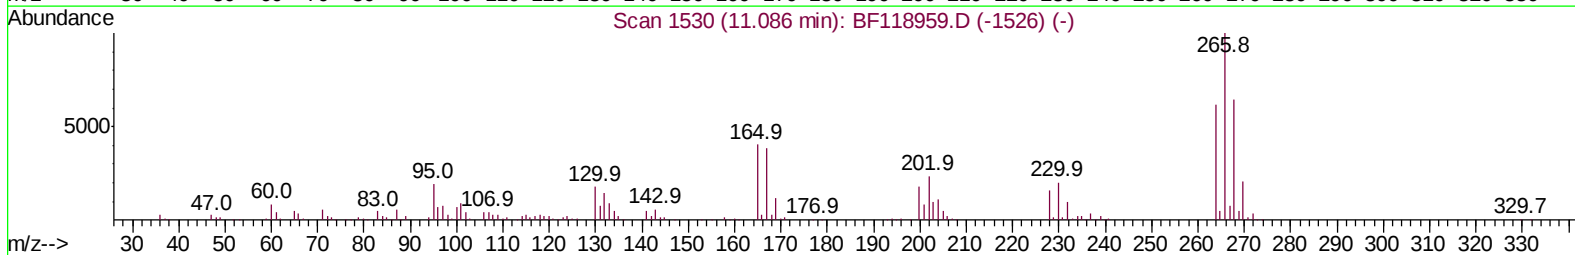
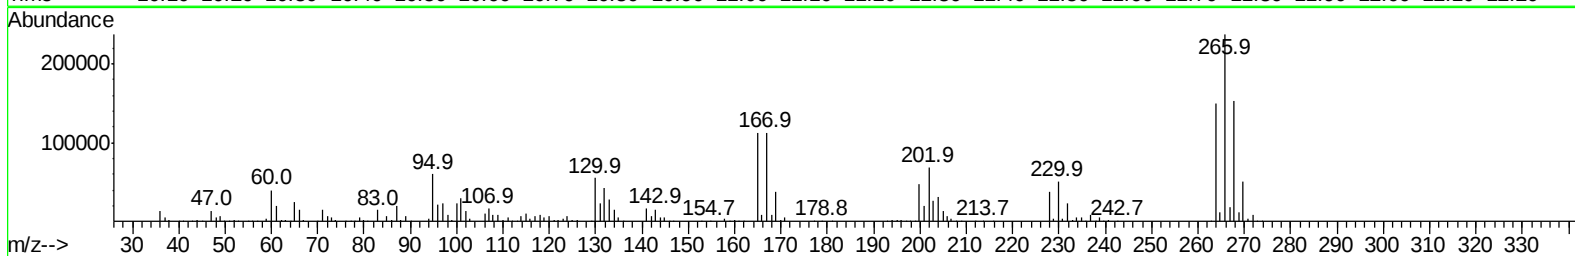


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF032420\
Data File : BF119482.D
Acq On : 24 Mar 2020 8:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 09:07:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 06 23:38:46 2020
Response via : Initial Calibration

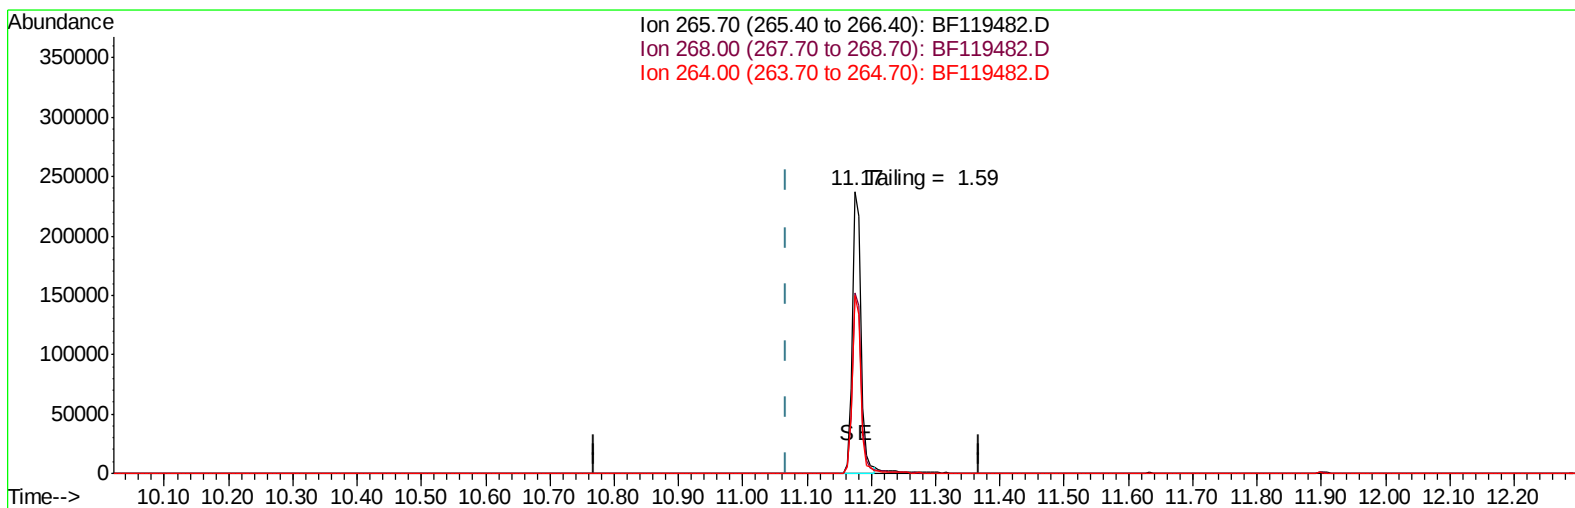

TIC: BF119482.D

(70) Pentachlorophenol (C)




11.174min (+0.106) 320003.17ng

response 225349

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	64.26
264.00	63.70	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF032420\
Data File : BF119482.D
Acq On : 24 Mar 2020 8:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 09:07:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 06 23:38:46 2020
Response via : Initial Calibration

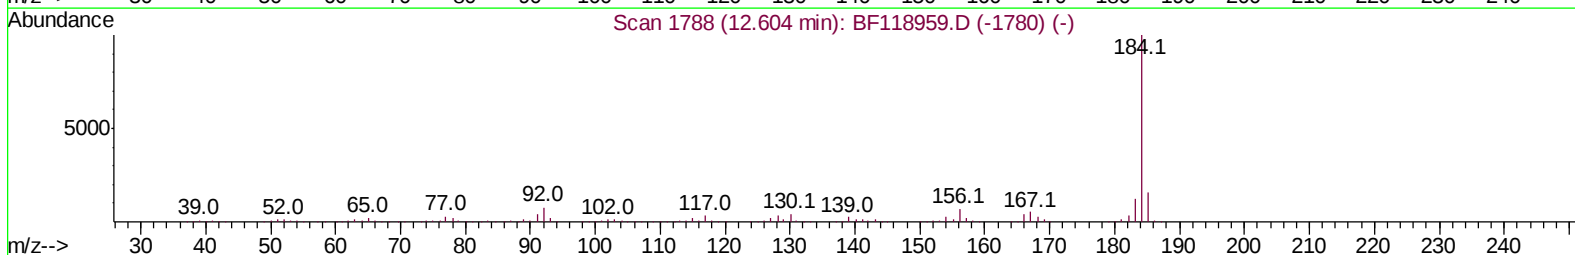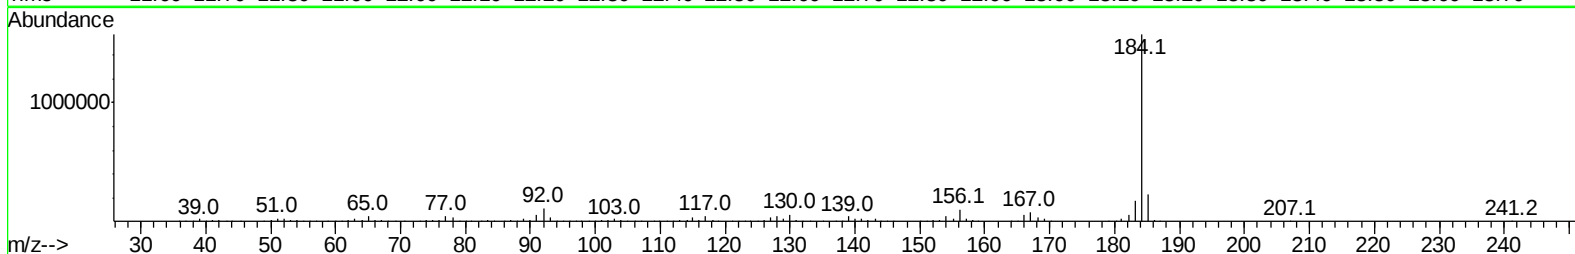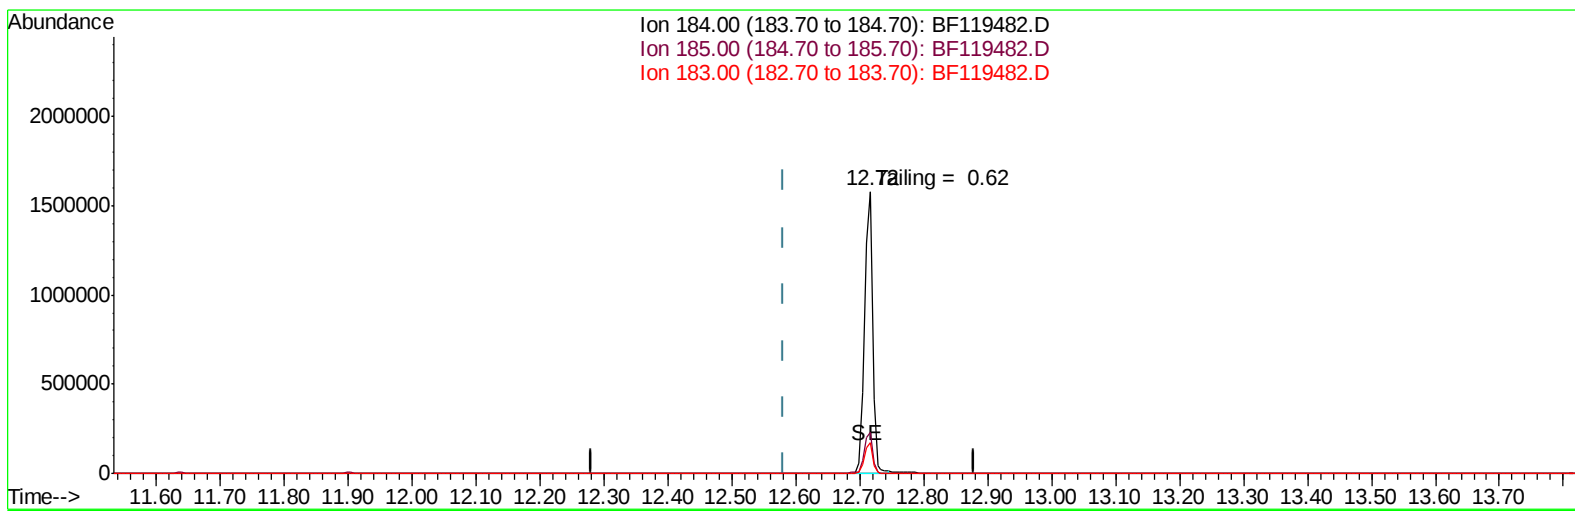

TIC: BF119482.D

(77) Benzidine

12.715min (+0.135) 0.00ng

response 1392494

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.63
183.00	12.40	10.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF032420\
 Data File : BF119482.D
 Acq On : 24 Mar 2020 8:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 09:07:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 06 23:38:46 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ng	-6.72
21) Naphthalene-d8	0.00	136	0	0.00	ng	-8.01
39) Acenaphthene-d10	0.00	164	0	0.00	ng	-9.76
64) Phenanthrene-d10	11.22	188	116	20.00	ng	-0.02
76) Chrysene-d12	0.00	240	0	0.00	ng	-13.89
87) Perylene-d12	0.00	264	0	0.00	ng	-15.31

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	0.00	112	0	0.00	ng	
7) Phenol-d6	0.00	99	0	0.00	ng	
23) Nitrobenzene-d5	0.00	82	0	0.00	ng	
42) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng	
45) 2-Fluorobiphenyl	0.00	172	0	0.00	ng	
79) Terphenyl-d14	12.95	244	2492	0.00	ng	0.12

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
66) n-Nitrosodiphenylamine	10.52	169	110	28.961	ng	# 24
69) Atrazine	11.17	200	40095	30213.071	ng	# 36
70) Pentachlorophenol	11.17	266	225349	320003.168	ng	# 99
71) Phenanthrene	11.25	178	889	140.529	ng	# 36
72) Anthracene	11.32	178	2221	351.379	ng	# 59
73) Carbazole	11.64	167	8964	1591.888	ng	# 79
74) Di-n-butylphthalate	11.90	149	277	40.620	ng	# 77
75) Fluoranthene	12.57	202	2397	356.965	ng	# 64

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF032420\
Data File : BF119482.D
Acq On : 24 Mar 2020 8:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 09:07:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 06 23:38:46 2020
Response via : Initial Calibration

