

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032420\  
 Data File : BF119485.D  
 Acq On : 24 Mar 2020 11:37  
 Operator : CG/JU  
 Sample : PB127731BL  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB127731BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0  
 Filtering: 5  
 Min Area: 3 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF031820.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.087       | 505           | 510         | 516          | rVB      | 98540          | 131040        | 1.07%           | 0.168%        |
| 2         | 5.463       | 568           | 574         | 577          | rBV      | 8624083        | 9349250       | 76.64%          | 12.003%       |
| 3         | 6.469       | 738           | 745         | 748          | rBV      | 8002944        | 9035839       | 74.07%          | 11.601%       |
| 4         | 6.845       | 805           | 809         | 812          | rVB      | 1965615        | 1773315       | 14.54%          | 2.277%        |
| 5         | 6.998       | 831           | 835         | 839          | rBV      | 7254267        | 7372833       | 60.44%          | 9.466%        |
| 6         | 7.404       | 898           | 904         | 907          | rBV      | 5466237        | 6108883       | 50.08%          | 7.843%        |
| 7         | 8.128       | 1022          | 1027        | 1030         | rBV      | 2509108        | 2330125       | 19.10%          | 2.992%        |
| 8         | 9.210       | 1205          | 1211        | 1214         | rBV      | 10433848       | 10877927      | 89.17%          | 13.966%       |
| 9         | 9.886       | 1321          | 1326        | 1329         | rBV      | 3151343        | 2650150       | 21.72%          | 3.402%        |
| 10        | 10.680      | 1454          | 1461        | 1464         | rBV      | 6780443        | 7217489       | 59.17%          | 9.266%        |
| 11        | 11.374      | 1575          | 1579        | 1582         | rBV      | 3578782        | 2916752       | 23.91%          | 3.745%        |
| 12        | 12.974      | 1845          | 1851        | 1854         | rBV      | 10749248       | 12198649      | 100.00%         | 15.661%       |
| 13        | 14.015      | 2024          | 2028        | 2032         | rBV      | 3262460        | 2938003       | 24.08%          | 3.772%        |
| 14        | 15.486      | 2272          | 2278        | 2283         | rBV      | 2443424        | 2990675       | 24.52%          | 3.840%        |


Sum of corrected areas: 77890930

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032420\  
Data File : BF119485.D  
Acq On : 24 Mar 2020 11:37  
Operator : CG/JU  
Sample : PB127731BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB127731BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031820.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

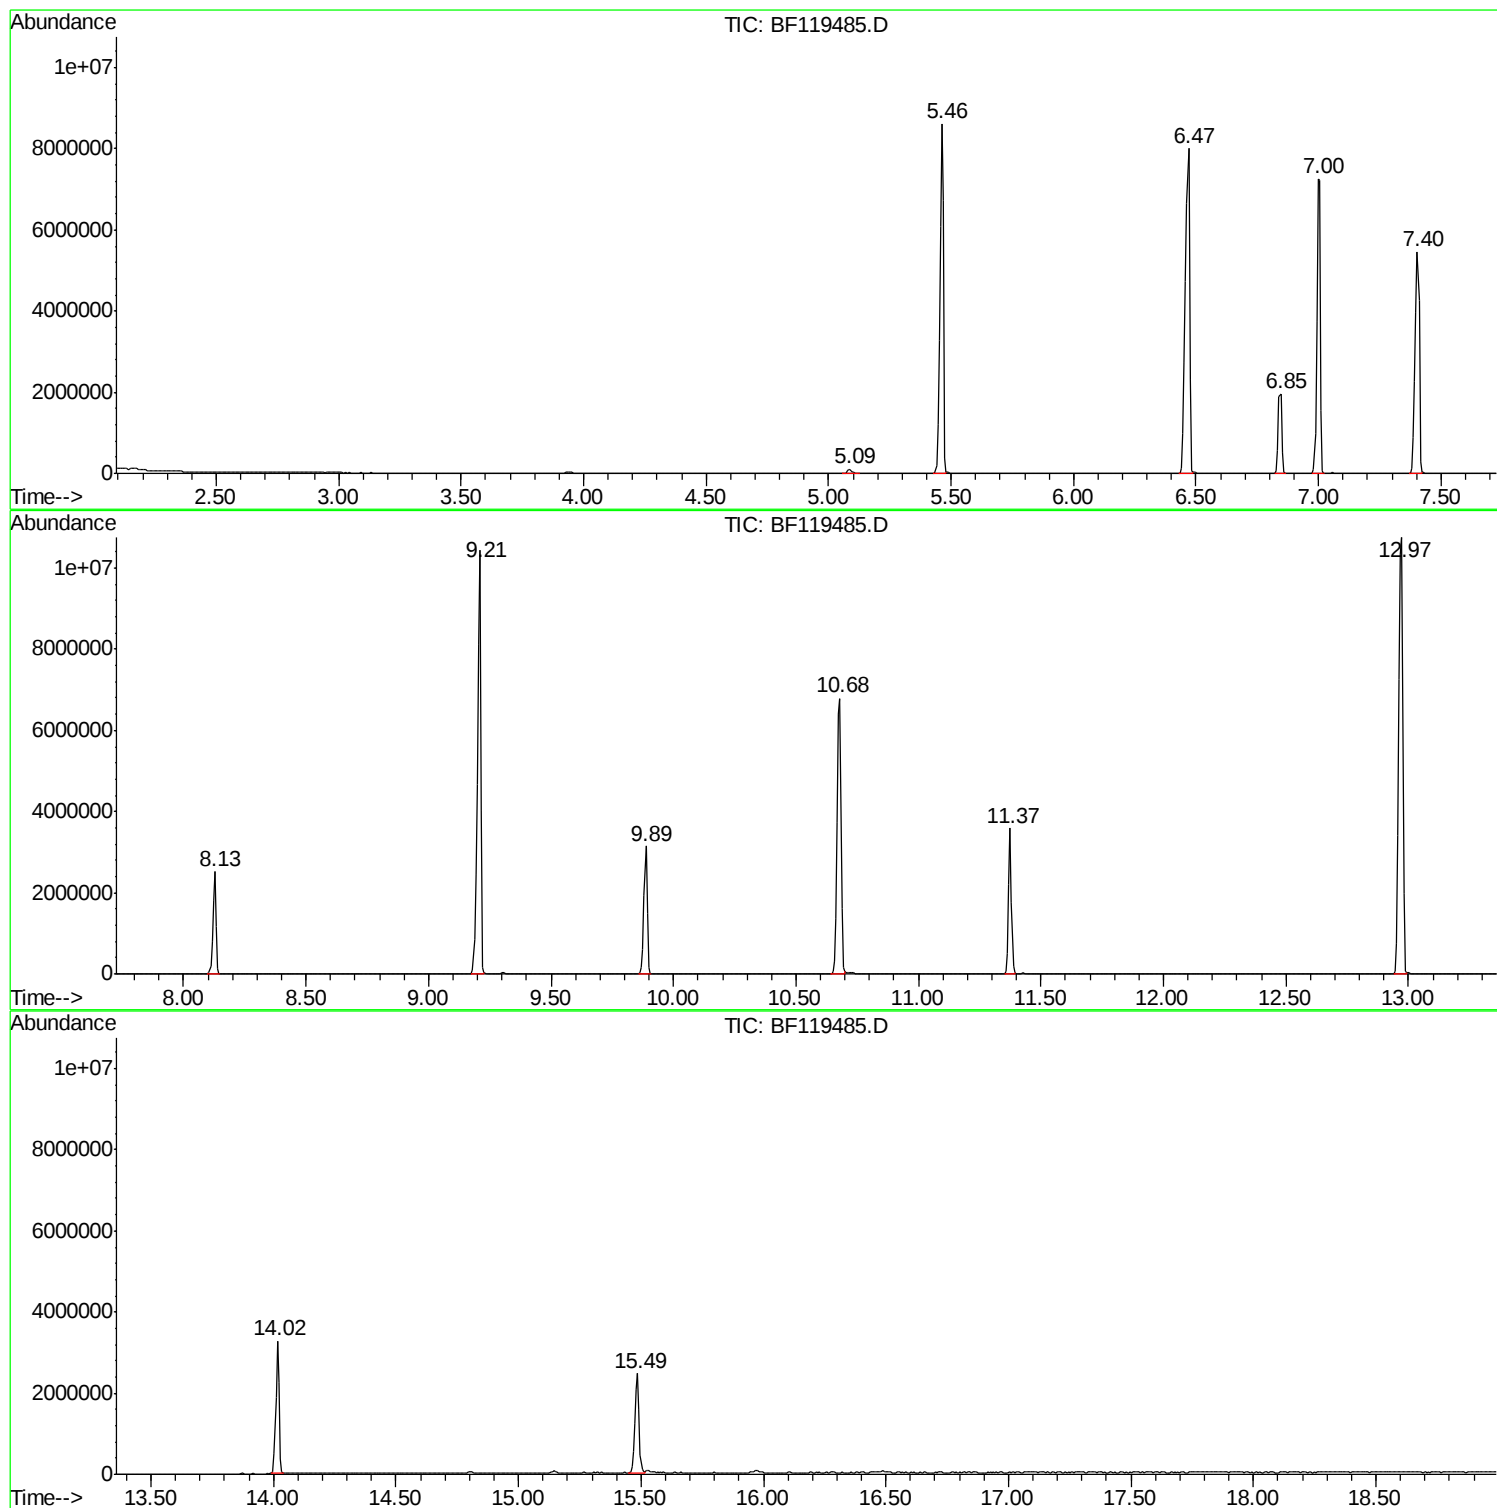

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF032420\  
Data File : BF119485.D  
Acq On : 24 Mar 2020 11:37  
Operator : CG/JU  
Sample : PB127731BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB127731BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF031820.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF032420\  
Data File : BF119485.D  
Acq On : 24 Mar 2020 11:37  
Operator : CG/JU  
Sample : PB127731BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB127731BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF031820.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |