


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF032420\  
 Data File : BF119482.D  
 Acq On : 24 Mar 2020 8:17  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF031820.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Mar 18 15:11:18 2020

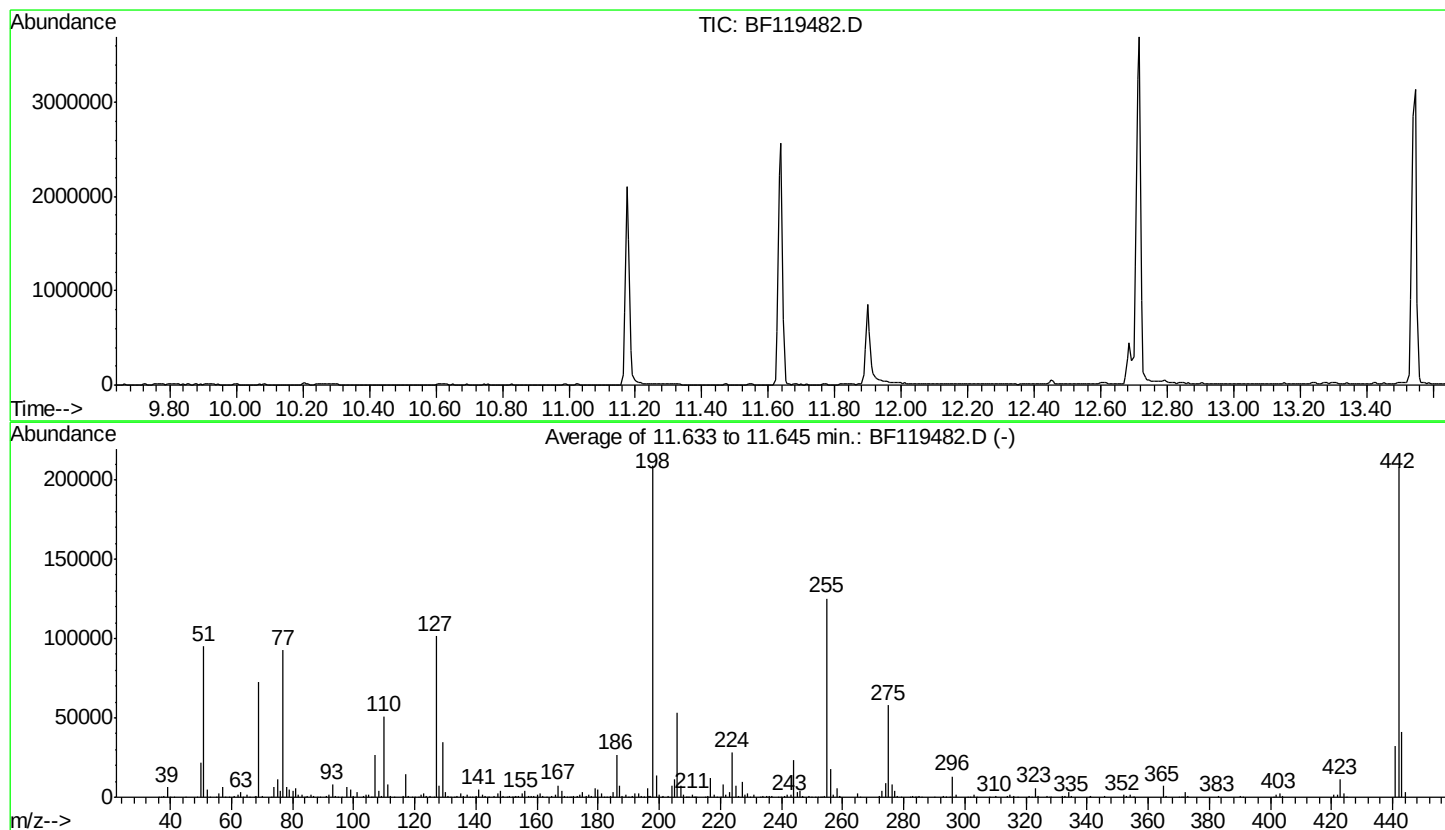

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 45.4      | 94882   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.6       | 1176    | PASS             |
| 69          | 198          | 0.00         | 100          | 34.8      | 72628   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 436     | PASS             |
| 127         | 198          | 10           | 80           | 48.6      | 101509  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.4       | 834     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 208842  | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 13950   | PASS             |
| 275         | 198          | 10           | 60           | 27.7      | 57906   | PASS             |
| 365         | 198          | 1            | 100          | 3.4       | 7075    | PASS             |
| 441         | 198          | 0.01         | 100          | 15.6      | 32666   | PASS             |
| 442         | 198          | 50           | 100          | 99.7      | 208128  | PASS             |
| 443         | 442          | 15           | 24           | 19.9      | 41373   | PASS             |