


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032519\
Data File : BF113272.D
Acq On : 25 Mar 2019 11:10
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 26 03:32:08 2019

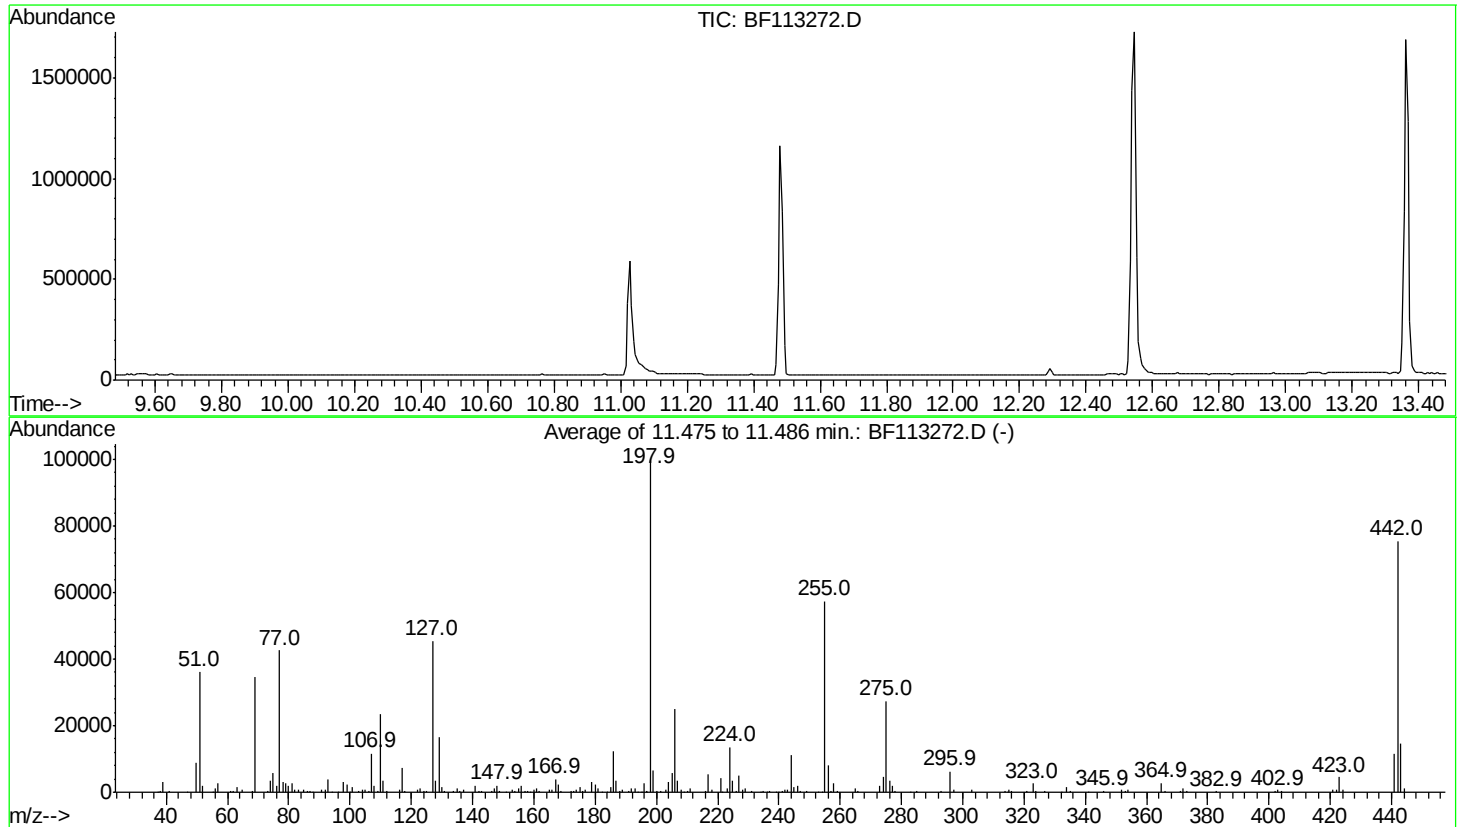

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	36309	PASS
68	69	0.00	2	1.6	546	PASS
69	198	0.00	100	34.8	34690	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.6	45477	PASS
197	198	0.00	2	0.5	509	PASS
198	198	100	100	100.0	99632	PASS
199	198	5	9	6.5	6449	PASS
275	198	10	60	27.5	27354	PASS
365	198	1	100	2.8	2786	PASS
441	198	0.01	100	11.7	11647	PASS
442	198	50	100	75.9	75581	PASS
443	442	15	24	19.5	14723	PASS