

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032522\
 Data File : BF127524.D
 Acq On : 25 Mar 2022 13:05
 Operator : CG\JU
 Sample : N2064-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20220281-FIELD-BLANK

Quant Time: Mar 25 17:26:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 22 02:16:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.845	152	95344	20.000	ng	0.00
21) Naphthalene-d8	8.128	136	353426	20.000	ng	0.00
39) Acenaphthene-d10	9.886	164	210995	20.000	ng	0.00
64) Phenanthrene-d10	11.380	188	389784	20.000	ng	0.00
76) Chrysene-d12	14.027	240	300382	20.000	ng	0.00
86) Perylene-d12	15.510	264	217474	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.475	112	427196	71.520	ng	0.00
7) Phenol-d6	6.481	99	379747	46.510	ng	0.00
23) Nitrobenzene-d5	7.416	82	750620	90.785	ng	0.00
42) 2,4,6-Tribromophenol	10.686	330	299167	133.103	ng	0.00
45) 2-Fluorobiphenyl	9.204	172	1236228	85.556	ng	0.00
79) Terphenyl-d14	12.969	244	1613413	87.928	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032522\
Data File : BF127524.D
Acq On : 25 Mar 2022 13:05
Operator : CG\JU
Sample : N2064-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20220281-FIELD-BLANK

Quant Time: Mar 25 17:26:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 22 02:16:33 2022
Response via : Initial Calibration




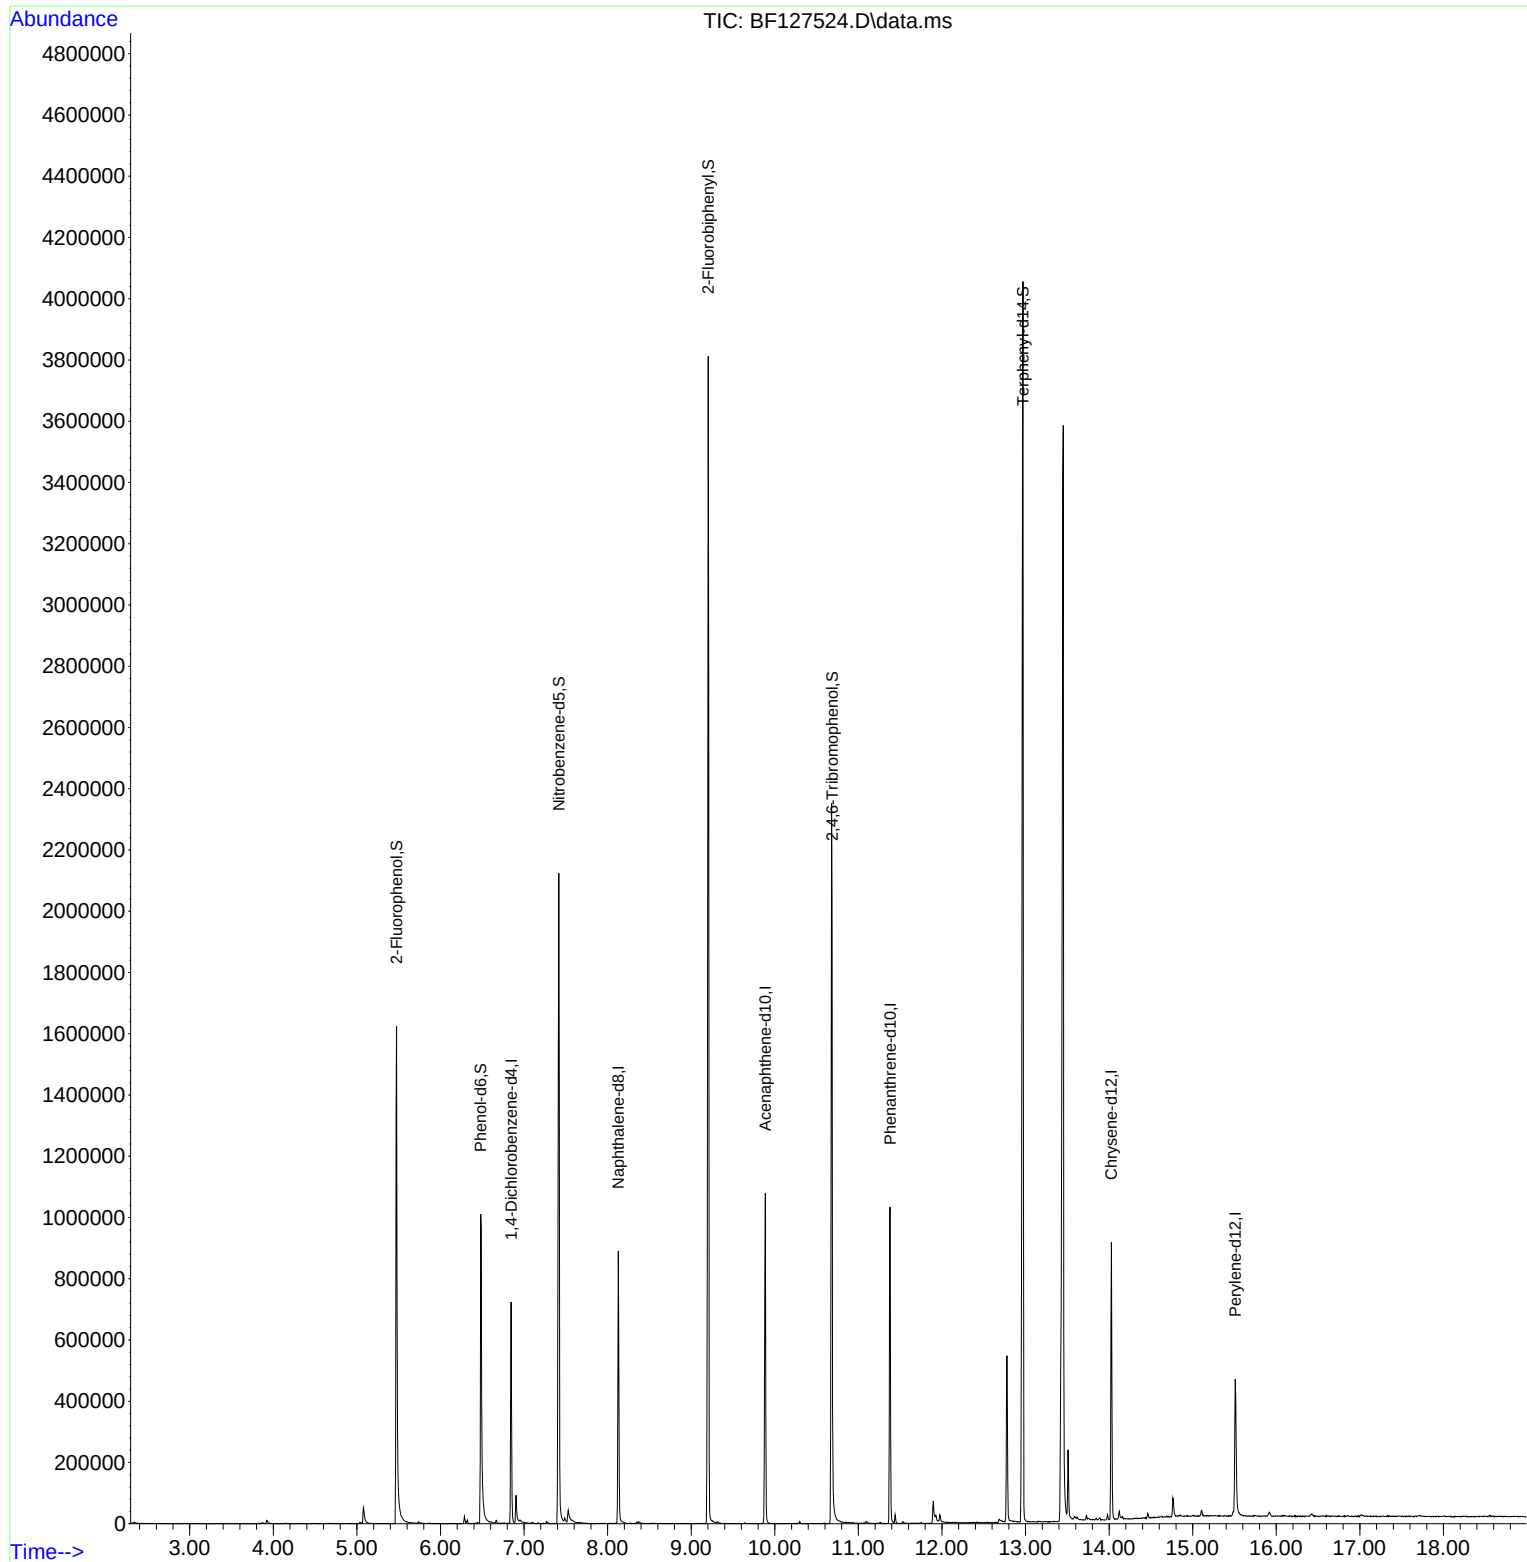


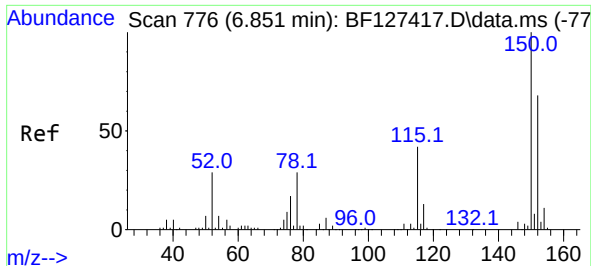

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.845 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF127524.D
Acq: 25 Mar 2022 13:05




Instrument :
BNA_F
ClientSampleId :
20220281-FIELD-BLANK


Tgt Ion:152 Resp: 95344
Ion Ratio Lower Upper
152 100
150 144.9 117.2 175.8
115 62.8 49.8 74.6

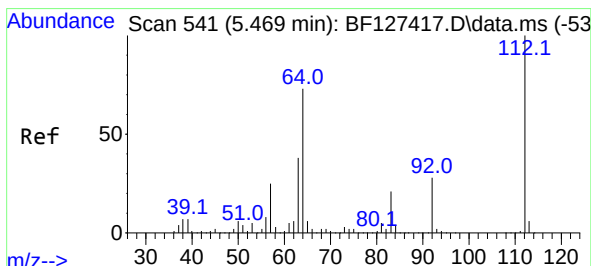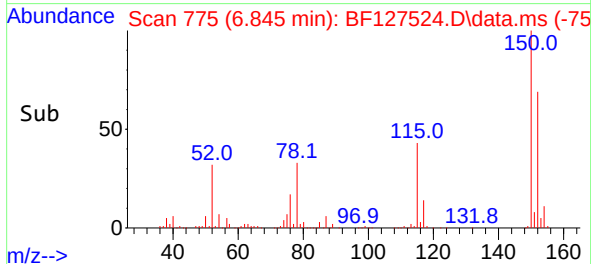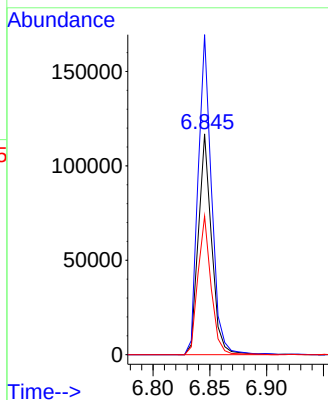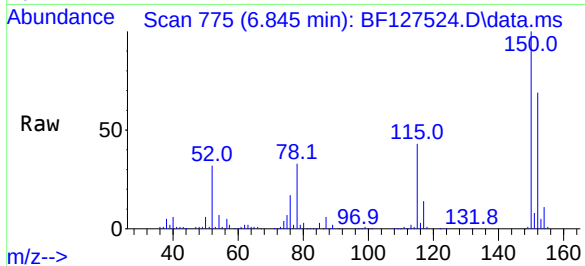

#5
2-Fluorophenol
Concen: 71.520 ng
RT: 5.475 min Scan# 542
Delta R.T. 0.006 min
Lab File: BF127524.D
Acq: 25 Mar 2022 13:05

Tgt Ion:112 Resp: 427196
Ion Ratio Lower Upper
112 100
64 74.1 58.4 87.6
63 39.1 30.1 45.1


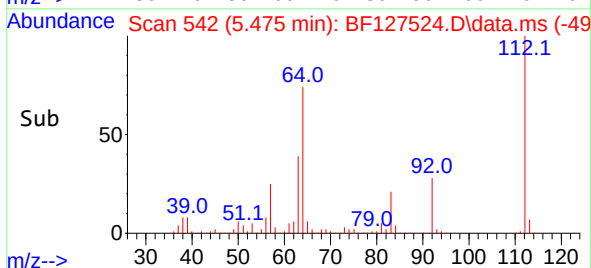
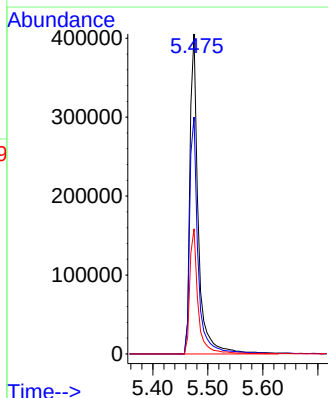
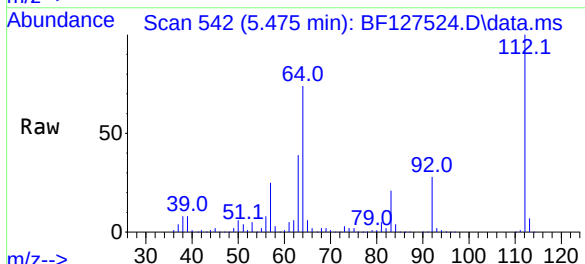


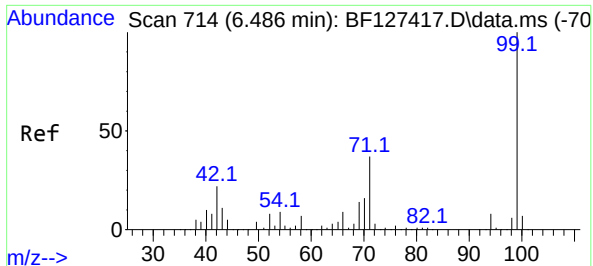

#7
Phenol-d6
Concen: 46.510 ng
RT: 6.481 min Scan# 714
Delta R.T. -0.006 min
Lab File: BF127524.D
Acq: 25 Mar 2022 13:05




Instrument :
BNA_F
ClientSampleId :
20220281-FIELD-BLANK


Tgt Ion: 99 Resp: 379747
Ion Ratio Lower Upper
99 100
42 22.9 17.8 26.6
71 36.4 29.6 44.4

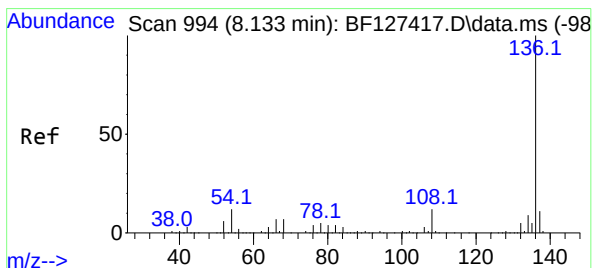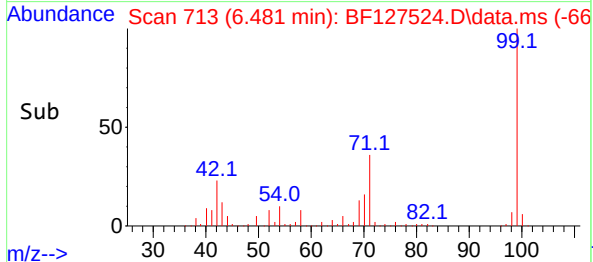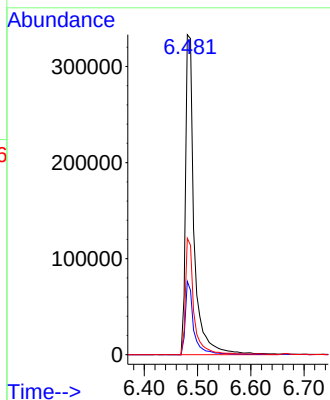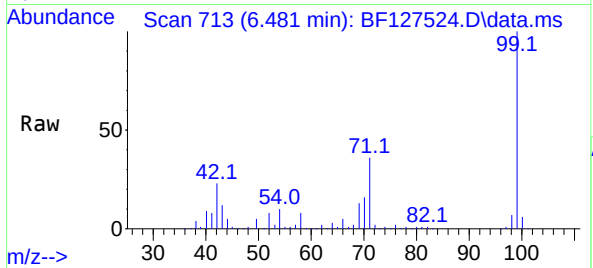

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.128 min Scan# 993
Delta R.T. -0.006 min
Lab File: BF127524.D
Acq: 25 Mar 2022 13:05

Tgt Ion: 136 Resp: 353426
Ion Ratio Lower Upper
136 100
137 10.8 8.6 13.0
54 12.2 9.2 13.8
68 7.0 5.4 8.0


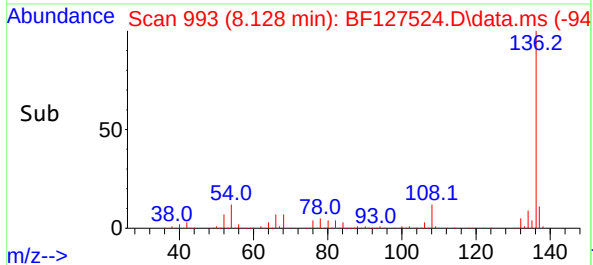
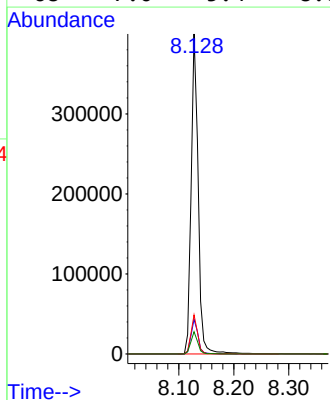
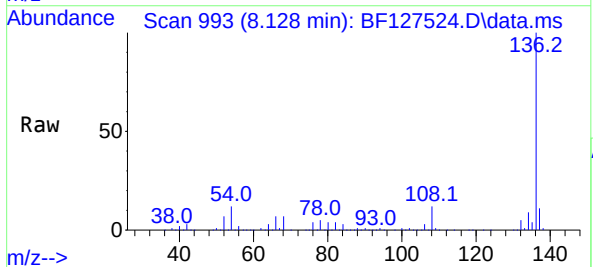


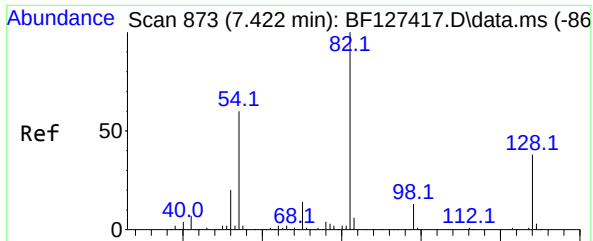

#23
Nitrobenzene-d5
Concen: 90.785 ng
RT: 7.416 min Scan# 81
Delta R.T. -0.006 min
Lab File: BF127524.D
Acq: 25 Mar 2022 13:05




Instrument :
BNA_F
ClientSampleId :
20220281-FIELD-BLANK


Tgt Ion: 82 Resp: 750620
Ion Ratio Lower Upper
82 100
128 38.1 30.6 45.8
54 61.1 48.2 72.2

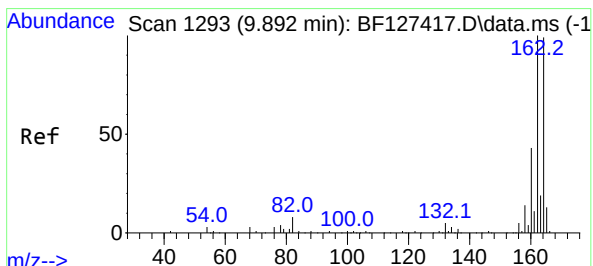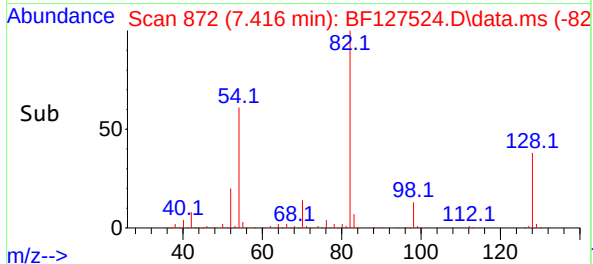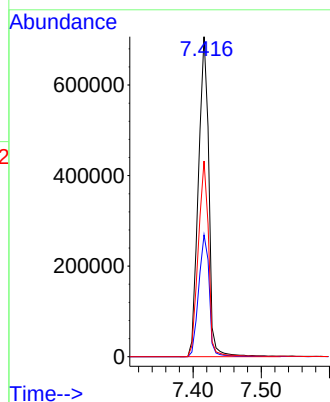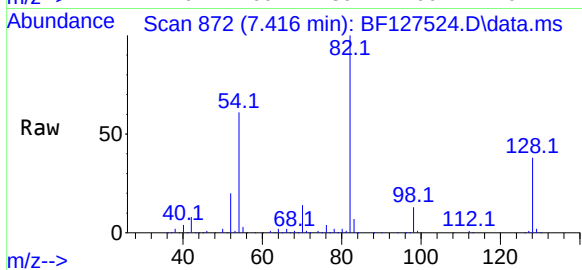

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.886 min Scan# 1292
Delta R.T. -0.006 min
Lab File: BF127524.D
Acq: 25 Mar 2022 13:05

Tgt Ion:164 Resp: 210995
Ion Ratio Lower Upper
164 100
162 98.0 81.2 121.8
160 43.6 34.6 52.0

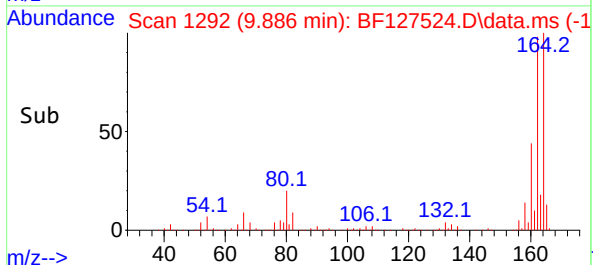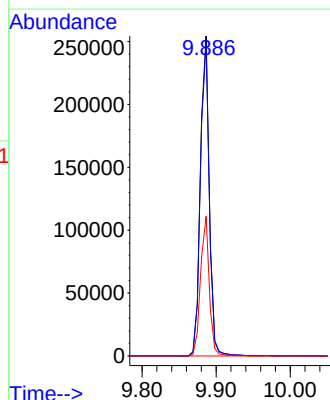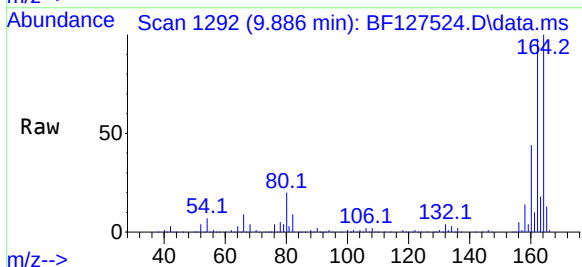

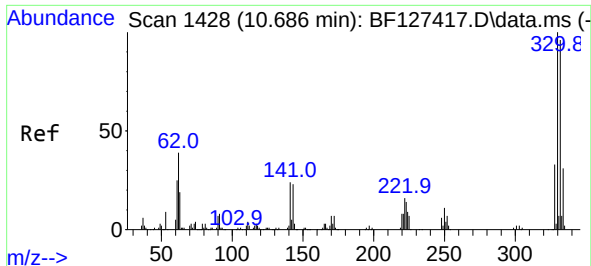

#42

2,4,6-Tribromophenol

Concen: 133.103 ng

RT: 10.686 min Scan# 1428

Delta R.T. 0.000 min

Lab File: BF127524.D


Acq: 25 Mar 2022 13:05

Instrument :

BNA_F

ClientSampleId :

20220281-FIELD-BLANK

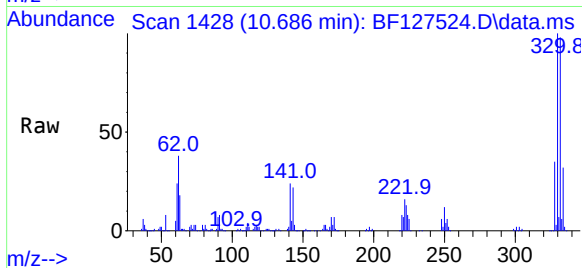




Tgt Ion:330 Resp: 299167

Ion Ratio Lower Upper

330 100

332 98.4 79.1 118.7

141 32.3 26.2 39.4

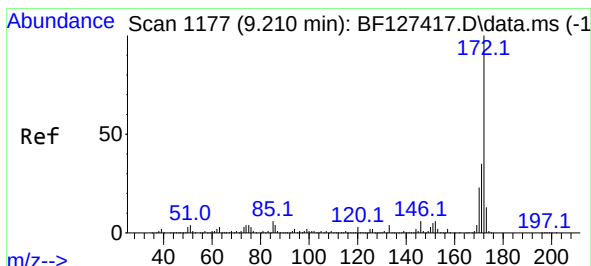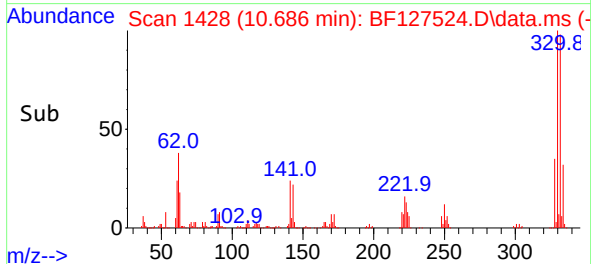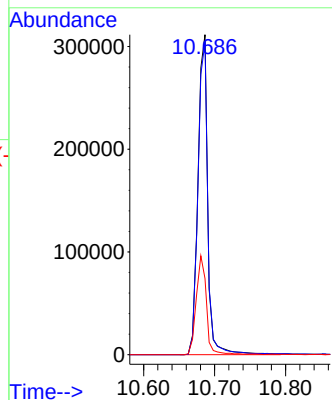

#45

2-Fluorobiphenyl

Concen: 85.556 ng

RT: 9.204 min Scan# 1176

Delta R.T. -0.006 min

Lab File: BF127524.D

Acq: 25 Mar 2022 13:05




Tgt Ion:172 Resp: 1236228


Ion Ratio Lower Upper

172 100

171 35.6 28.4 42.6

170 23.6 18.6 27.8


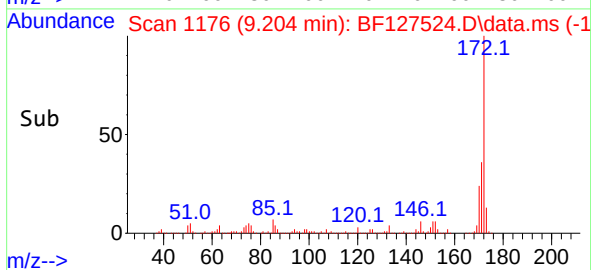
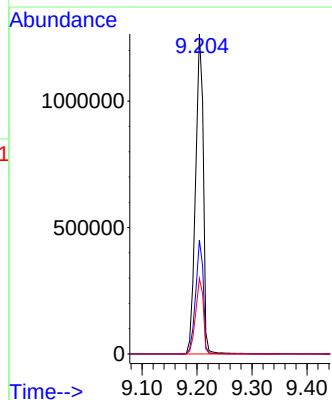
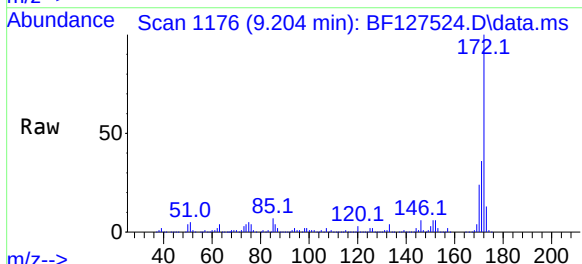


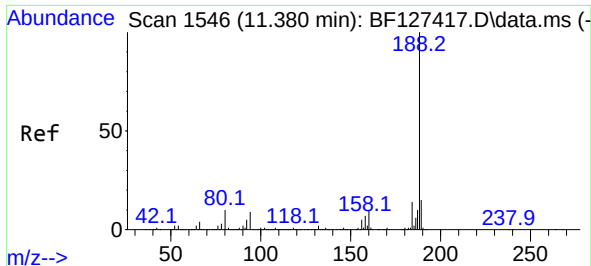

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.380 min Scan# 11
Delta R.T. 0.000 min
Lab File: BF127524.D
Acq: 25 Mar 2022 13:05




Instrument :
BNA_F
ClientSampleId :
20220281-FIELD-BLANK


Tgt Ion:188 Resp: 389784
Ion Ratio Lower Upper
188 100
94 8.8 7.4 11.0
80 9.2 8.0 12.0

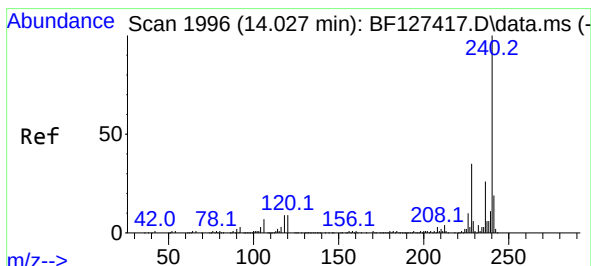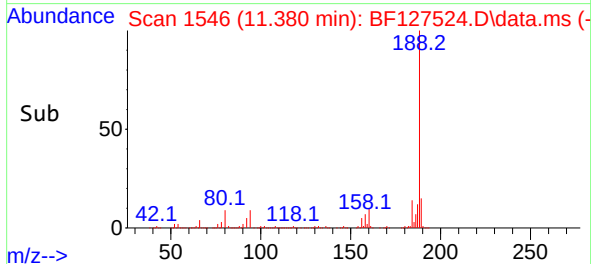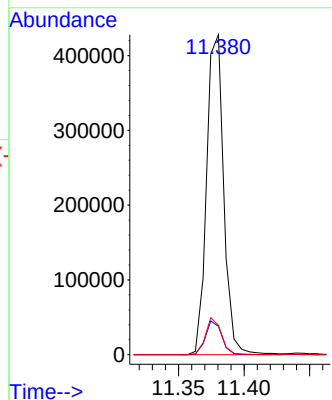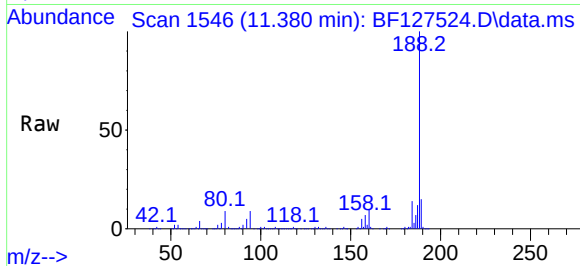

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.027 min Scan# 1996
Delta R.T. 0.000 min
Lab File: BF127524.D
Acq: 25 Mar 2022 13:05


Tgt Ion:240 Resp: 300382
Ion Ratio Lower Upper
240 100
120 9.2 7.1 10.7
236 25.8 20.7 31.1

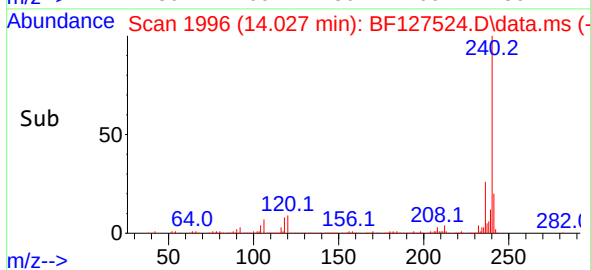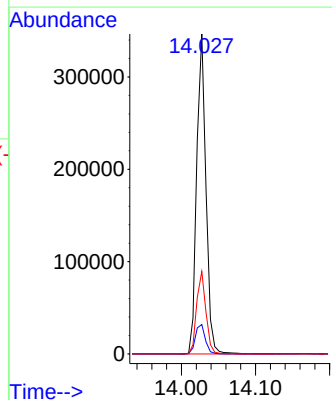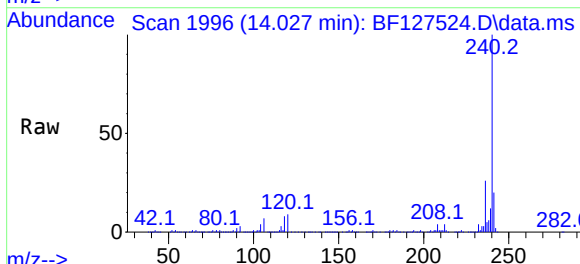

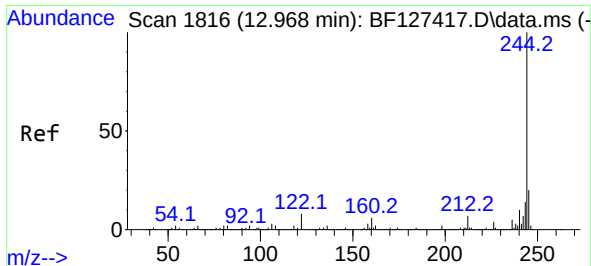




#79
 Terphenyl-d14
 Concen: 87.928 ng
 RT: 12.969 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BF127524.D
 Acq: 25 Mar 2022 13:05

Instrument :
 BNA_F
 ClientSampleId :
 20220281-FIELD-BLANK

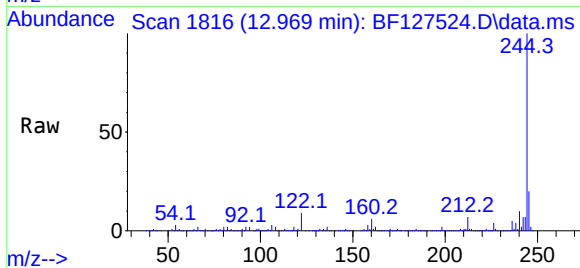

Tgt Ion:244 Resp: 1613413

Ion	Ratio	Lower	Upper
244	100		
212	7.0	5.7	8.5
122	9.1	6.2	9.2

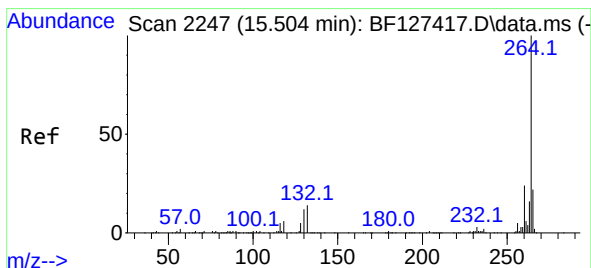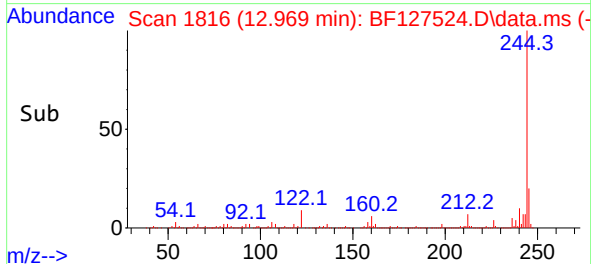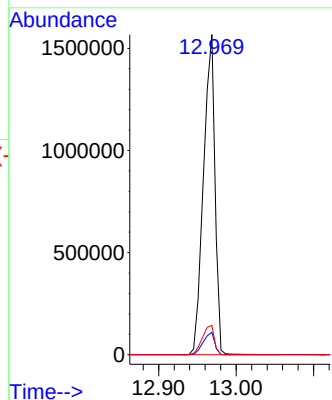

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.510 min Scan# 2248
 Delta R.T. 0.006 min
 Lab File: BF127524.D
 Acq: 25 Mar 2022 13:05

Tgt Ion:264 Resp: 217474

Ion	Ratio	Lower	Upper
264	100		
260	23.5	19.1	28.7
265	21.3	17.4	26.2

