
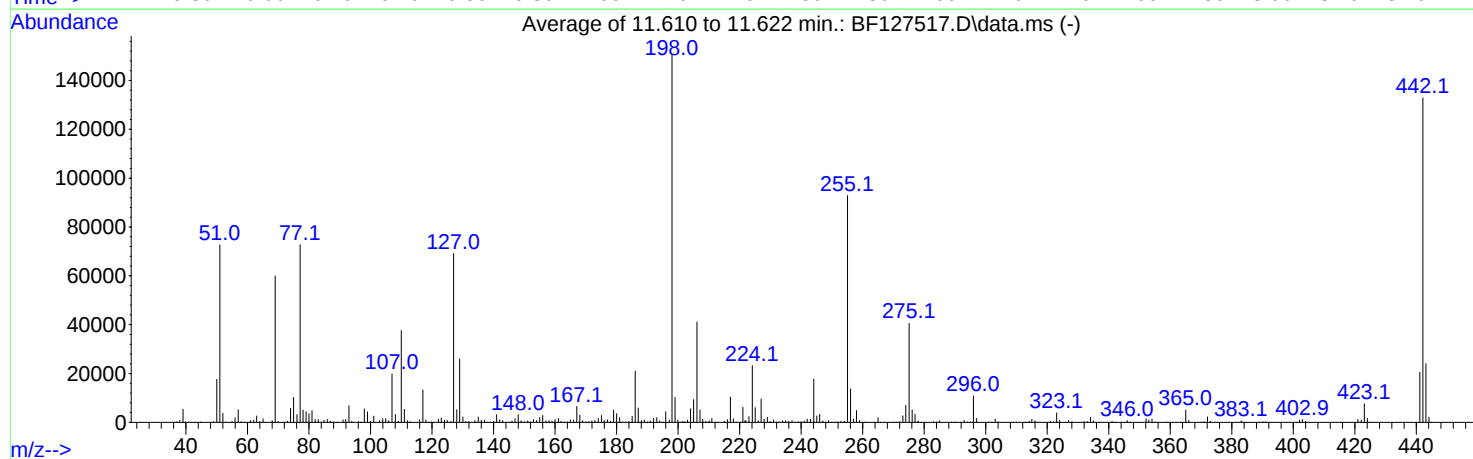


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032522\
 Data File : BF127517.D
 Acq On : 25 Mar 2022 09:19
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 22 02:16:33 2022

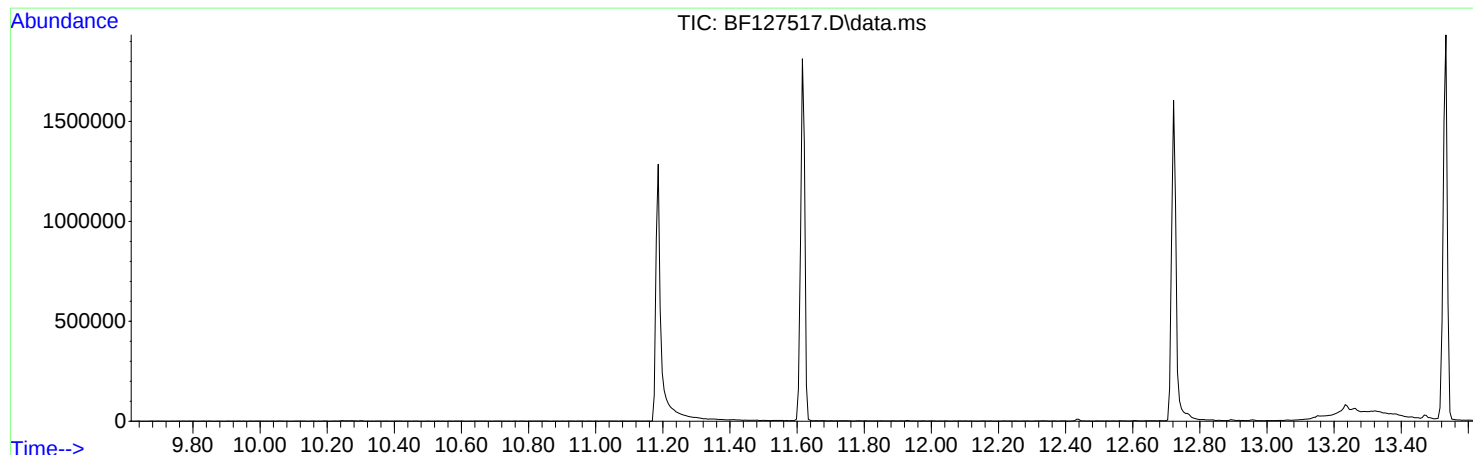




AutoFind: Scans 1585, 1586, 1587; Background Corrected with Scan 1580

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.2	72659	PASS
68	69	0.00	2	1.1	631	PASS
69	198	0.00	100	39.8	59968	PASS
70	69	0.00	2	0.5	324	PASS
127	198	10	80	45.9	69136	PASS
197	198	0.00	2	0.6	969	PASS
198	198	100	100	100.0	150619	PASS
199	198	5	9	6.8	10249	PASS
275	198	10	60	26.9	40589	PASS
365	198	1	100	3.4	5048	PASS
441	198	0.01	100	13.6	20517	PASS
442	442	50	100	100.0	132851	PASS
443	442	15	24	18.1	24071	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032522\
Data File : BF127517.D
Acq On : 25 Mar 2022 09:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 25 18:10:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 22 02:16:33 2022
Response via : Initial Calibration

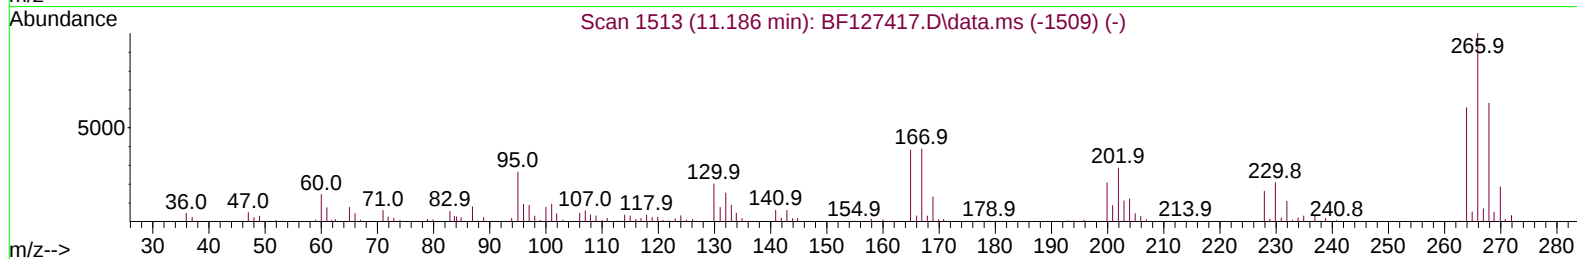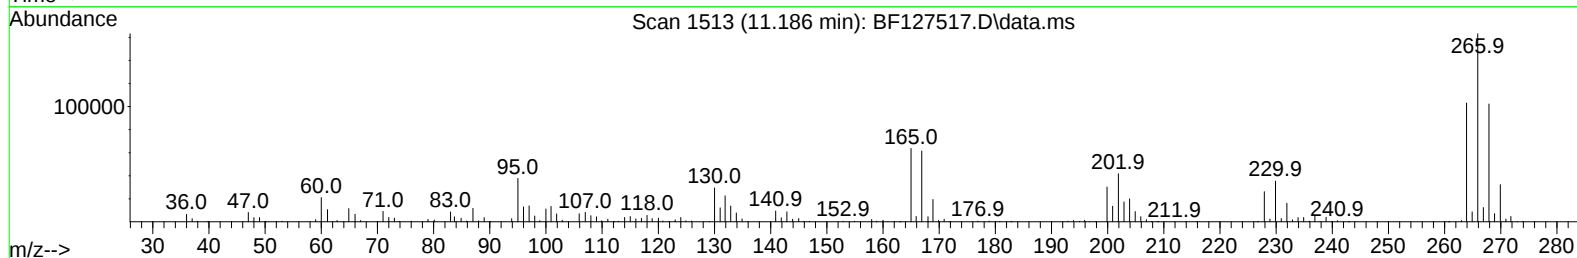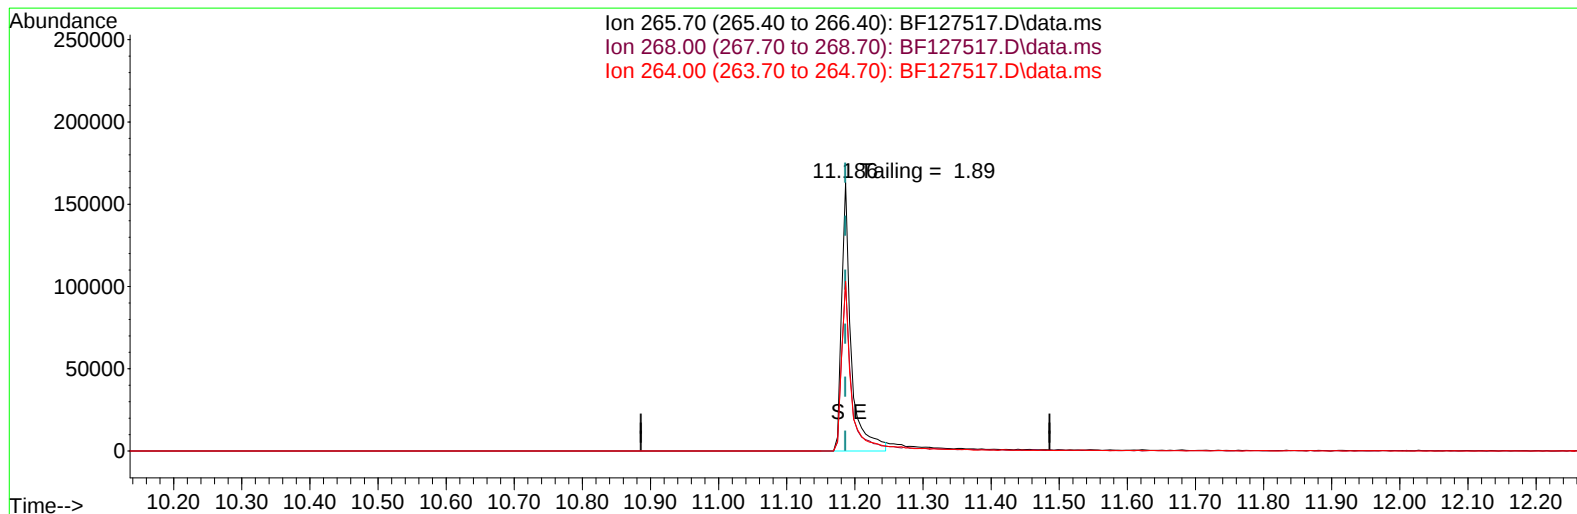

TIC: BF127517.D\data.ms

(70) Pentachlorophenol (C)

11.186min (+ 0.000) 449094.64 ng




response 164089

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.65
264.00	60.60	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032522\
Data File : BF127517.D
Acq On : 25 Mar 2022 09:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 25 18:10:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 22 02:16:33 2022
Response via : Initial Calibration

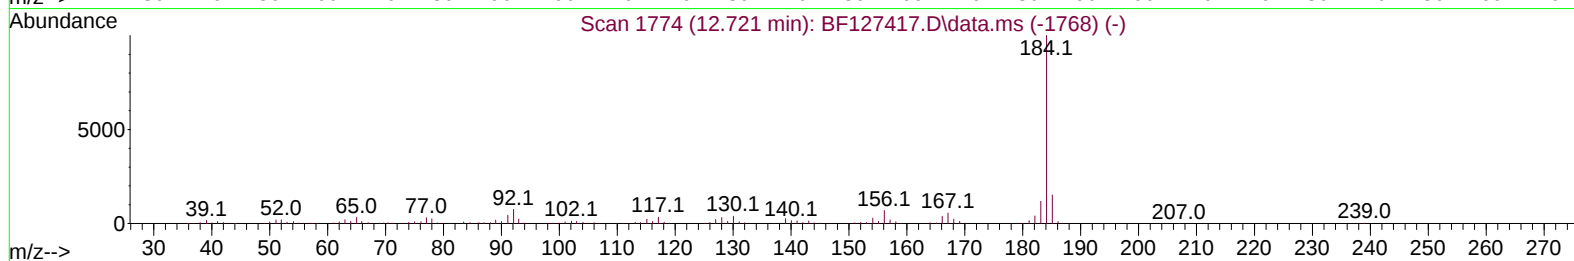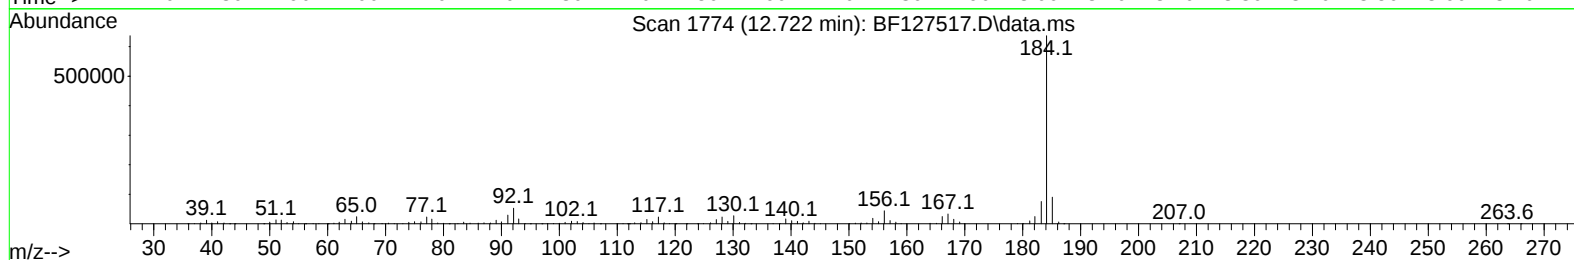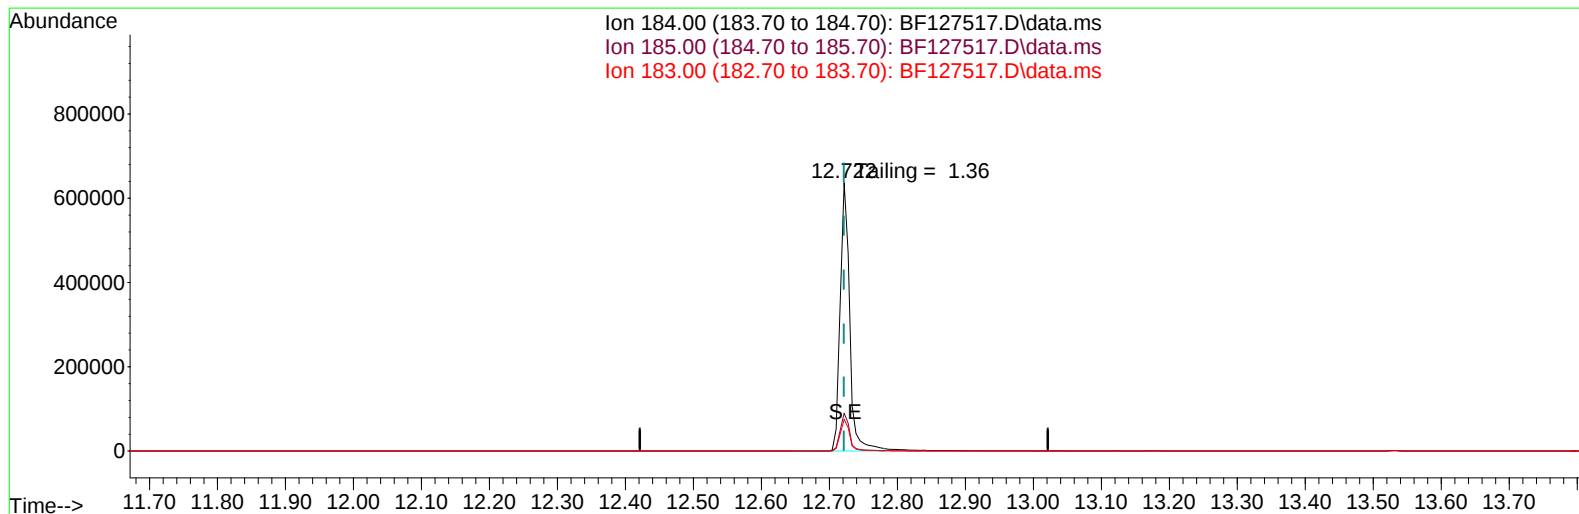

TIC: BF127517.D\data.ms

(77) Benzidine

12.722min (+ 0.000) 5915.12 ng m

response 614087

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.16
183.00	11.70	11.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/25/2022	BNA_F	<u>BF127517.D</u>
Compound Name	Response	Retention Time
DDT	330204	13.53
DDD	6139	13.23
DDE	716	12.89
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6855	337059	2.03

Instrument :
BNA_F
ClientSampleId :
DFTPP