

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032619\
 Data File : BF113302.D
 Acq On : 26 Mar 2019 20:25
 Operator : JU/SJ
 Sample : K2081-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S4C(6-18)COMP

Quant Time: Mar 27 07:22:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 26 03:32:08 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	167336	20.00	ng	0.00
21) Naphthalene-d8	7.98	136	647228	20.00	ng	0.00
39) Acenaphthene-d10	9.73	164	309540	20.00	ng	0.00
64) Phenanthrene-d10	11.21	188	595321	20.00	ng	0.00
76) Chrysene-d12	13.83	240	404496	20.00	ng	-0.01
87) Perylene-d12	15.23	264	428660	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	1366578	133.53	ng	0.01
7) Phenol-d6	6.36	99	1714807	132.45	ng	0.00
23) Nitrobenzene-d5	7.26	82	1162324	106.59	ng	0.00
42) 2,4,6-Tribromophenol	10.52	330	385794	100.90	ng	0.00
45) 2-Fluorobiphenyl	9.06	172	1931212	101.14	ng	0.00
79) Terphenyl-d14	12.79	244	1750789	95.40	ng	0.00
Target Compounds						
10) Phenol	6.36	94	45426	3.073	ng	79
50) Dimethylphthalate	9.45	163	131356	5.726	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032619\
Data File : BF113302.D
Acq On : 26 Mar 2019 20:25
Operator : JU/SJ
Sample : K2081-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S4C(6-18)COMP

Quant Time: Mar 27 07:22:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 26 03:32:08 2019
Response via : Initial Calibration

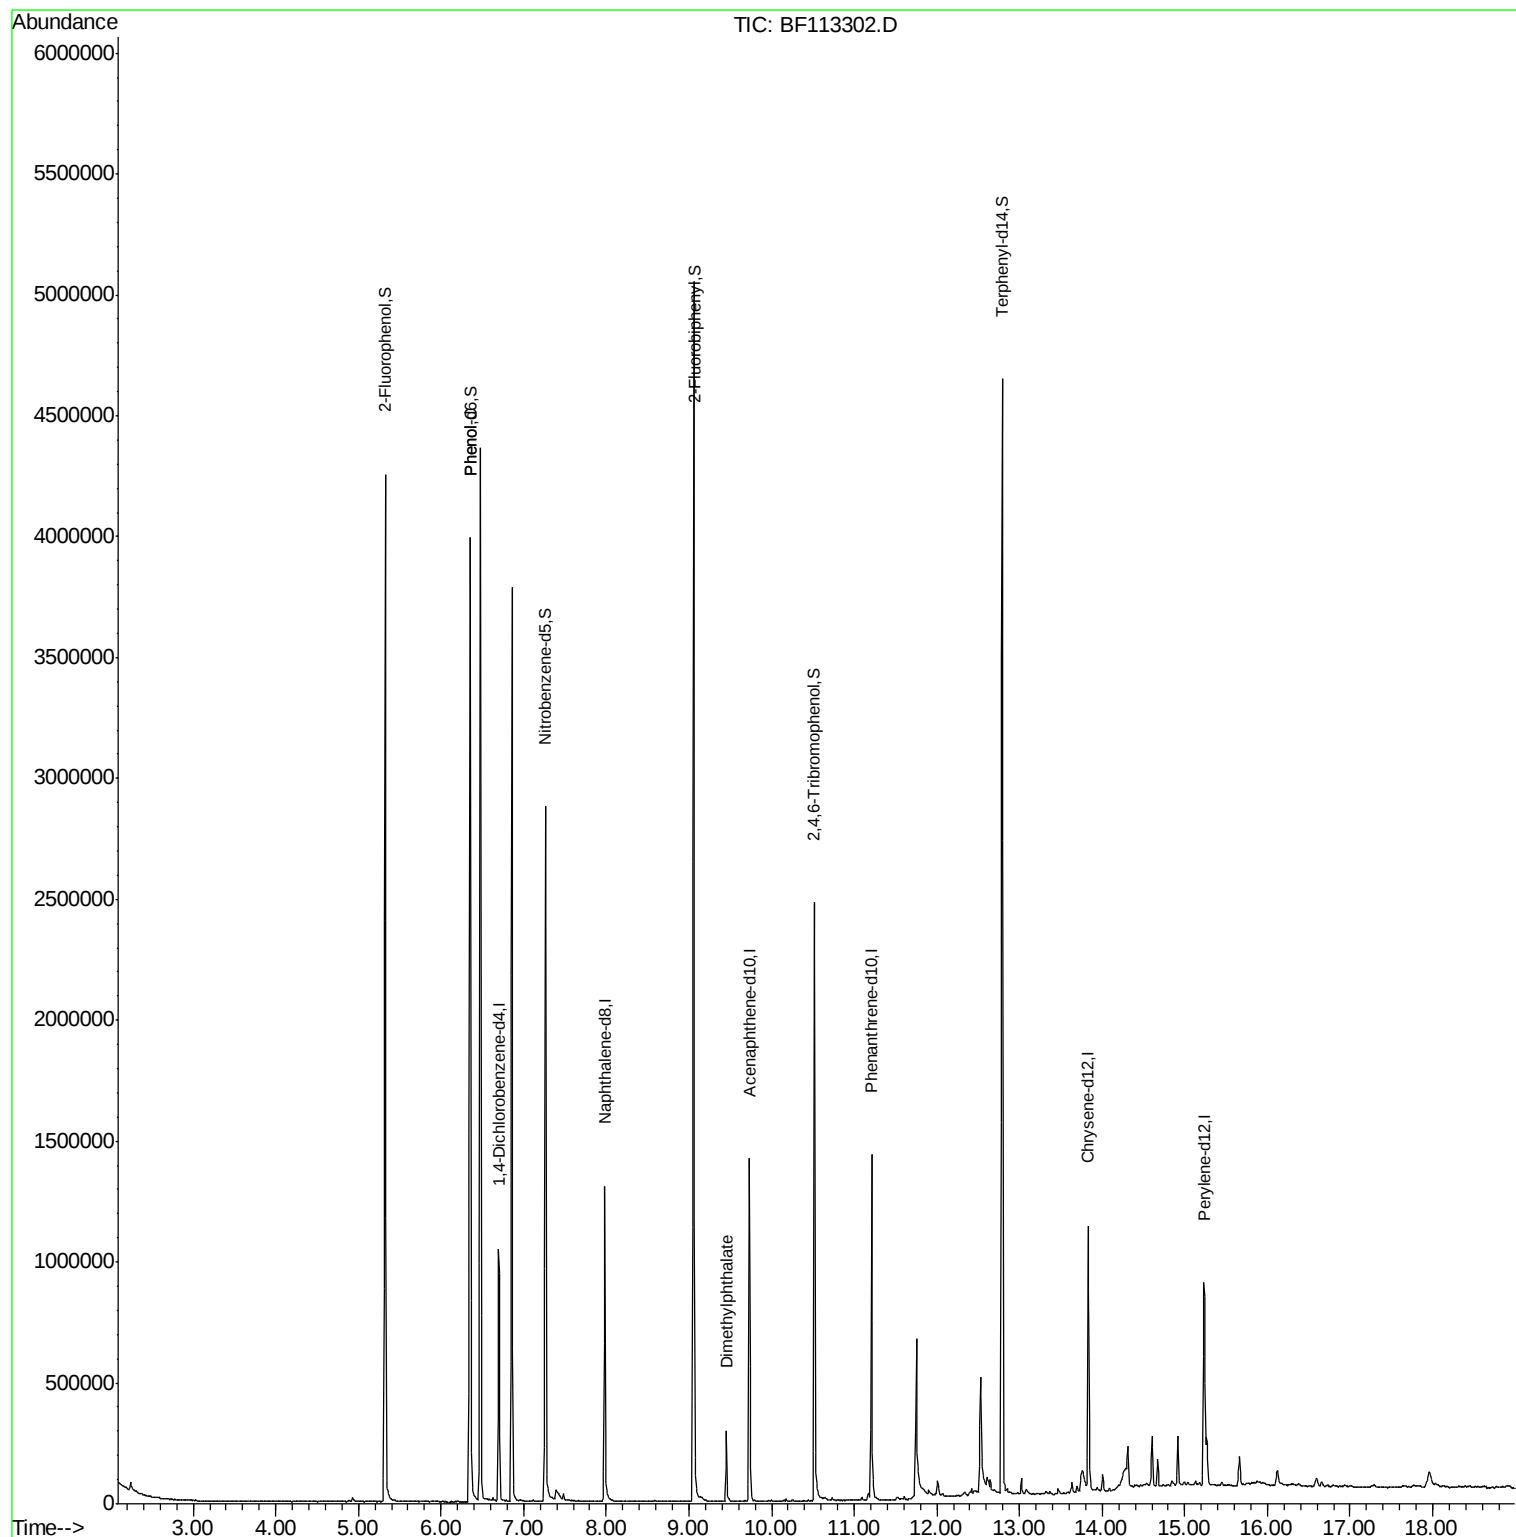

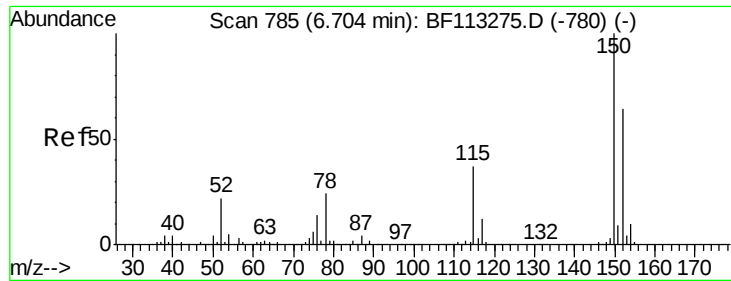


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.70 min Scan# 784
Delta R.T. -0.01 min
Lab File: BF113302.D
Acq: 26 Mar 2019 20:25

Instrument :
BNA_F
ClientSampleId :
S4C(6-18)COMP

Tgt Ion:152 Resp: 167336
Ion Ratio Lower Upper
152 100
150 161.3 124.7 187.1
115 60.4 46.0 69.0

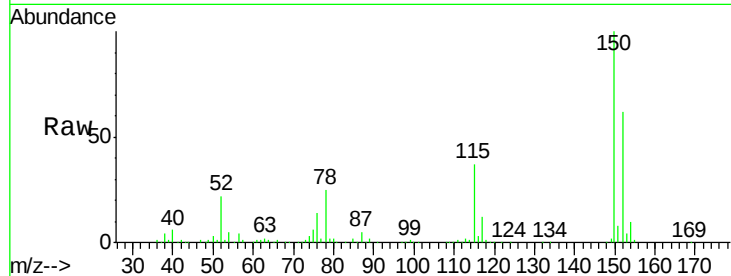


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

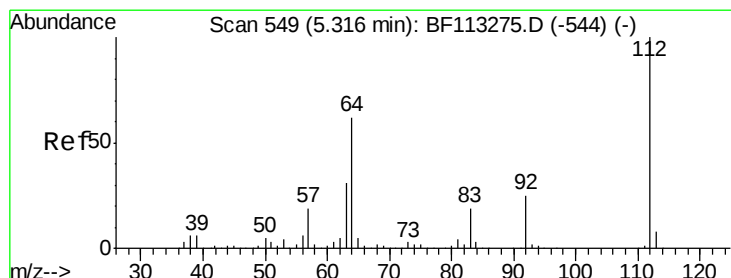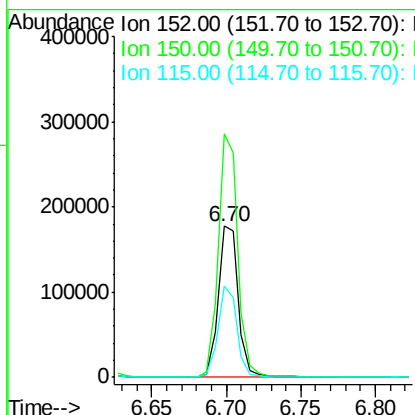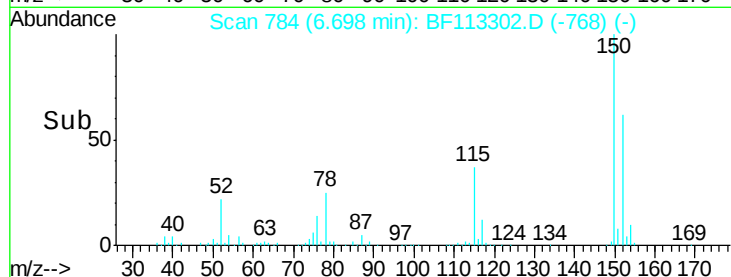



#5


2-Fluorophenol
Concen: 133.535 ng
RT: 5.33 min Scan# 551
Delta R.T. 0.01 min
Lab File: BF113302.D
Acq: 26 Mar 2019 20:25

Tgt Ion:112 Resp: 1366578
Ion Ratio Lower Upper
112 100
64 58.7 49.2 73.8
63 30.1 24.9 37.3

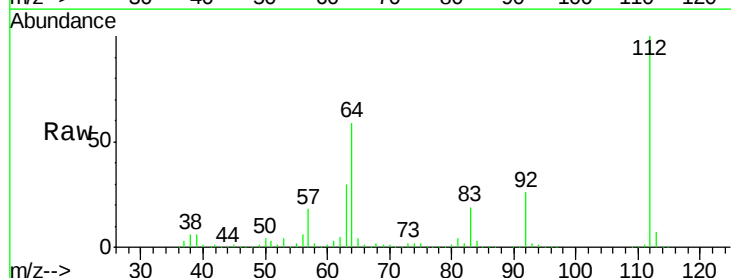

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

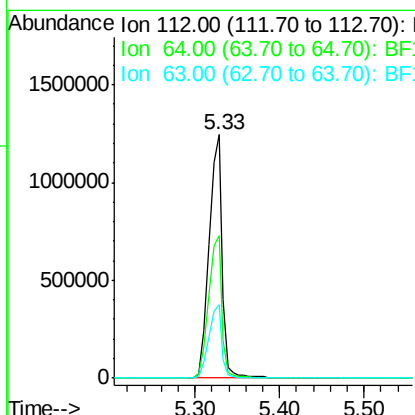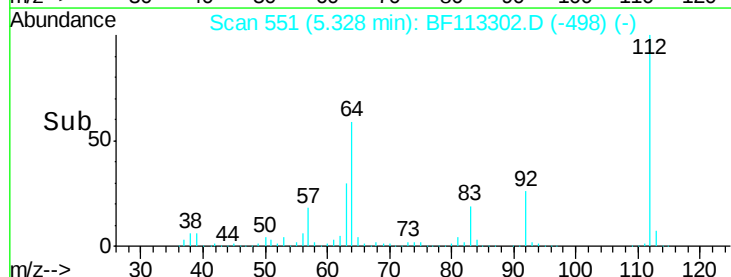

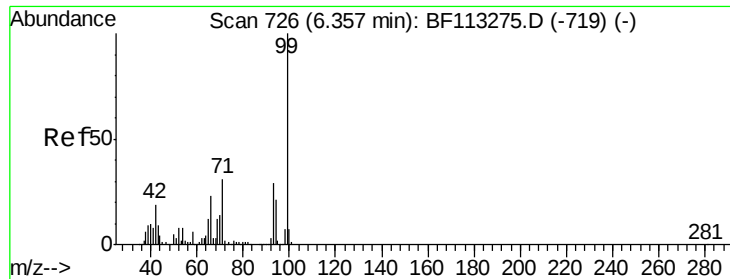

#7

Phenol-d6

Concen: 132.454 ng

RT: 6.36 min Scan# 726

Delta R.T. 0.00 min

Lab File: BF113302.D

Acq: 26 Mar 2019 20:25

Instrument :

BNA_F

ClientSampleId :

S4C(6-18)COMP


Tgt Ion: 99 Resp: 1714807

Ion Ratio Lower Upper

99 100

42 18.6 14.8 22.2




71 32.3 24.9 37.3

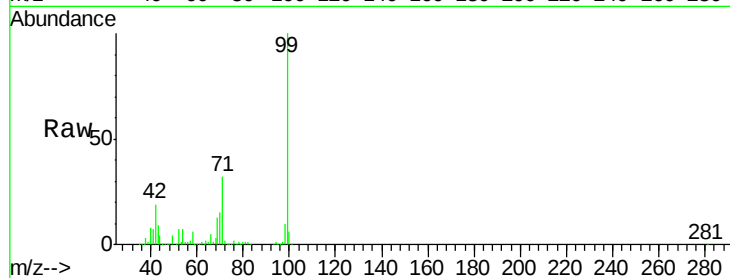

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

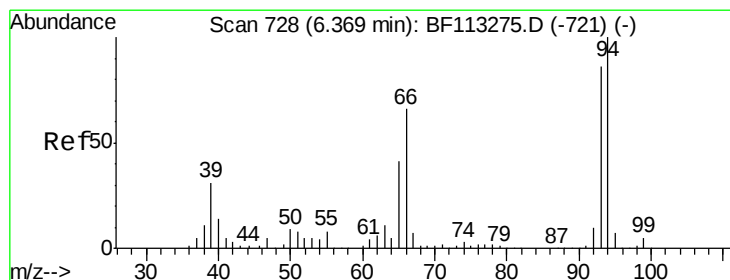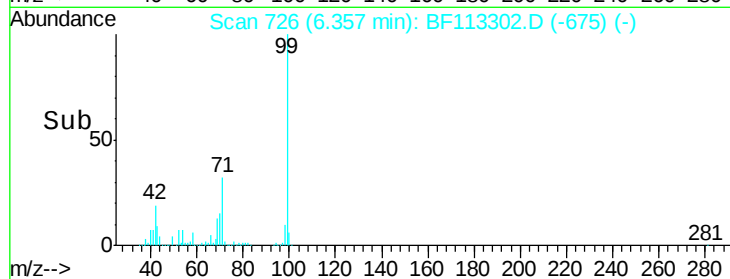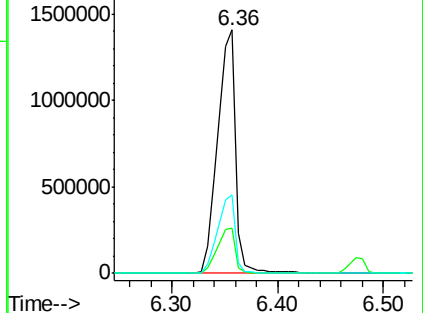

#10

Phenol

Concen: 3.073 ng

RT: 6.36 min Scan# 727

Delta R.T. -0.01 min

Lab File: BF113302.D

Acq: 26 Mar 2019 20:25


Tgt Ion: 94 Resp: 45426

Ion Ratio Lower Upper

94 100

65 28.7 21.4 61.4



66 48.6 46.4 86.4

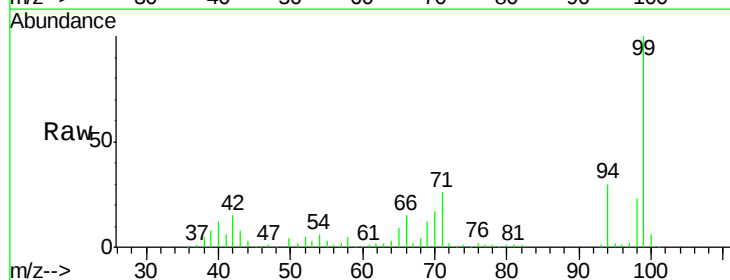

Abundance Ion 94.00 (93.70 to 94.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

Ion 66.00 (65.70 to 66.70): BF1

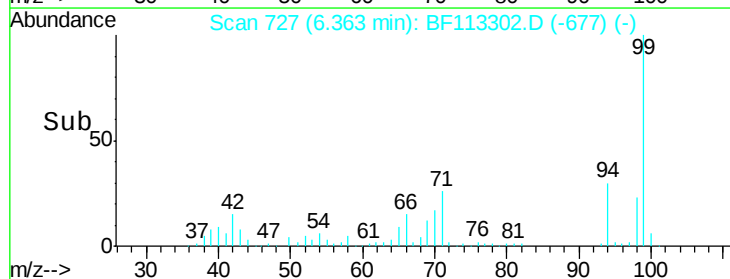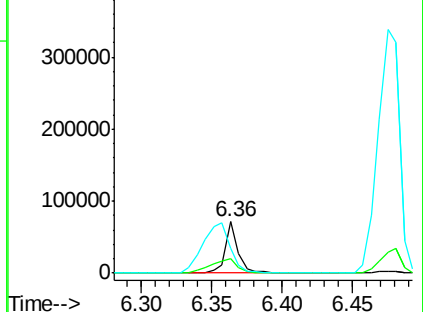







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.98 min Scan# 1002
Delta R.T. -0.01 min
Lab File: BF113302.D
Acq: 26 Mar 2019 20:25

Instrument :
BNA_F
ClientSampleId :
S4C(6-18)COMP

Tgt Ion:136	Resp:	647228
Ion	Ratio	Lower Upper
136	100	
137	11.4	8.9 13.3
54	8.2	7.0 10.6
68	6.4	4.8 7.2

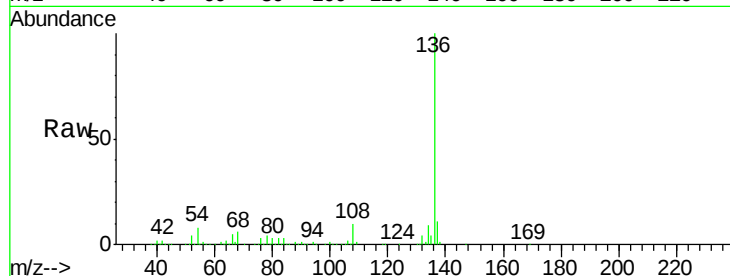


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

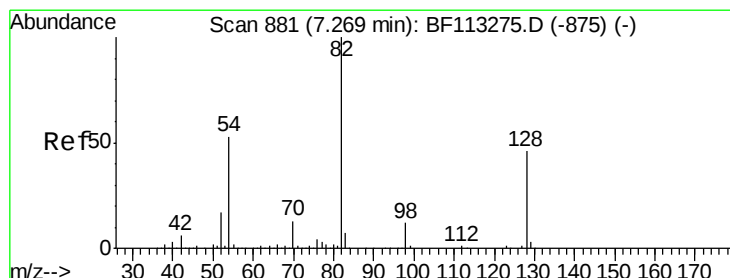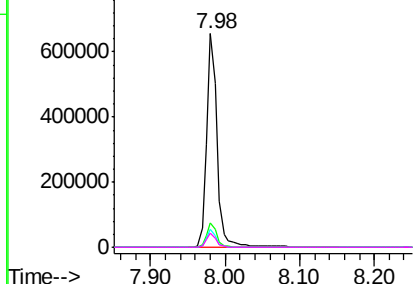
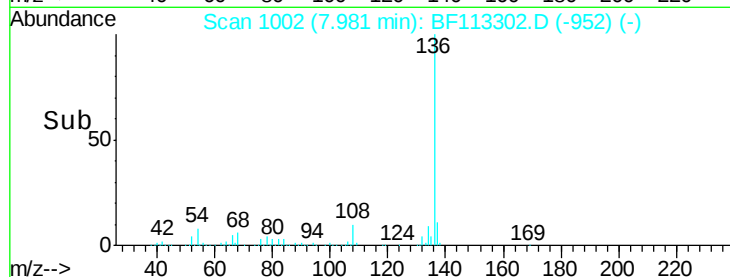



#23
Nitrobenzene-d5
Concen: 106.591 ng
RT: 7.26 min Scan# 880
Delta R.T. -0.00 min
Lab File: BF113302.D
Acq: 26 Mar 2019 20:25

Tgt Ion: 82	Resp:	1162324
Ion	Ratio	Lower Upper
82	100	
128	46.3	36.5 54.7
54	52.6	42.2 63.2

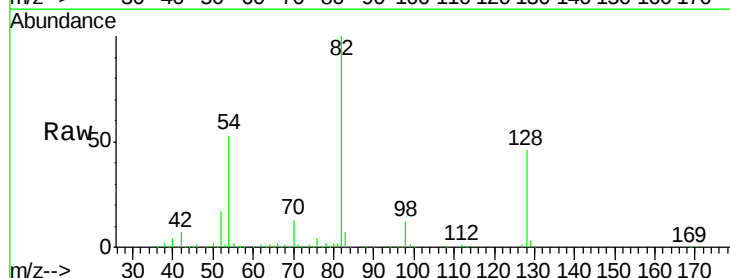

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

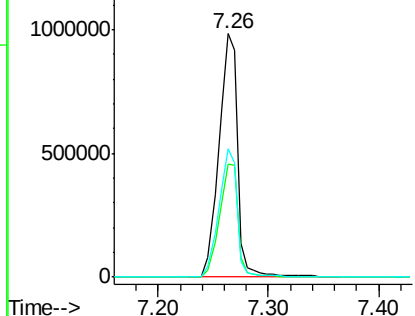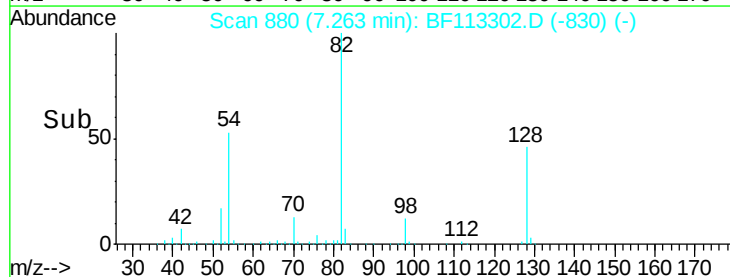

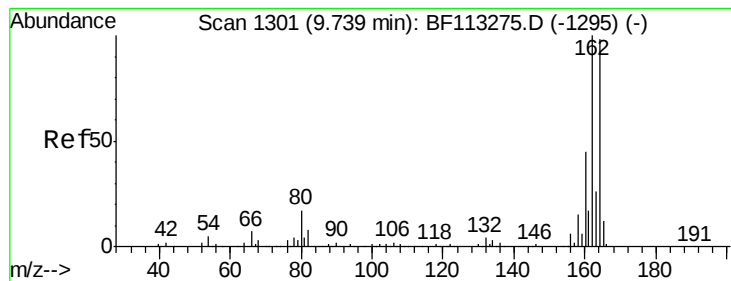

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.73 min Scan# 1300

Delta R.T. -0.01 min

Lab File: BF113302.D

Acq: 26 Mar 2019 20:25

Instrument :

BNA_F

ClientSampleId :

S4C(6-18)COMP


Tgt Ion:164 Resp: 309540

Ion Ratio Lower Upper

164 100

162 100.3 81.8 122.6




160 45.2 36.4 54.6

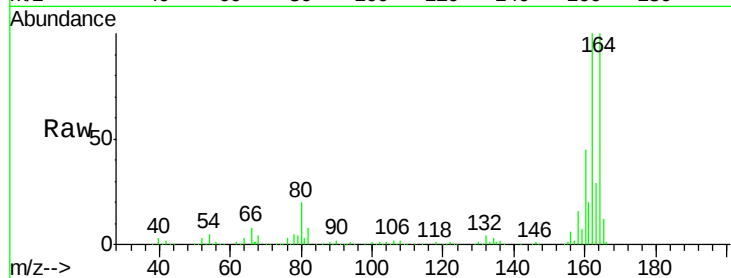

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

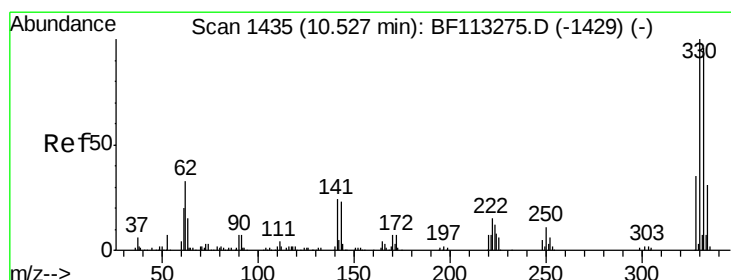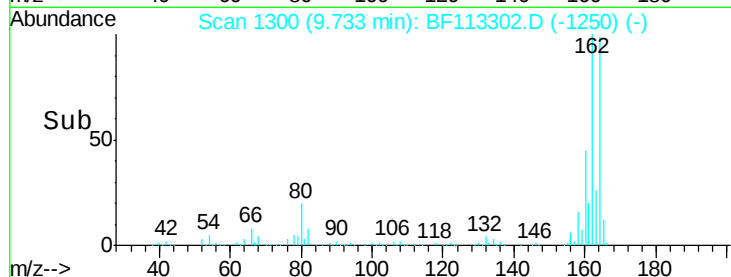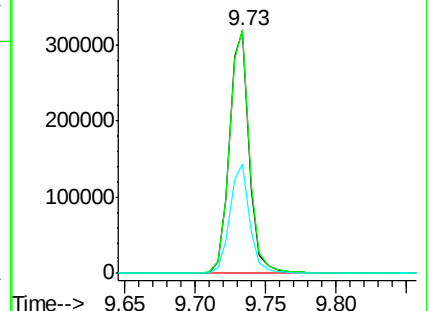

#42

2,4,6-Tribromophenol

Concen: 100.900 ng

RT: 10.52 min Scan# 1434

Delta R.T. -0.01 min

Lab File: BF113302.D

Acq: 26 Mar 2019 20:25


Tgt Ion:330 Resp: 385794

Ion Ratio Lower Upper

330 100

332 95.6 77.8 116.6



141 27.6 22.7 34.1

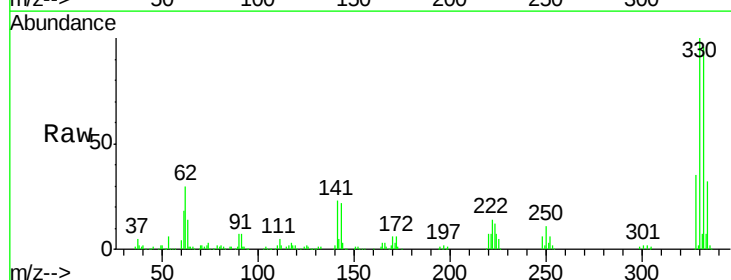


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

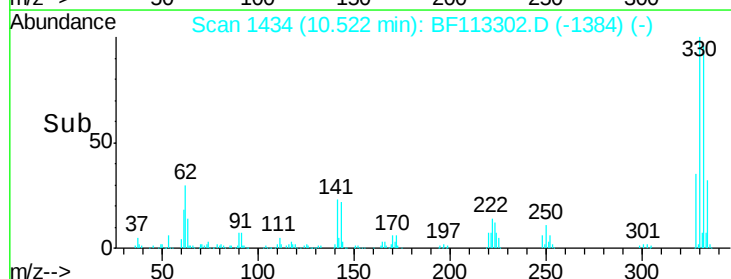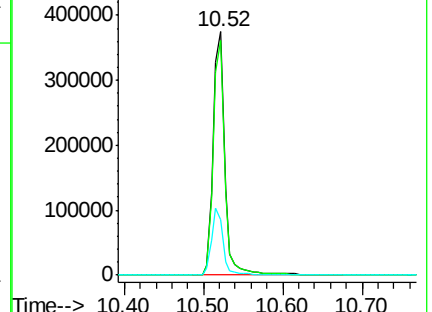


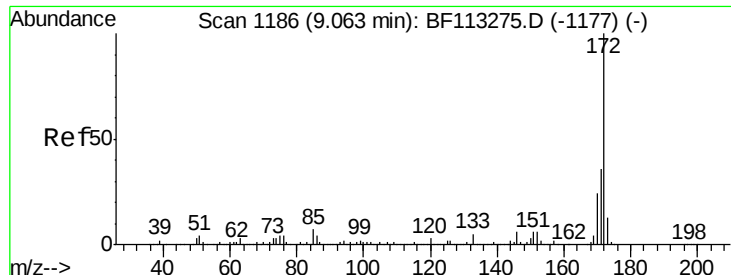




#45
 2-Fluorobiphenyl
 Concen: 101.135 ng
 RT: 9.06 min Scan# 1186
 Delta R.T. 0.00 min
 Lab File: BF113302.D
 Acq: 26 Mar 2019 20:25

Instrument :
 BNA_F
 ClientSampleId :
 S4C(6-18)COMP

Tgt Ion:172 Resp: 1931212
 Ion Ratio Lower Upper
 172 100
 171 36.3 29.0 43.6
 170 24.7 19.5 29.3

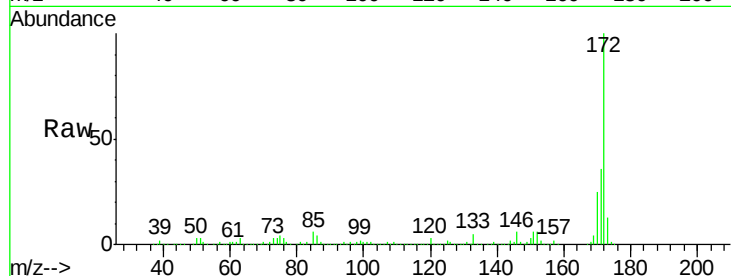


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

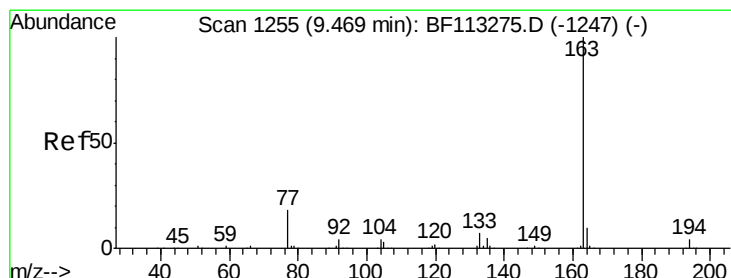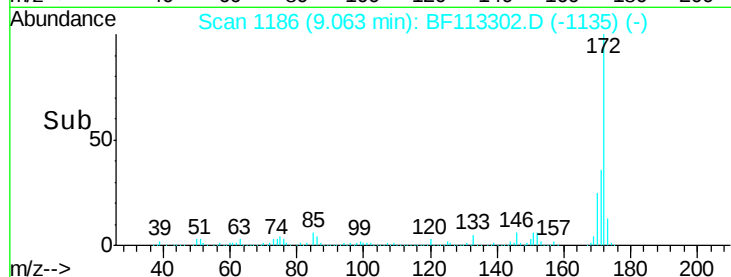
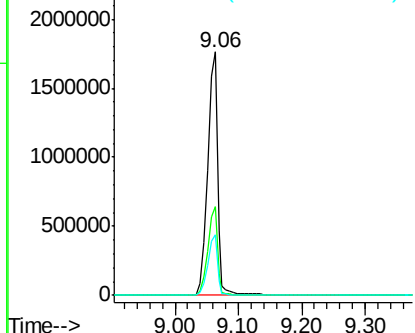



#50
 Dimethylphthalate
 Concen: 5.726 ng
 RT: 9.45 min Scan# 1252
 Delta R.T. -0.02 min
 Lab File: BF113302.D
 Acq: 26 Mar 2019 20:25

Tgt Ion:163 Resp: 131356
 Ion Ratio Lower Upper
 163 100
 194 3.9 3.0 4.6
 164 9.4 8.1 12.1

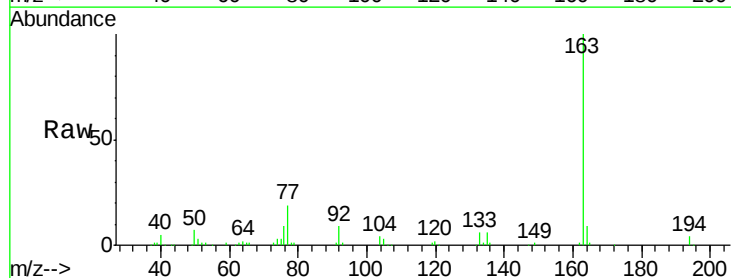

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E



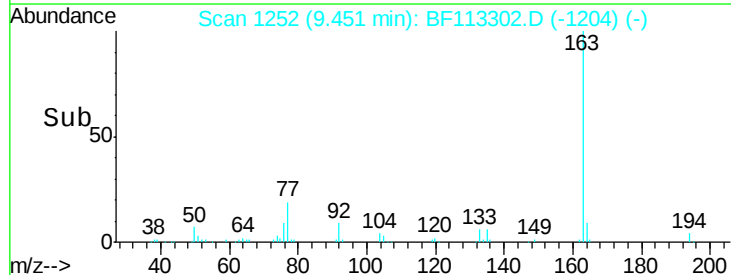
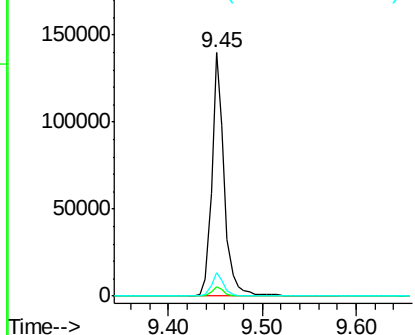


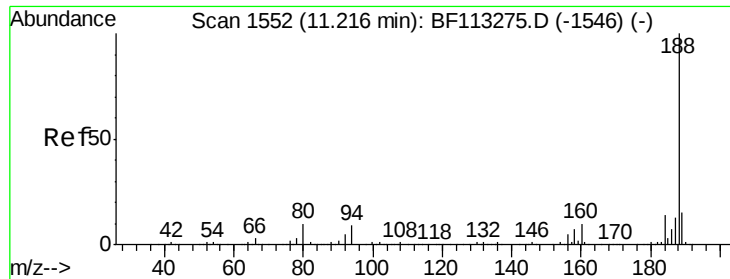

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.21 min Scan# 1551
Delta R.T. -0.01 min
Lab File: BF113302.D
Acq: 26 Mar 2019 20:25




Instrument :
BNA_F
ClientSampleId :
S4C(6-18)COMP


Tgt Ion:188 Resp: 595321
Ion Ratio Lower Upper
188 100
94 9.5 7.0 10.6
80 9.6 7.7 11.5

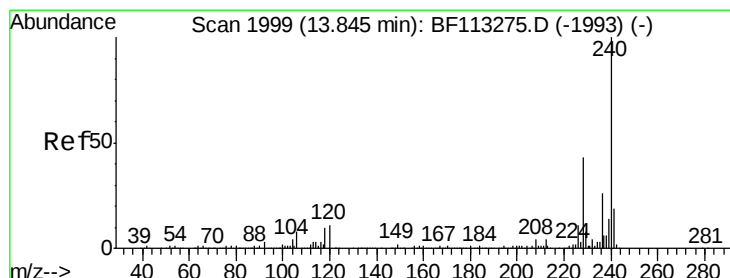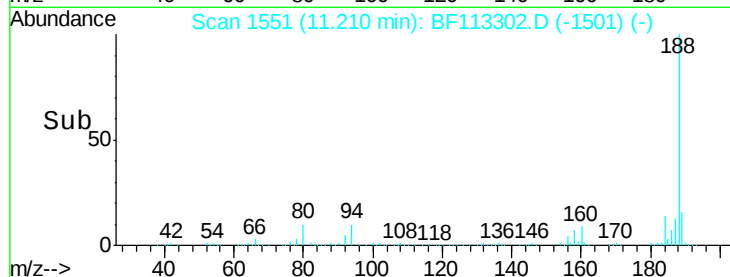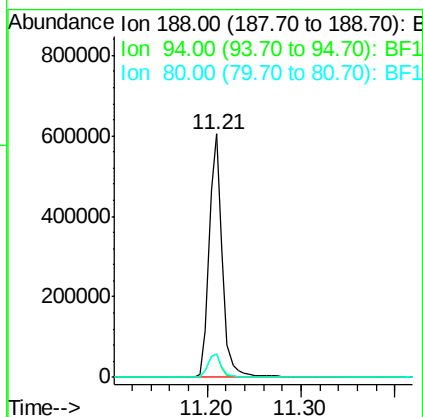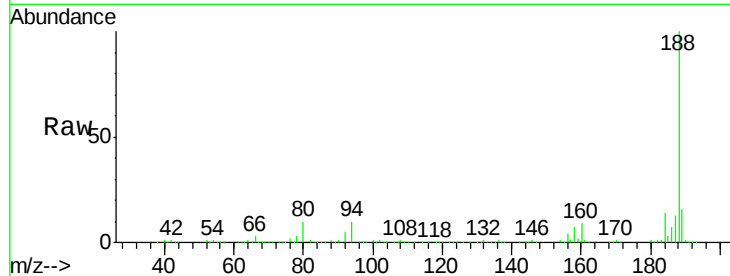

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.83 min Scan# 1997
Delta R.T. -0.01 min
Lab File: BF113302.D
Acq: 26 Mar 2019 20:25

Tgt Ion:240 Resp: 404496
Ion Ratio Lower Upper
240 100
120 11.0 8.8 13.2
236 25.8 20.9 31.3


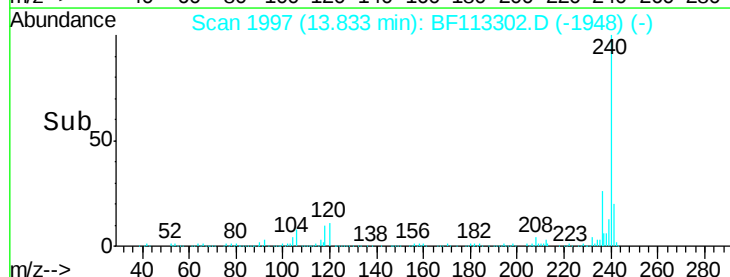
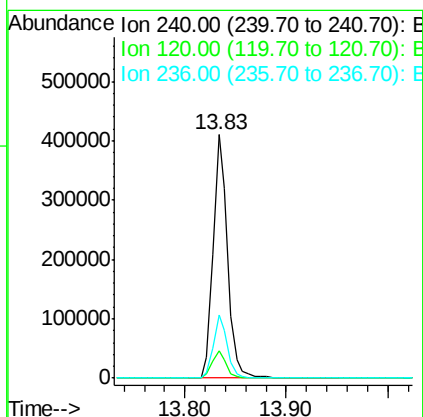
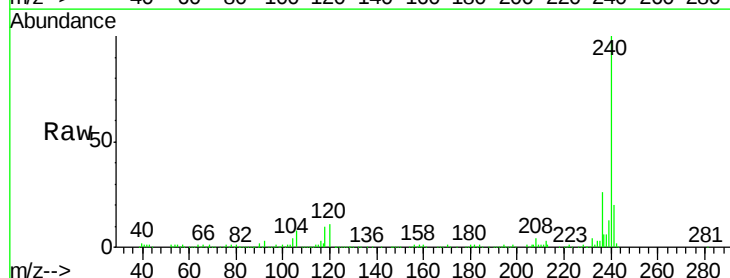


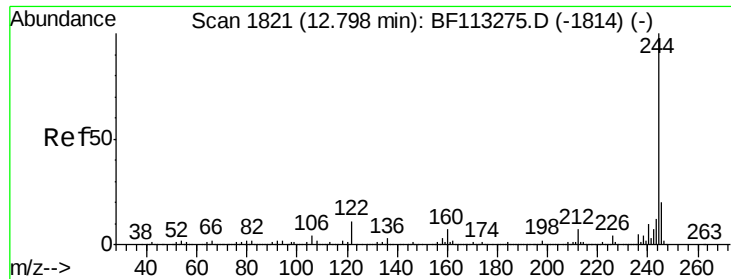

#79
 Terphenyl-d14
 Concen: 95.404 ng
 RT: 12.79 min Scan# 1820
 Delta R.T. -0.00 min
 Lab File: BF113302.D
 Acq: 26 Mar 2019 20:25

Instrument :
 BNA_F
 ClientSampleId :
 S4C(6-18)COMP

Tgt Ion:244 Resp: 1750789
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.5 8.3
 122 11.3 8.6 13.0

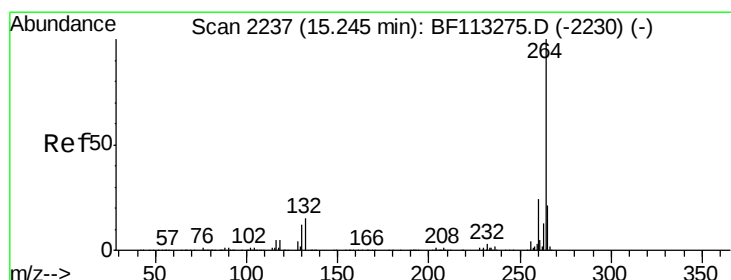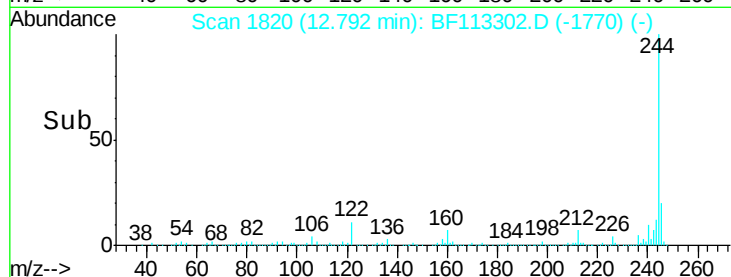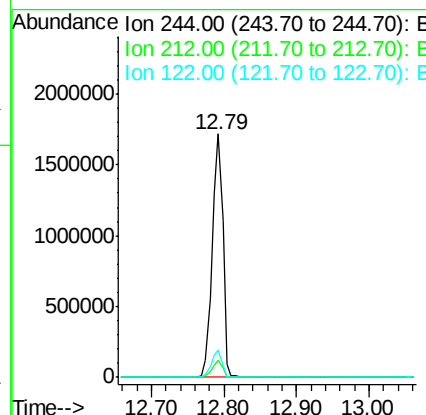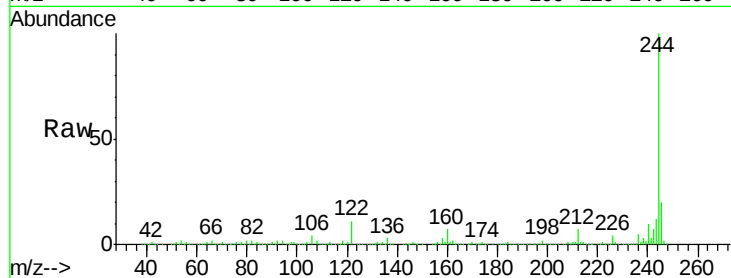

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.23 min Scan# 2235
 Delta R.T. -0.01 min
 Lab File: BF113302.D
 Acq: 26 Mar 2019 20:25

Tgt Ion:264 Resp: 428660
 Ion Ratio Lower Upper
 264 100
 260 23.6 19.1 28.7
 265 21.4 17.1 25.7

