

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032619\
 Data File : BF113289.D
 Acq On : 26 Mar 2019 13:52
 Operator : JU/SJ
 Sample : PB118273BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB118273BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.328	546	551	571	rBV	3679448	4132831	83.85%	10.550%
2	6.351	720	725	728	rBV	3770720	4161219	84.43%	10.622%
3	6.475	741	746	750	rBV	4174407	4272803	86.69%	10.907%
4	6.698	781	784	798	rVB	1115067	1067009	21.65%	2.724%
5	6.857	807	811	815	rBV	3464142	3318915	67.34%	8.472%
6	7.263	875	880	883	rBV	2471683	2749150	55.78%	7.018%
7	7.981	997	1002	1019	rBV	1261413	1345362	27.30%	3.434%
8	9.063	1179	1186	1189	rBV	4773973	4928627	100.00%	12.581%
9	9.733	1294	1300	1313	rBV	1480888	1492622	30.28%	3.810%
10	10.522	1429	1434	1454	rBV	2849766	2951819	59.89%	7.535%
11	11.210	1547	1551	1569	rVB	1655472	1642975	33.34%	4.194%
12	12.792	1815	1820	1823	rBV	4581351	4655520	94.46%	11.884%
13	13.839	1993	1998	2008	rBV	979066	1127230	22.87%	2.878%
14	14.921	2178	2182	2186	rBV	50421	60736	1.23%	0.155%
15	15.239	2231	2236	2253	rBV	793407	1135529	23.04%	2.899%
16	15.668	2305	2309	2314	rVB	48057	64865	1.32%	0.166%
17	16.127	2382	2387	2394	rVB2	37178	66710	1.35%	0.170%


Sum of corrected areas: 39173922

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032619\
Data File : BF113289.D
Acq On : 26 Mar 2019 13:52
Operator : JU/SJ
Sample : PB118273BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118273BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

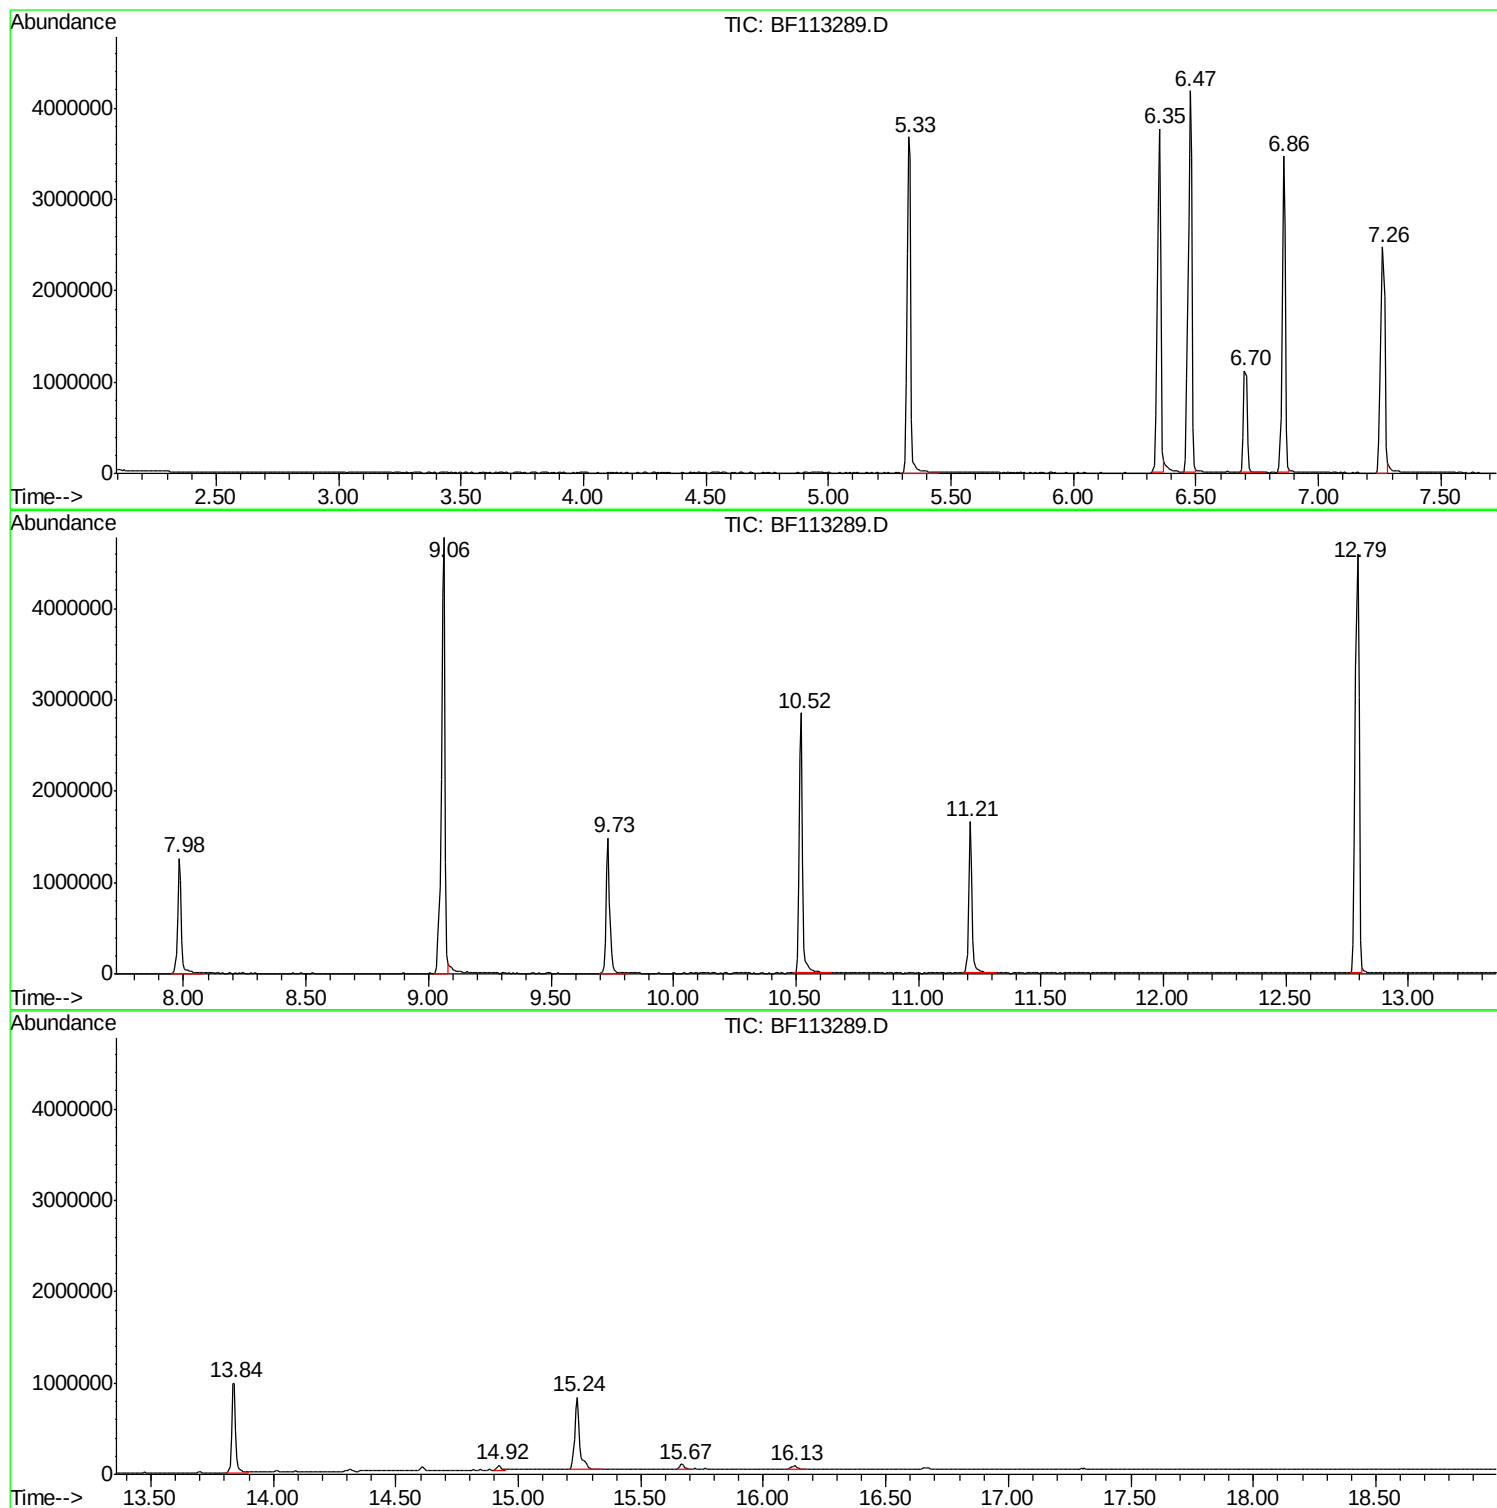

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032619\
Data File : BF113289.D
Acq On : 26 Mar 2019 13:52
Operator : JU/SJ
Sample : PB118273BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118273BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.47 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.47	80.09 ng	4272800	1,4-Dichlorobenzene-d4	6.70

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3		Amphetaminil	250	C17H18N2	017590-01-1	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12

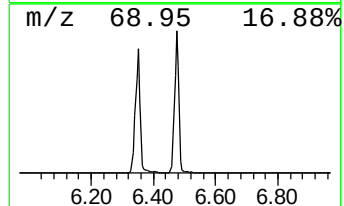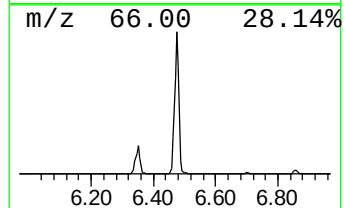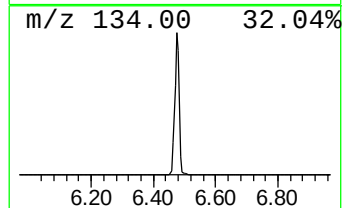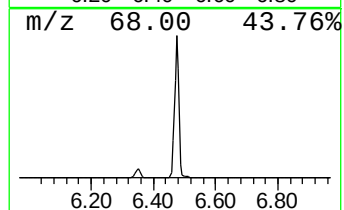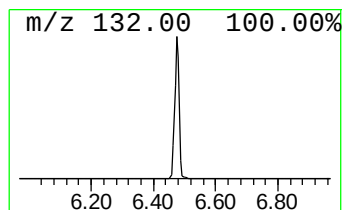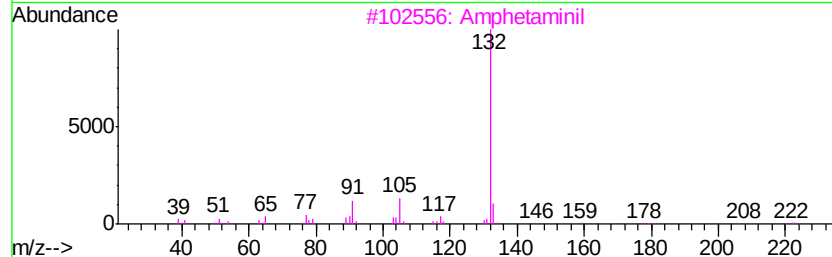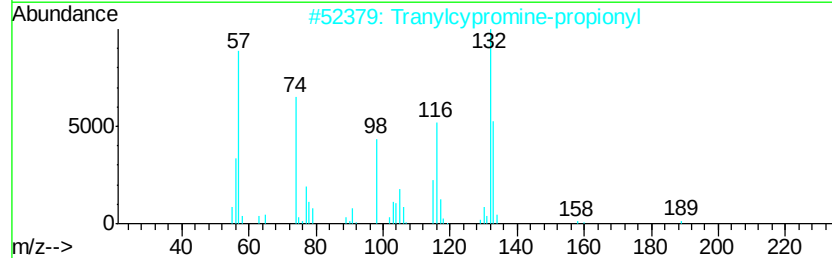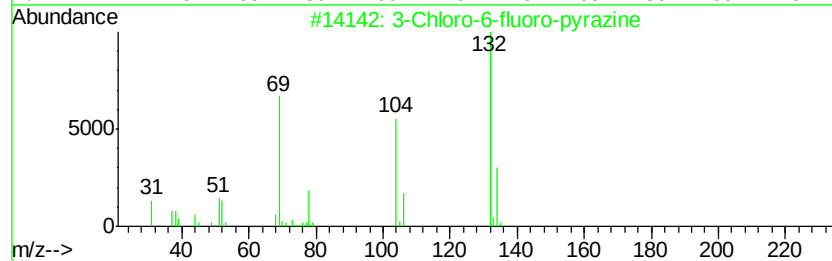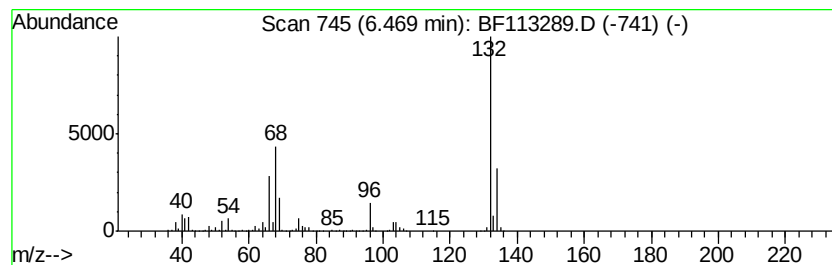

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032619\
Data File : BF113289.D
Acq On : 26 Mar 2019 13:52
Operator : JU/SJ
Sample : PB118273BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118273BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.47	6.47	80.1	ng	4272800	1	6.70	1067010	20.0