


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032619\
 Data File : BF113286.D
 Acq On : 26 Mar 2019 12:18
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 26 03:32:08 2019

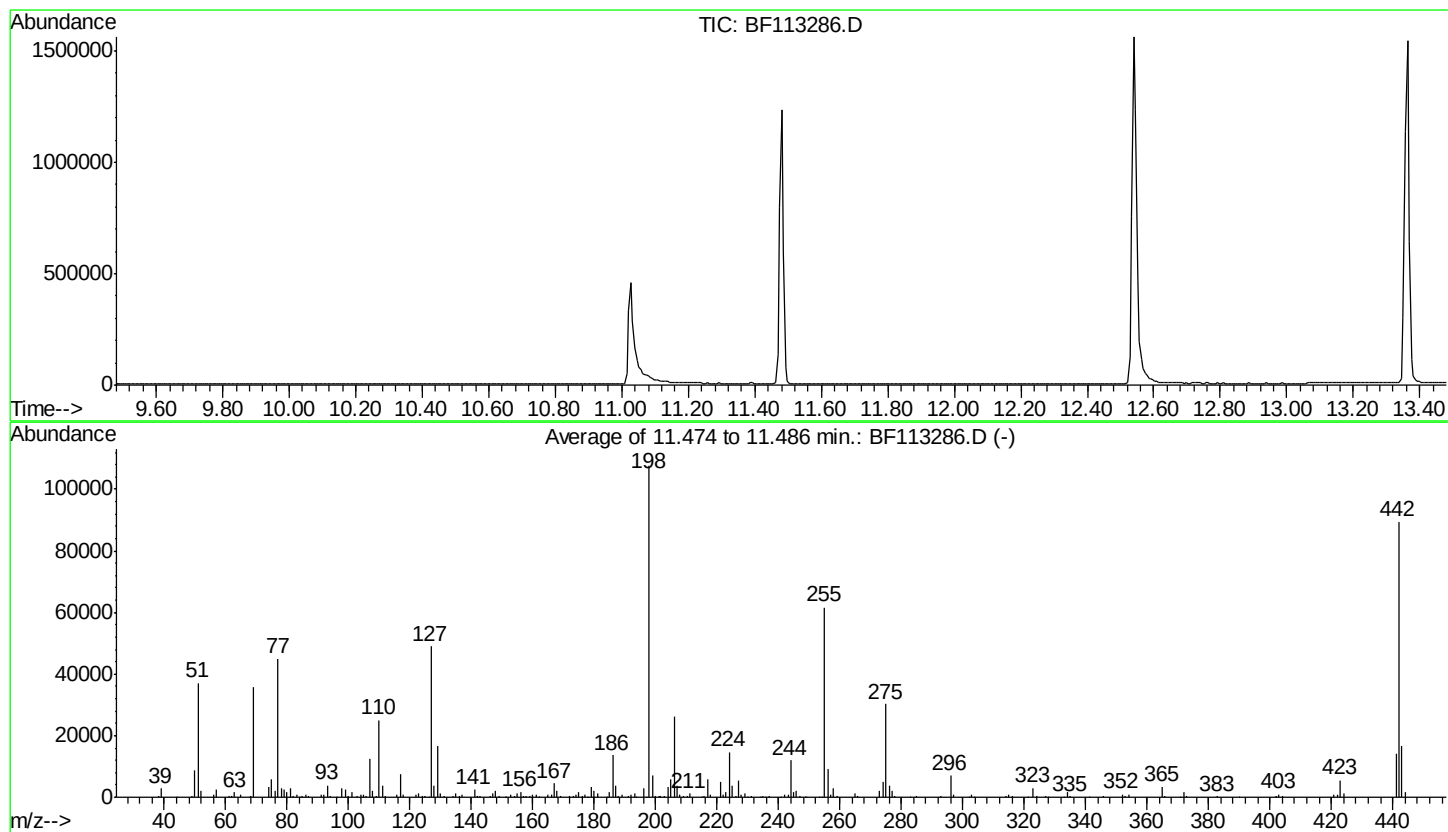

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	37074	PASS
68	69	0.00	2	1.1	397	PASS
69	198	0.00	100	33.2	35724	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.4	48936	PASS
197	198	0.00	2	0.1	149	PASS
198	198	100	100	100.0	107685	PASS
199	198	5	9	6.6	7107	PASS
275	198	10	60	28.0	30194	PASS
365	198	1	100	3.2	3396	PASS
441	198	0.01	100	13.3	14326	PASS
442	198	50	100	83.1	89448	PASS
443	442	15	24	18.8	16817	PASS