


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032619\
 Data File : BF113297.D
 Acq On : 26 Mar 2019 17:54
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 26 03:32:08 2019

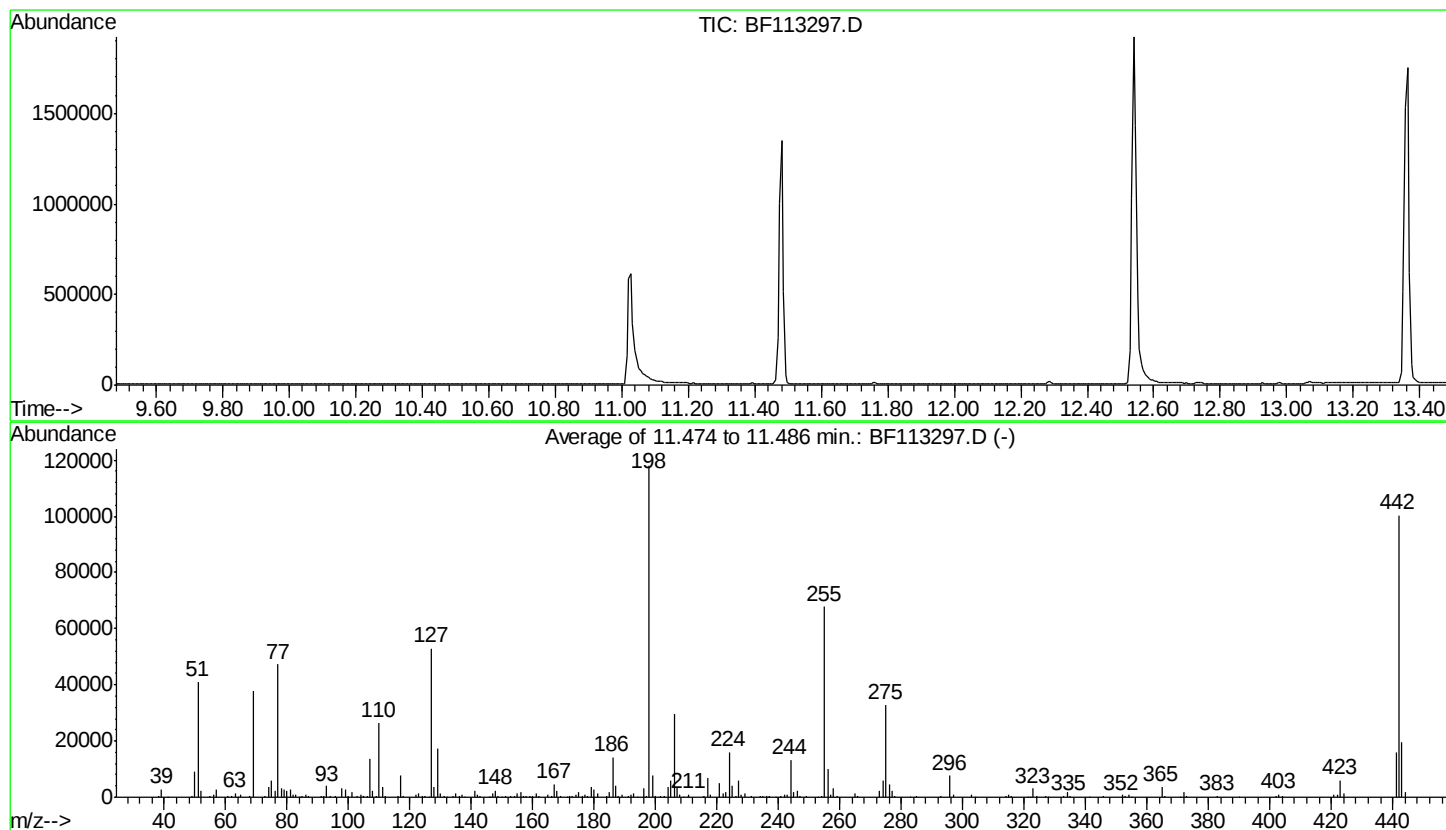

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	41048	PASS
68	69	0.00	2	1.4	530	PASS
69	198	0.00	100	32.1	37861	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.0	53096	PASS
197	198	0.00	2	0.5	615	PASS
198	198	100	100	100.0	118037	PASS
199	198	5	9	6.7	7877	PASS
275	198	10	60	27.9	32954	PASS
365	198	1	100	3.1	3673	PASS
441	198	0.01	100	13.5	15922	PASS
442	198	50	100	85.0	100349	PASS
443	442	15	24	19.3	19409	PASS