

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032620\
 Data File : BF119544.D
 Acq On : 26 Mar 2020 21:59
 Operator : CG/JU
 Sample : L2040-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RO-346

Quant Time: Mar 27 02:02:35 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 26 16:30:13 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	269870	20.00	ng	0.00
21) Naphthalene-d8	8.12	136	1014564	20.00	ng	0.00
39) Acenaphthene-d10	9.87	164	548755	20.00	ng	-0.01
64) Phenanthrene-d10	11.36	188	1104143	20.00	ng	0.00
76) Chrysene-d12	14.01	240	880148	20.00	ng	0.00
87) Perylene-d12	15.47	264	831762	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	2010057	118.57	ng	0.02
7) Phenol-d6	6.46	99	2233846	103.15	ng	0.00
23) Nitrobenzene-d5	7.40	82	1847240	98.95	ng	0.00
42) 2,4,6-Tribromophenol	10.67	330	939555	165.96	ng	0.00
45) 2-Fluorobiphenyl	9.20	172	3429991	92.60	ng	0.00
79) Terphenyl-d14	12.96	244	4228701	94.13	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.59	163	169688	4.353	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032620\
Data File : BF119544.D
Acq On : 26 Mar 2020 21:59
Operator : CG/JU
Sample : L2040-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RO-346

Quant Time: Mar 27 02:02:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 26 16:30:13 2020
Response via : Initial Calibration

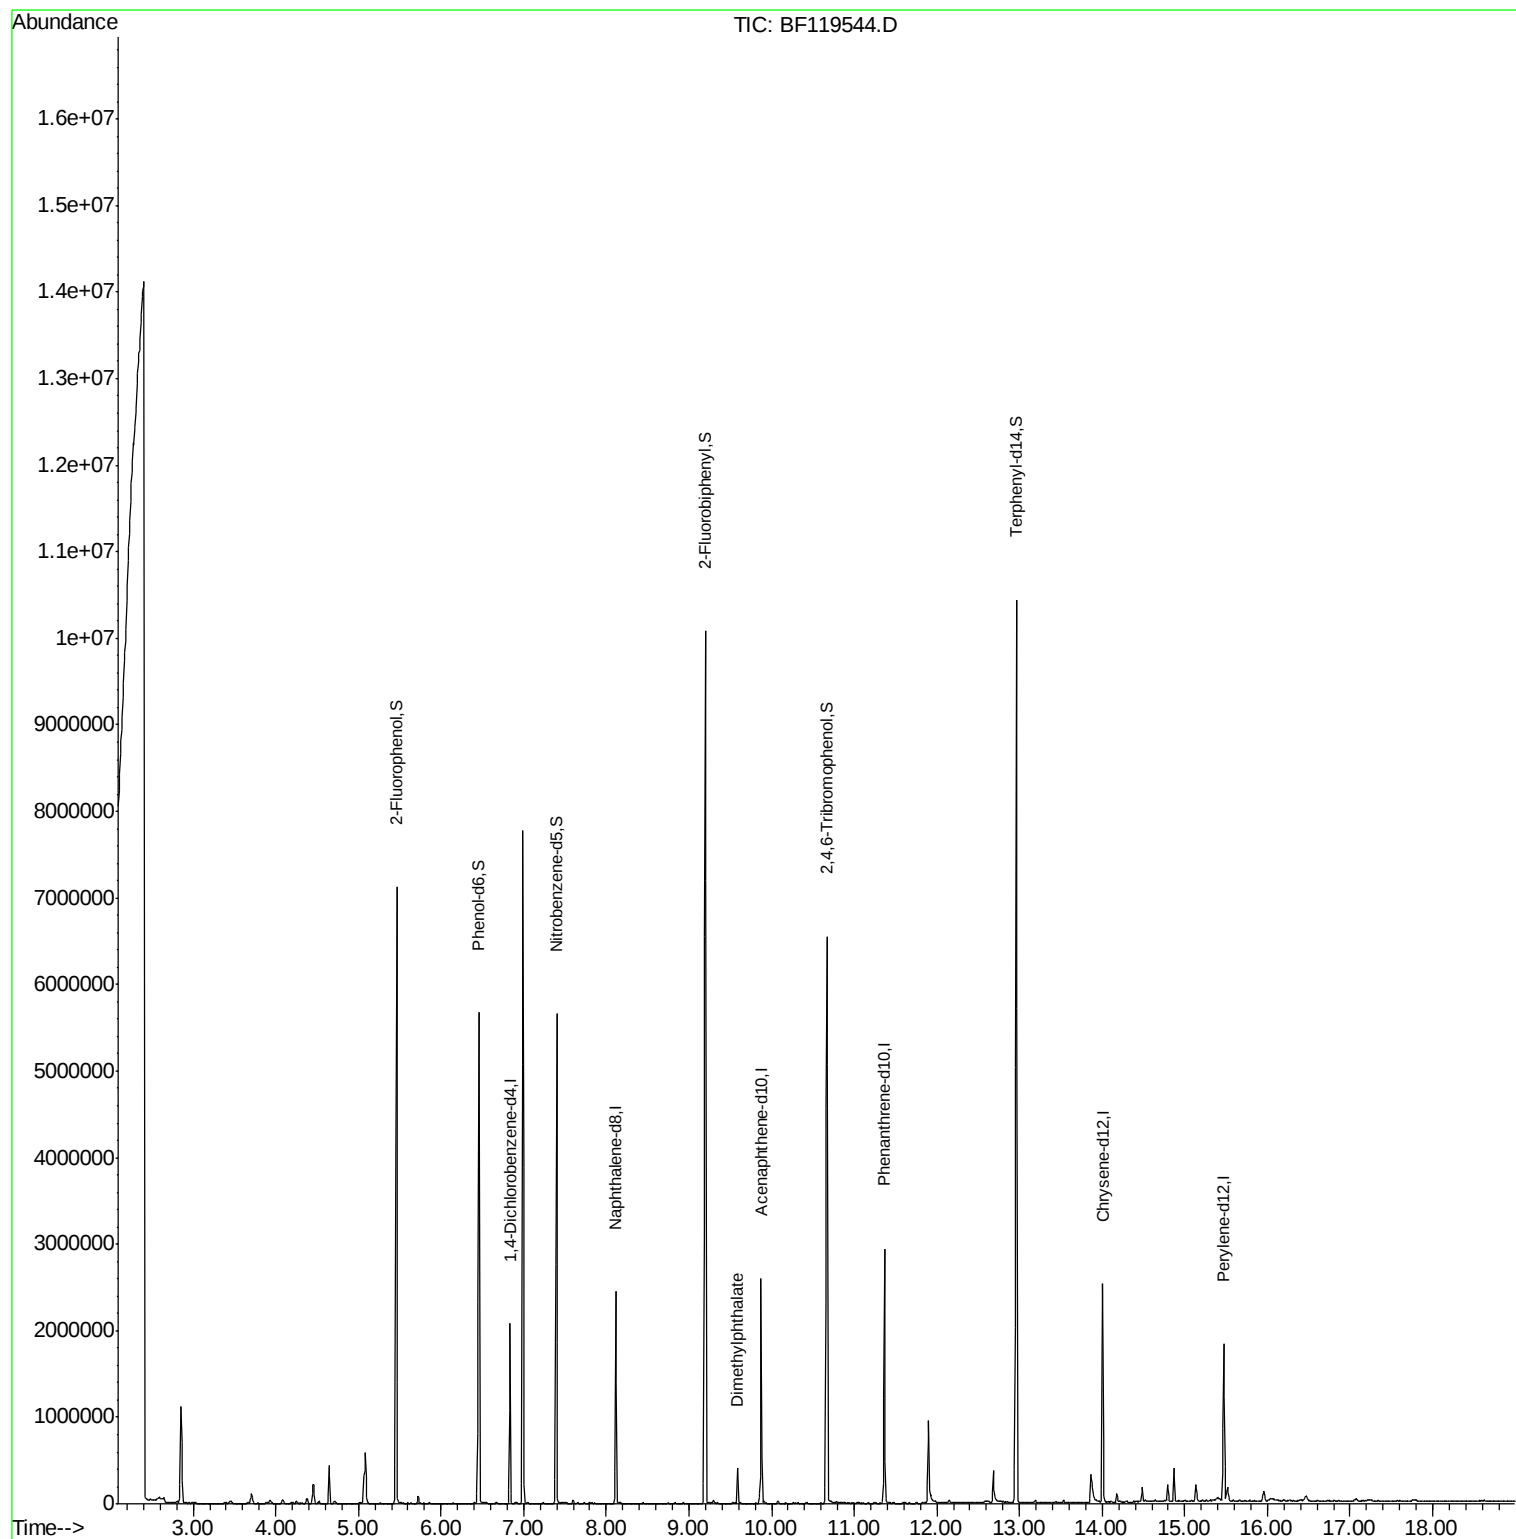




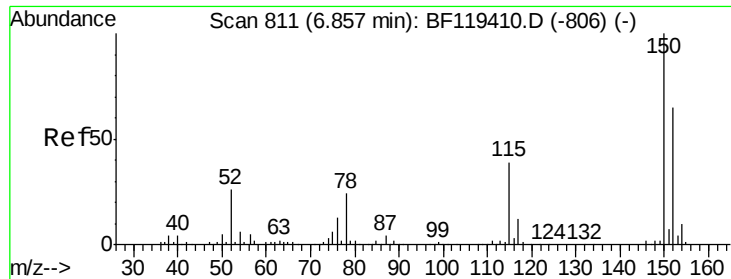


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.83 min Scan# 807
Delta R.T. -0.00 min
Lab File: BF119544.D
Acq: 26 Mar 2020 21:59

Instrument :
BNA_F
ClientSampleId :
RO-346




Tot Ion:152 Resp: 269870
Ion Ratio Lower Upper
152 100
150 154.9 123.9 185.9
115 59.8 47.8 71.6

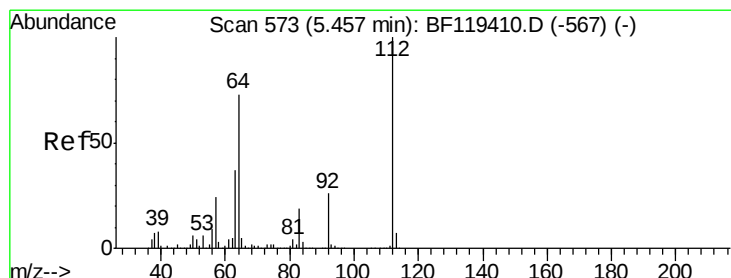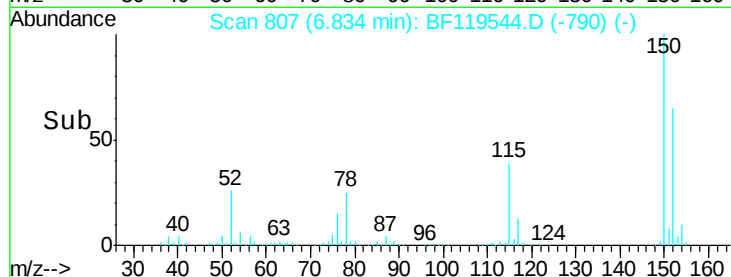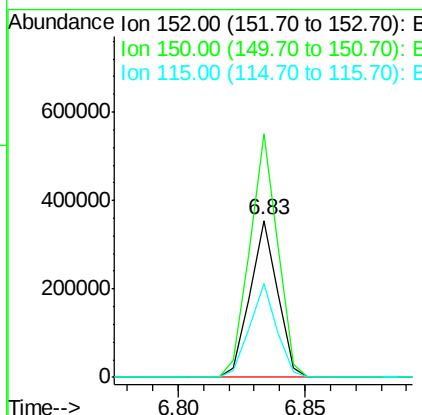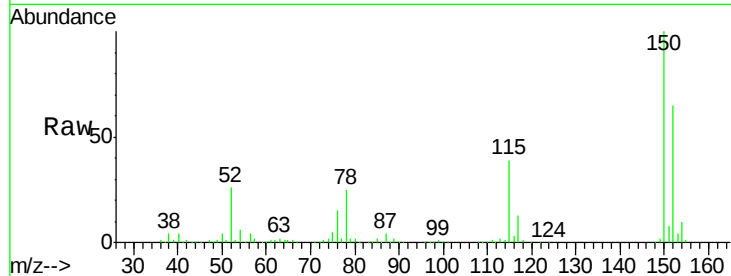


#5

2-Fluorophenol
Concen: 118.569 ng
RT: 5.46 min Scan# 574
Delta R.T. 0.02 min
Lab File: BF119544.D
Acq: 26 Mar 2020 21:59

Tgt Ion:112 Resp: 2010057
Ion Ratio Lower Upper
112 100
64 69.1 58.1 87.1
63 36.3 29.7 44.5

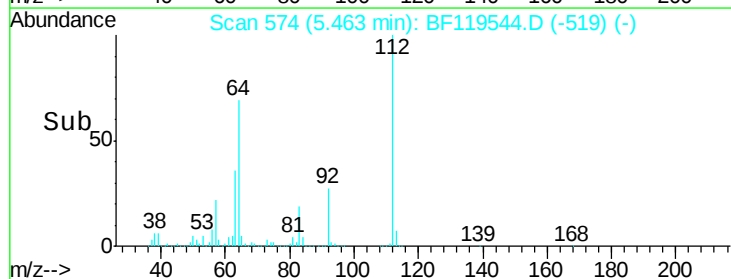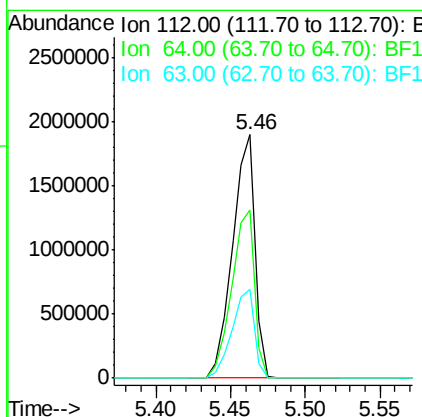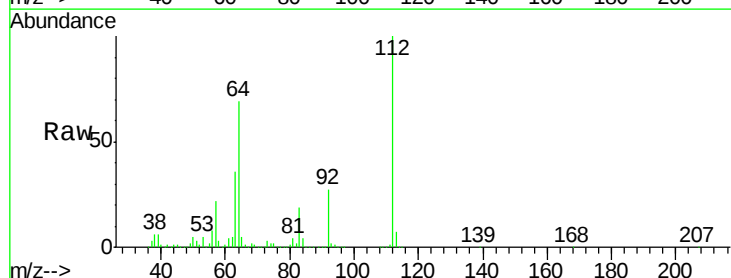

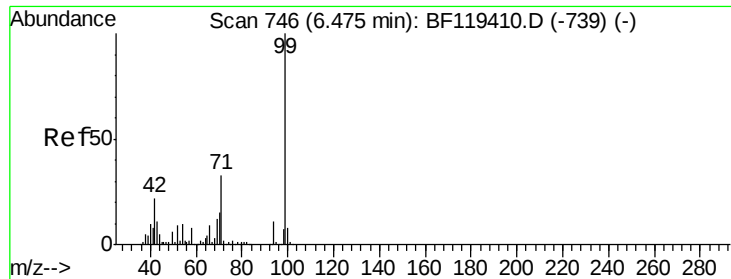

#7

Phenol-d6

Concen: 103.152 ng

RT: 6.46 min Scan# 743

Delta R.T. -0.01 min

Lab File: BF119544.D

Acq: 26 Mar 2020 21:59

Instrument :

BNA_F

ClientSampleId :

RO-346





Tot Ion: 99 Resp: 2233846

Ion Ratio Lower Upper

99 100

42 20.8 17.8 26.6

71 33.8 26.0 39.0

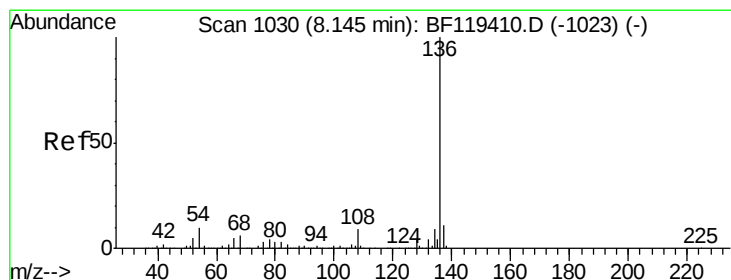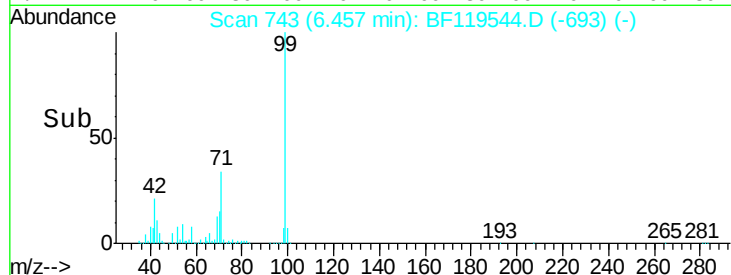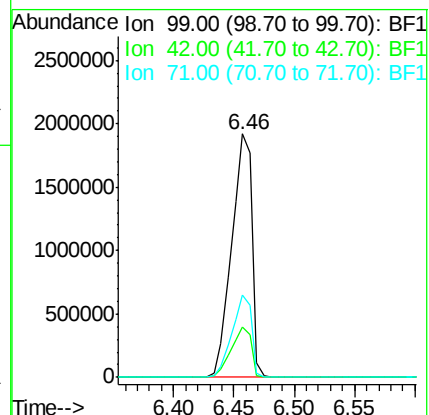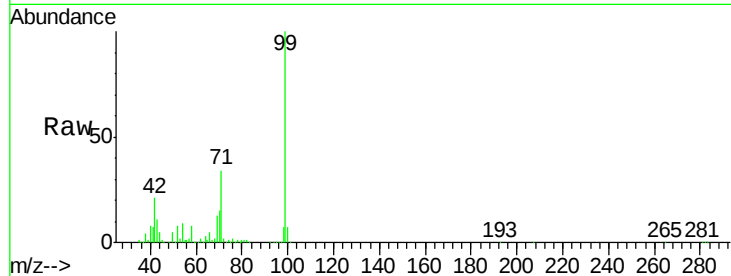

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.12 min Scan# 1025

Delta R.T. -0.01 min

Lab File: BF119544.D

Acq: 26 Mar 2020 21:59

Tgt Ion: 136 Resp: 1014564




Ion Ratio Lower Upper


136 100

137 11.0 8.4 12.6

54 10.8 8.3 12.5

68 5.9 4.9 7.3

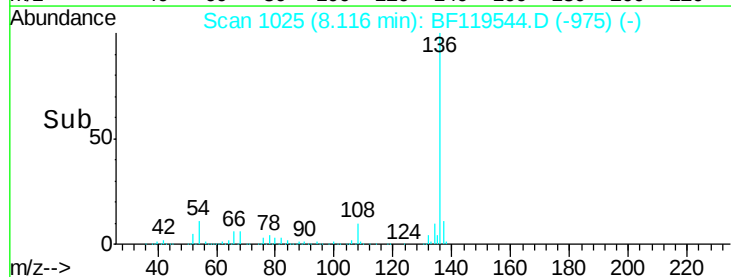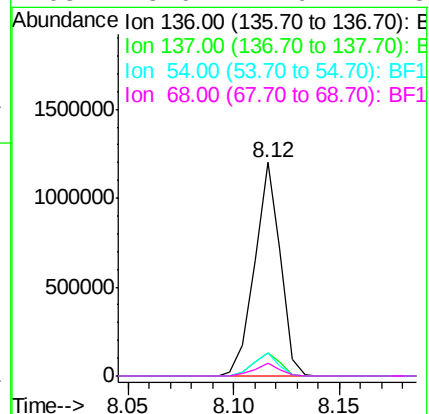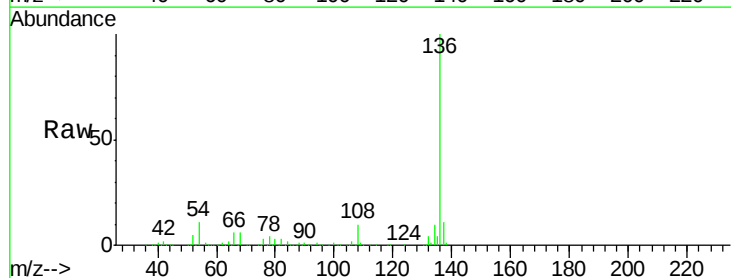


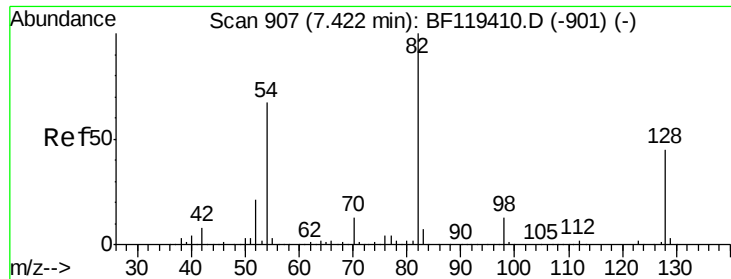




#23
Nitrobenzene-d5
Concen: 98.952 ng
RT: 7.40 min Scan# 903
Delta R.T. -0.01 min
Lab File: BF119544.D
Acq: 26 Mar 2020 21:59

Instrument :
BNA_F
ClientSampled :
RO-346

Tot Ion: 82 Resp: 1847240
Ion Ratio Lower Upper
82 100
128 45.7 35.8 53.8
54 63.7 53.4 80.0

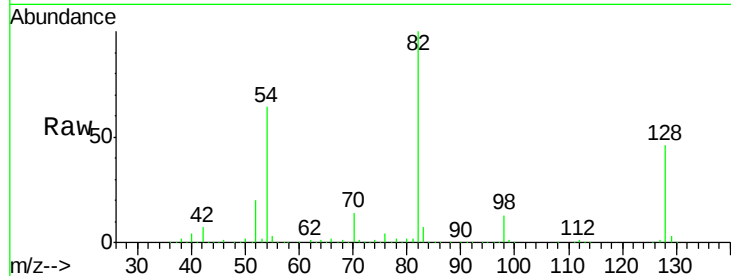


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

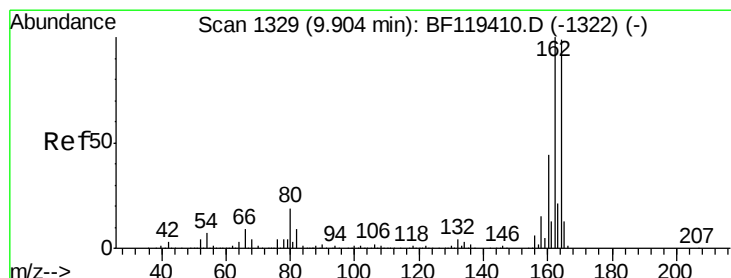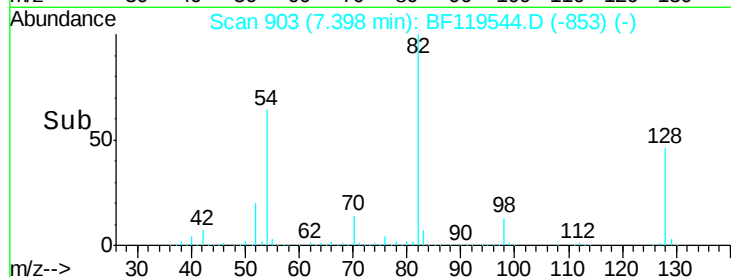
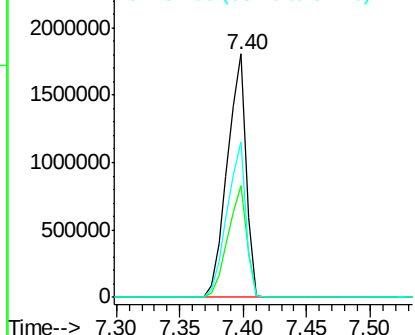



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.87 min Scan# 1324
Delta R.T. -0.01 min
Lab File: BF119544.D
Acq: 26 Mar 2020 21:59

Tgt Ion:164 Resp: 548755
Ion Ratio Lower Upper
164 100
162 103.3 80.7 121.1
160 46.3 35.5 53.3

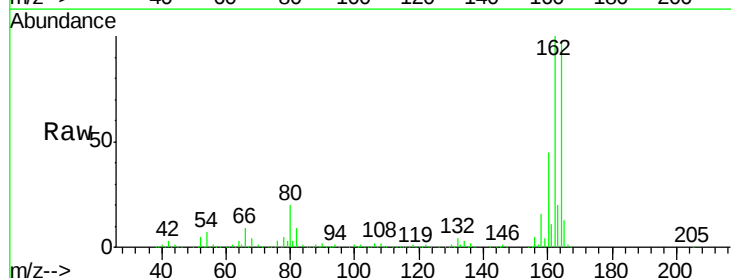

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

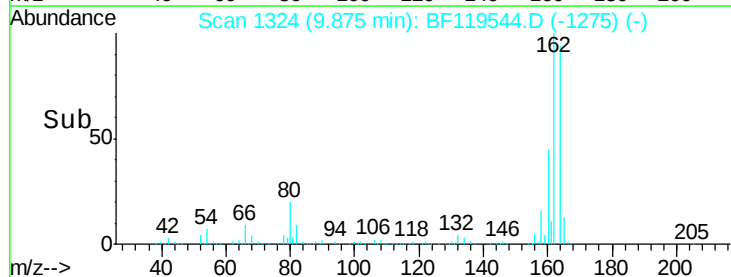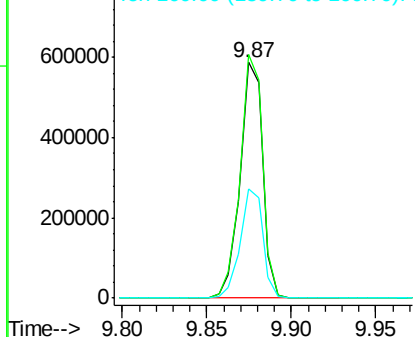


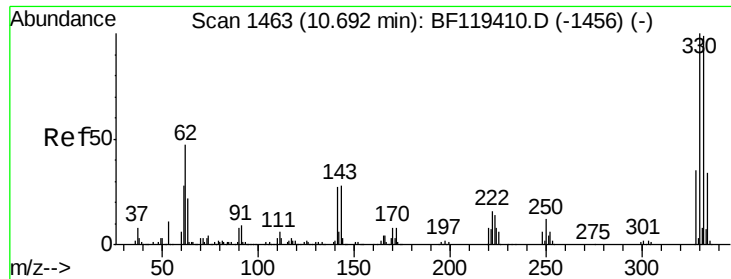




#42
 2,4,6-Tribromophenol
 Concen: 165.961 ng
 RT: 10.67 min Scan# 1460
 Delta R.T. -0.00 min
 Lab File: BF119544.D
 Acq: 26 Mar 2020 21:59

Instrument :
 BNA_F
 ClientSampleId :
 RO-346

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.0	77.6	116.4
141	31.2	26.6	40.0

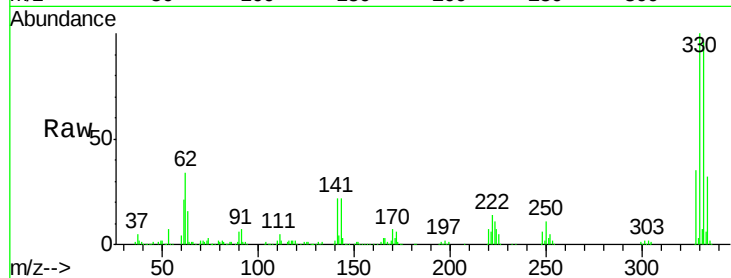


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

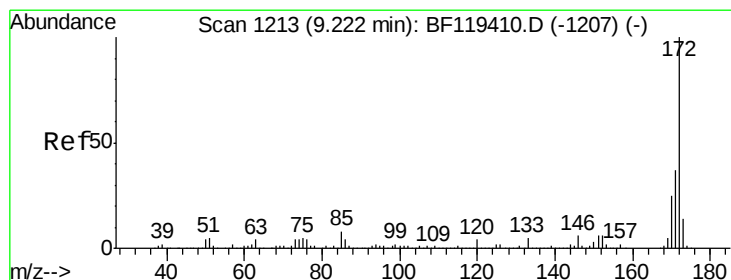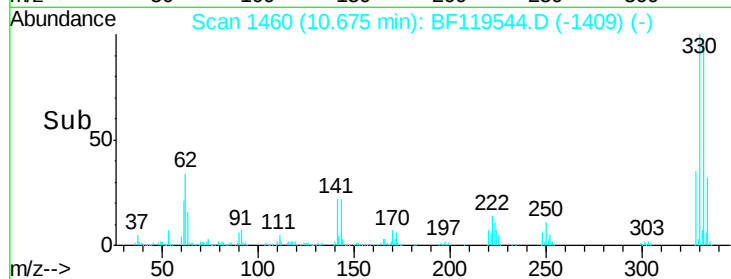
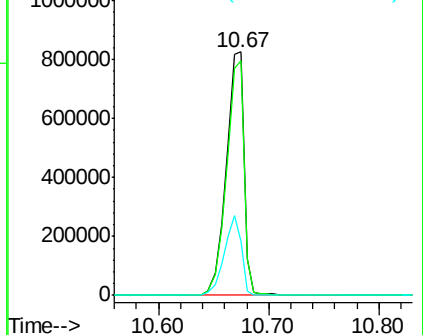



#45
 2-Fluorobiphenyl
 Concen: 92.599 ng
 RT: 9.20 min Scan# 1209
 Delta R.T. -0.01 min
 Lab File: BF119544.D
 Acq: 26 Mar 2020 21:59

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.0	29.9	44.9
170	25.1	20.1	30.1

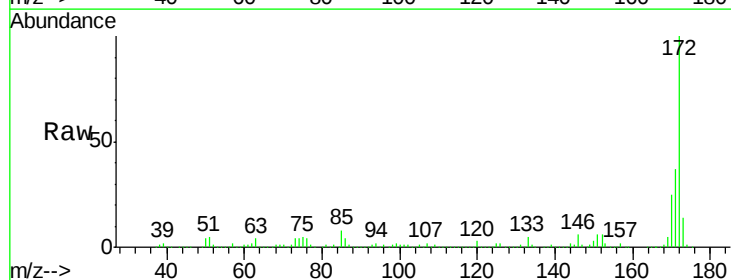

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

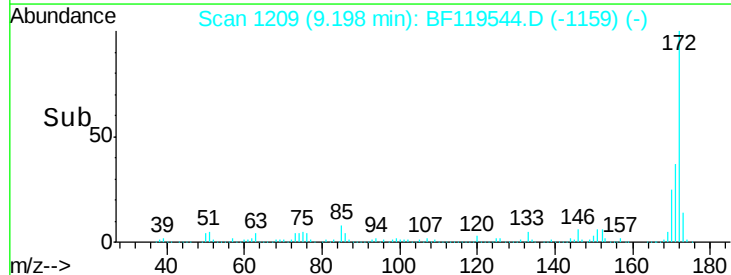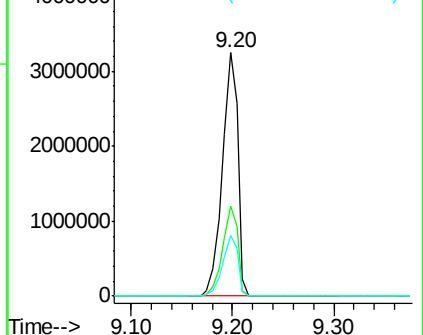

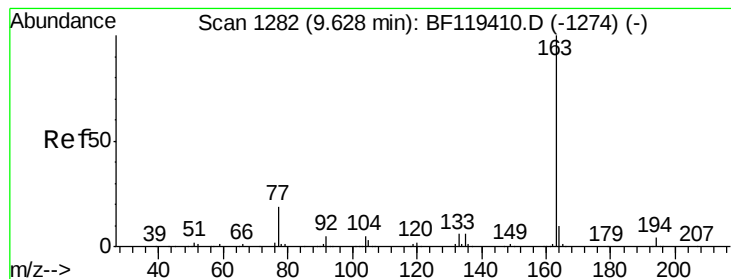

#50

Dimethylphthalate

Concen: 4.353 ng

RT: 9.59 min Scan# 1276

Delta R.T. -0.02 min

Lab File: BF119544.D

Acq: 26 Mar 2020 21:59

Instrument :

BNA_F

ClientSampleId :

RO-346


Tot Ion:163 Resp: 169688

Ion Ratio Lower Upper

163 100

194 4.4 3.2 4.8




164 9.6 8.1 12.1

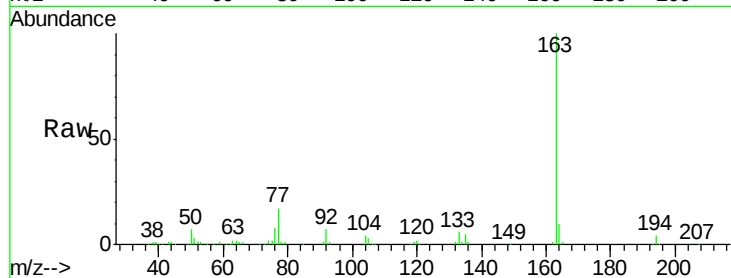

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

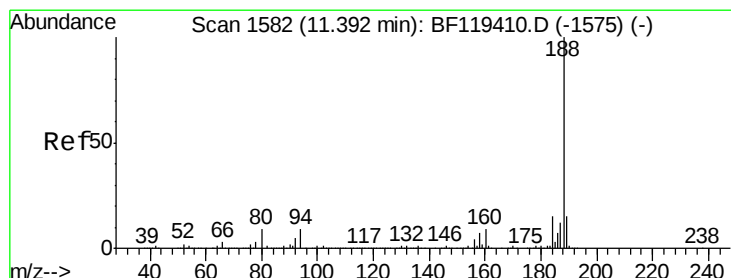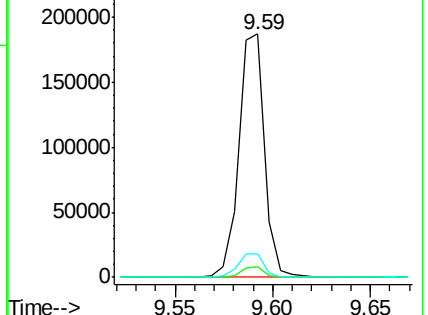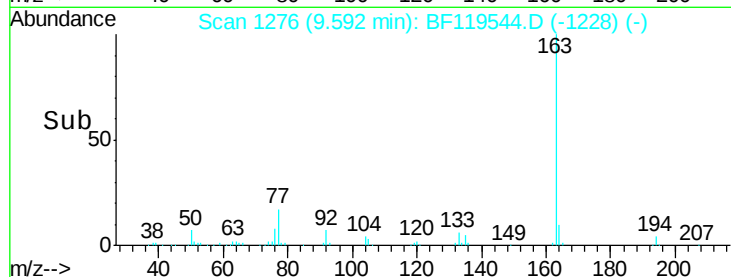

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.36 min Scan# 1577

Delta R.T. -0.01 min

Lab File: BF119544.D

Acq: 26 Mar 2020 21:59


Tgt Ion:188 Resp: 1104143

Ion Ratio Lower Upper

188 100

94 10.0 7.1 10.7



80 11.0 7.5 11.3

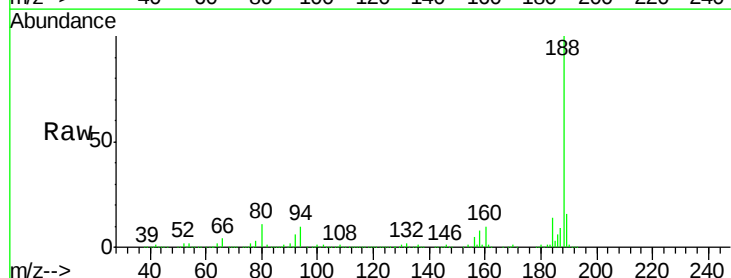


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1



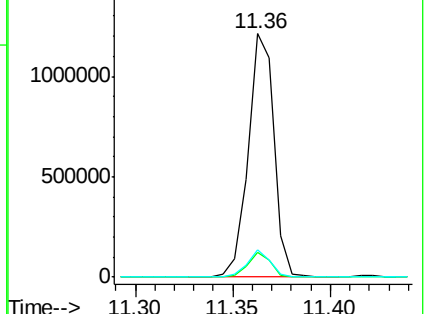
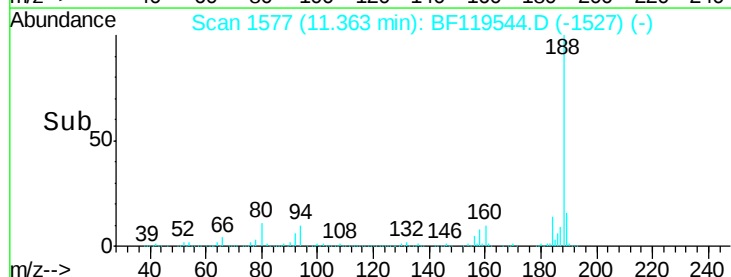


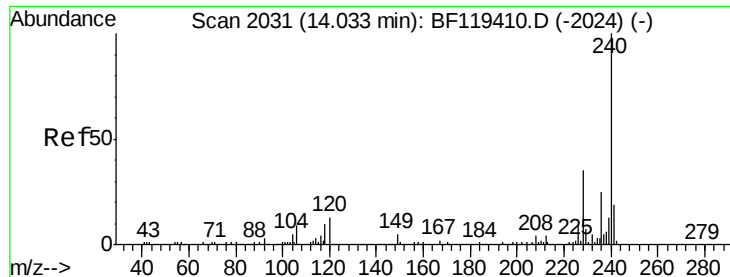

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.01 min Scan# 2027
Delta R.T. -0.01 min
Lab File: BF119544.D
Acq: 26 Mar 2020 21:59




Instrument :
BNA_F
ClientSampleId :
RO-346




Tot Ion:240 Resp: 880148
Ion Ratio Lower Upper
240 100
120 10.7 10.2 15.4
236 25.9 20.4 30.6

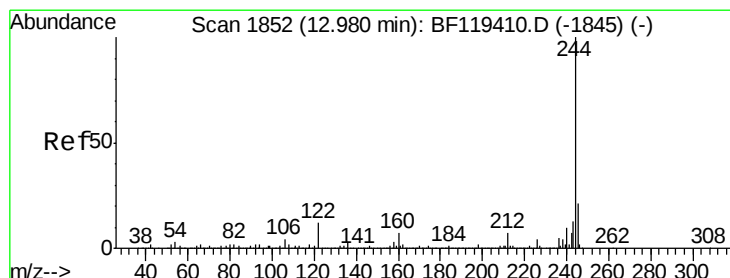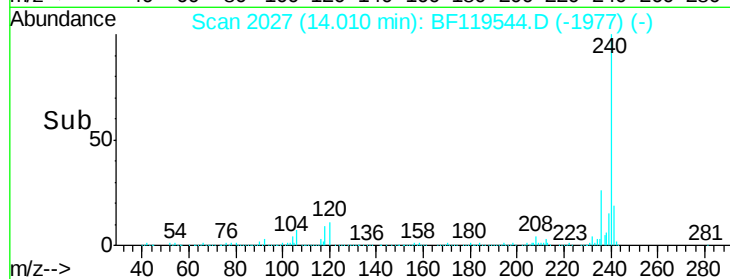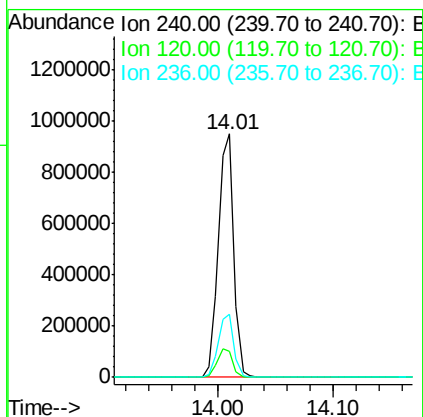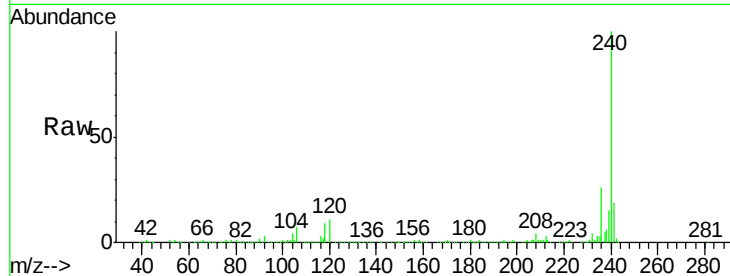

#79
Terphenyl-d14
Concen: 94.131 ng
RT: 12.96 min Scan# 1849
Delta R.T. -0.00 min
Lab File: BF119544.D
Acq: 26 Mar 2020 21:59

Tgt Ion:244 Resp: 4228701
Ion Ratio Lower Upper
244 100
212 7.2 5.7 8.5
122 13.4 9.8 14.8

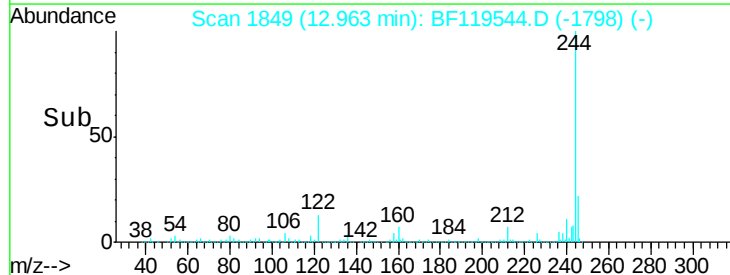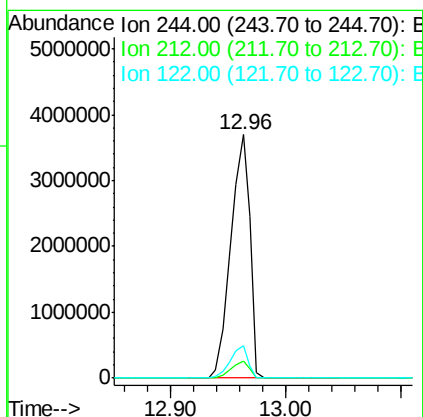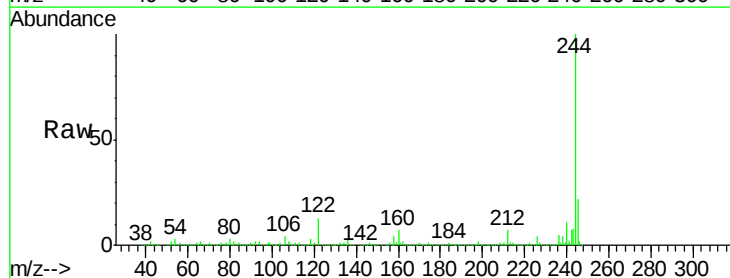

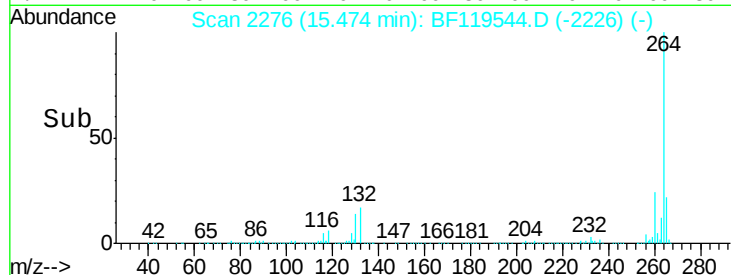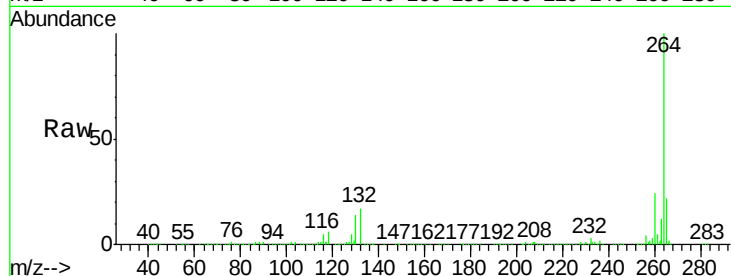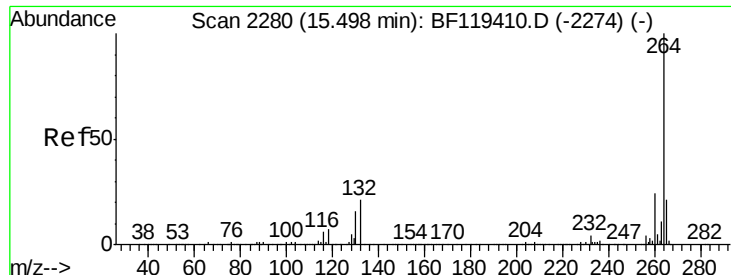

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.47 min Scan# 2276
Delta R.T. -0.01 min
Lab File: BF119544.D
Acq: 26 Mar 2020 21:59

Instrument :
BNA_F
ClientSampleId :
RO-346

Tot Ion:	264	Resp:	831762
Ion	Ratio	Lower	Upper
264	100		
260	24.4	19.2	28.8
265	21.9	16.9	25.3

