

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032620\
 Data File : BF119535.D
 Acq On : 26 Mar 2020 17:56
 Operator : CG/JU
 Sample : PB127833BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB127833BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	499	505	512	rBV	82903	103978	1.37%	0.201%
2	5.451	567	572	575	rBV	6118411	5731803	75.53%	11.053%
3	6.457	737	743	746	rBV	5470173	5613414	73.97%	10.824%
4	6.834	803	807	810	rBV	1986779	1534199	20.22%	2.958%
5	6.992	829	834	837	rBV	5242916	4561983	60.12%	8.797%
6	7.392	897	902	905	rBV	3703413	3746370	49.37%	7.224%
7	8.116	1020	1025	1029	rBV	2166410	1988972	26.21%	3.835%
8	9.198	1203	1209	1212	rBV	7161035	6805719	89.68%	13.123%
9	9.875	1319	1324	1328	rBV	2377859	2333211	30.75%	4.499%
10	10.669	1453	1459	1462	rBV	4882399	4544203	59.88%	8.763%
11	11.369	1572	1578	1581	rBV	2748108	2542950	33.51%	4.904%
12	12.957	1843	1848	1852	rBV	7271537	7588488	100.00%	14.633%
13	14.010	2023	2027	2031	rBV	2660463	2398962	31.61%	4.626%
14	15.480	2271	2277	2282	rBV	1852954	2364777	31.16%	4.560%




Sum of corrected areas: 51859029

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032620\
Data File : BF119535.D
Acq On : 26 Mar 2020 17:56
Operator : CG/JU
Sample : PB127833BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB127833BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

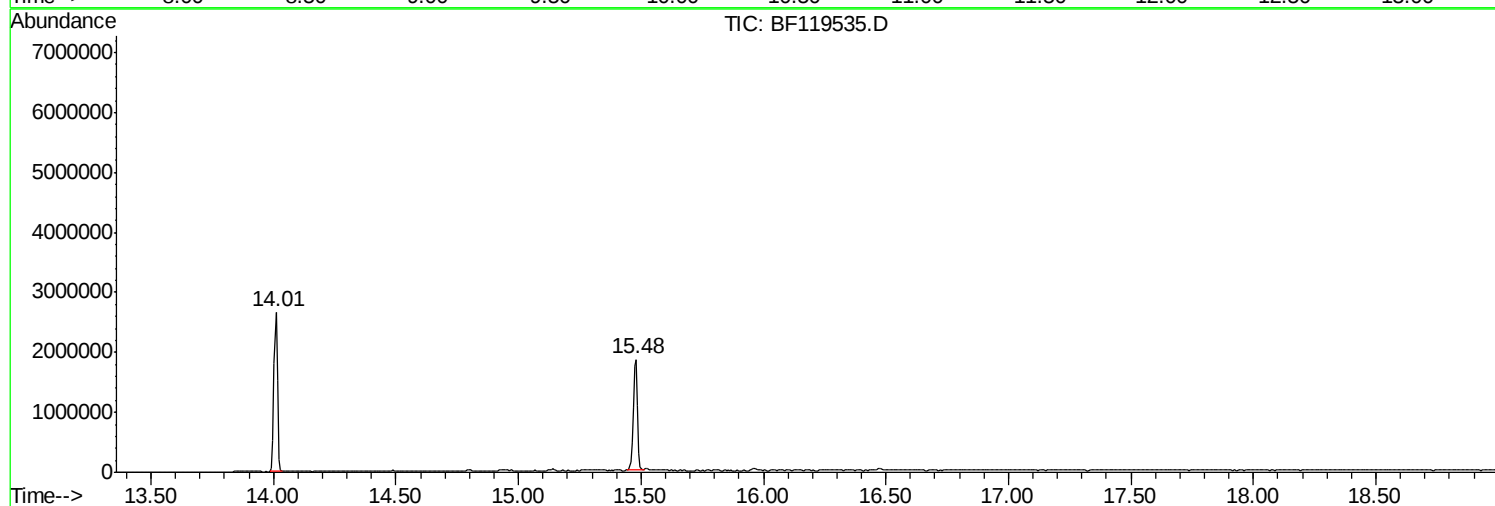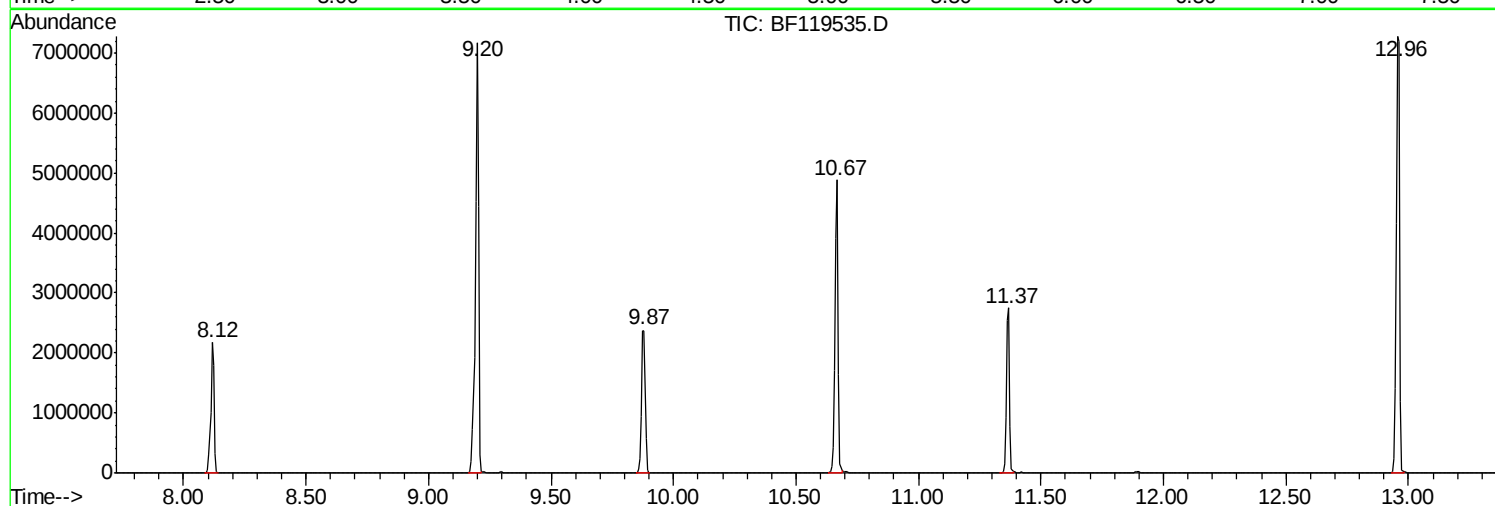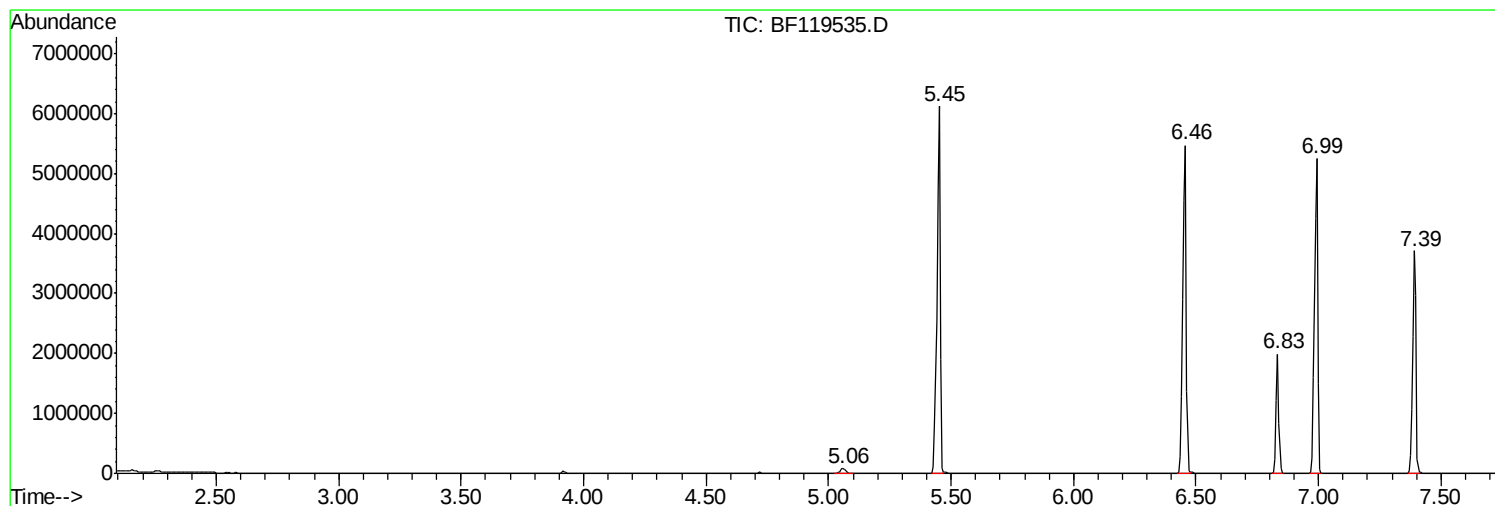

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032620\
Data File : BF119535.D
Acq On : 26 Mar 2020 17:56
Operator : CG/JU
Sample : PB127833BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB127833BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032620\
Data File : BF119535.D
Acq On : 26 Mar 2020 17:56
Operator : CG/JU
Sample : PB127833BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB127833BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc