


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032620\
 Data File : BF119551.D
 Acq On : 27 Mar 2020 4:36
 Operator : CG/JU
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTTP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 27 07:52:09 2020

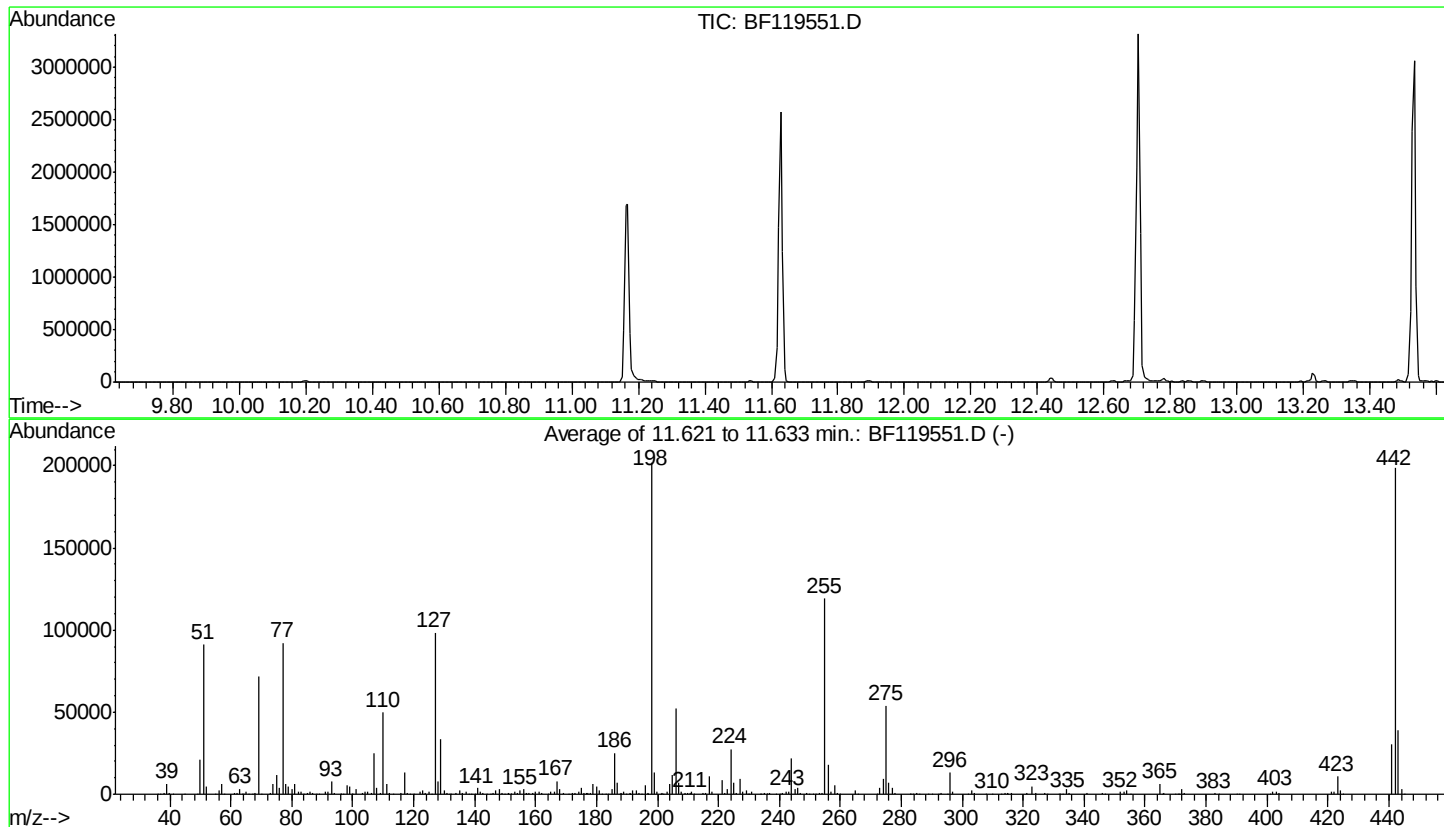

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	91010	PASS
68	69	0.00	2	1.7	1196	PASS
69	198	0.00	100	35.5	71602	PASS
70	69	0.00	2	0.4	304	PASS
127	198	10	80	48.7	98434	PASS
197	198	0.00	2	0.5	1013	PASS
198	198	100	100	100.0	201941	PASS
199	198	5	9	6.6	13390	PASS
275	198	10	60	26.7	53824	PASS
365	198	1	100	3.2	6545	PASS
441	198	0.01	100	15.1	30450	PASS
442	198	50	100	98.5	198898	PASS
443	442	15	24	19.7	39208	PASS