
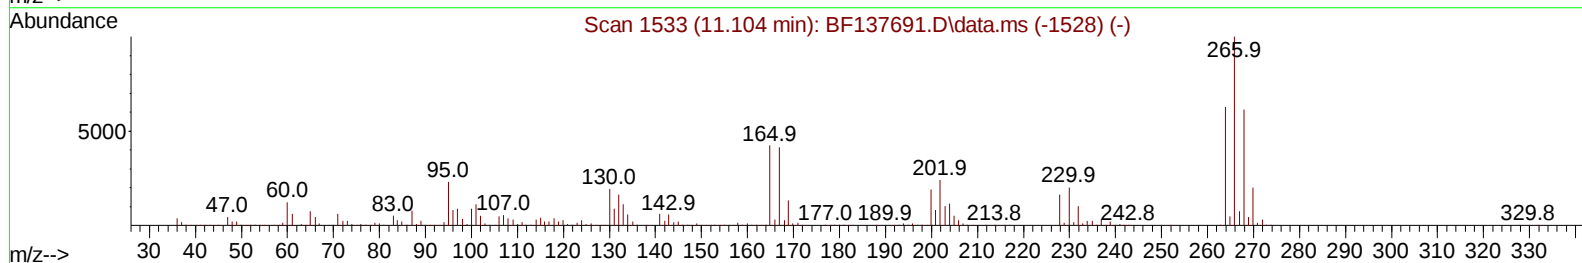
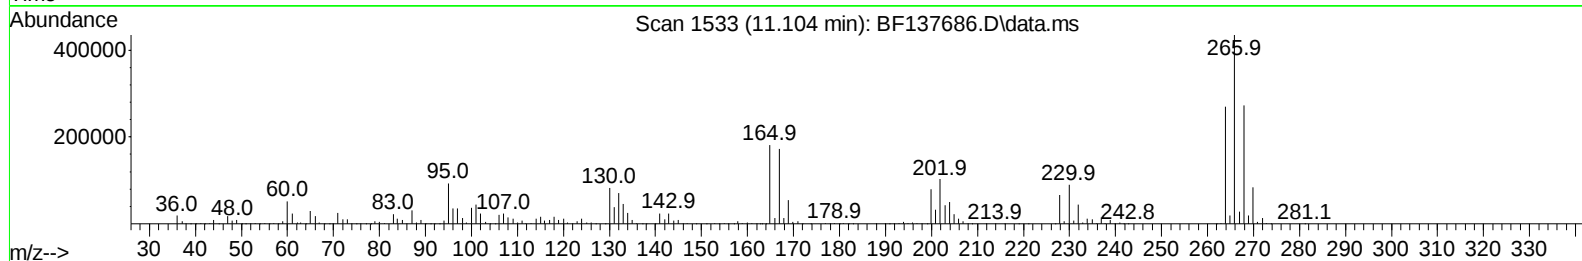


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032624\
Data File : BF137686.D
Acq On : 26 Mar 2024 14:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 02:04:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 01:52:09 2024
Response via : Initial Calibration

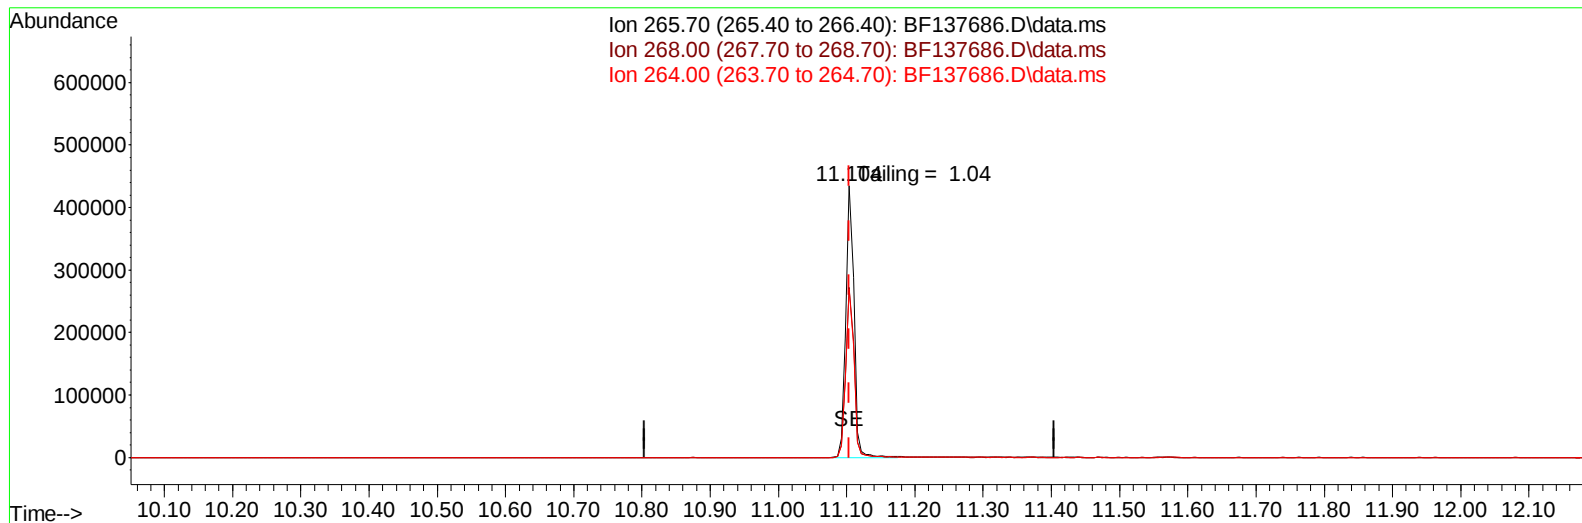

TIC: BF137686.D\data.ms

(70) Pentachlorophenol (C)




11.104min (-0.000) 345367.38 ng

response 360499

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.30	62.61
264.00	62.70	62.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032624\
Data File : BF137686.D
Acq On : 26 Mar 2024 14:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 02:04:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 01:52:09 2024
Response via : Initial Calibration

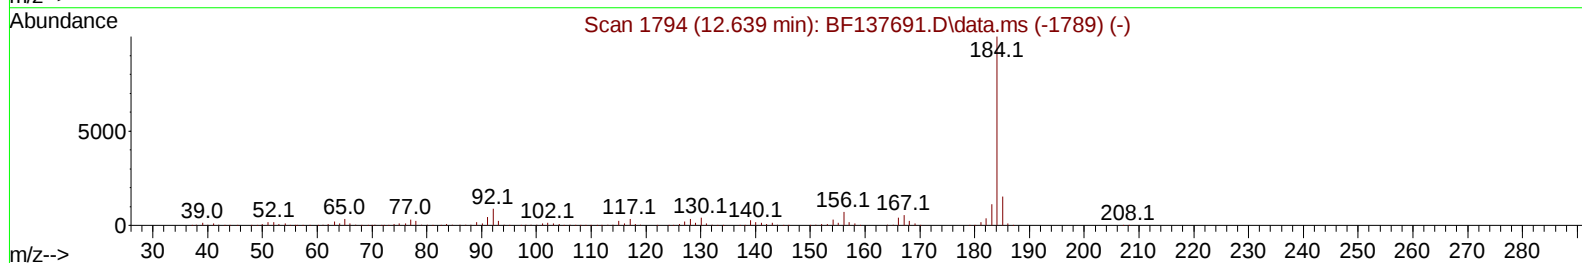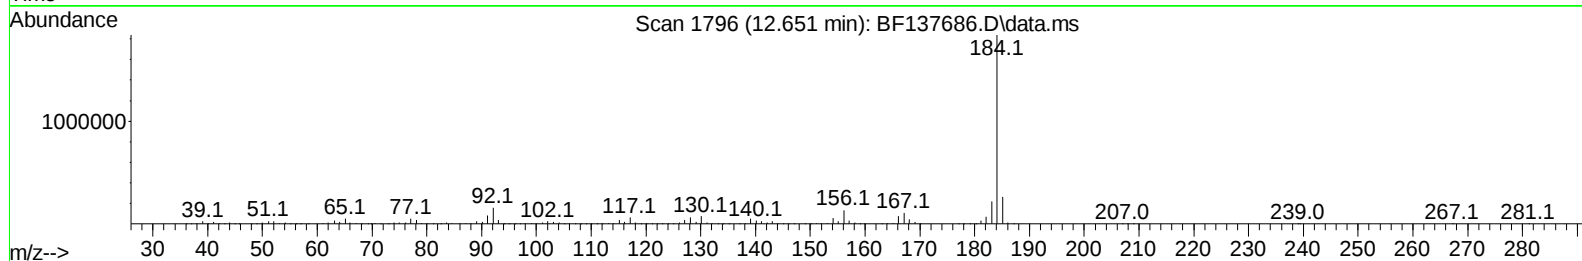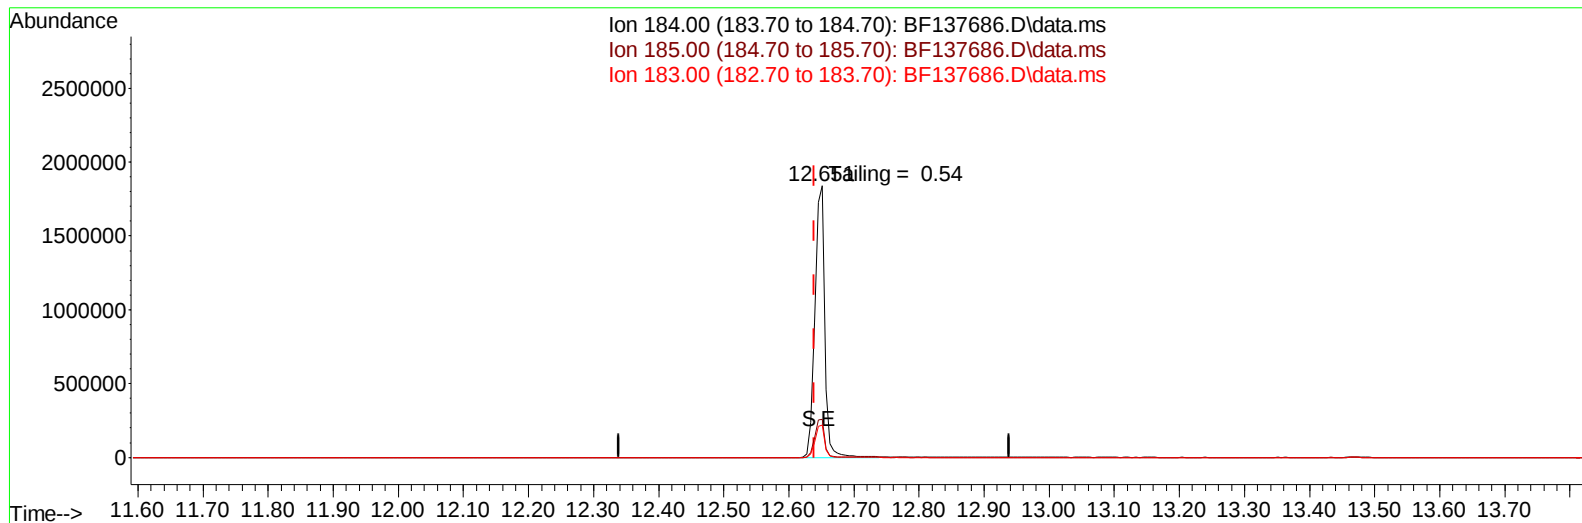

TIC: BF137686.D\data.ms

(77) Benzidine**12.651min (+ 0.012) 9594.38 ng m****response 1943475**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.11
183.00	11.30	11.95
0.00	0.00	0.00